

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
 Data File : BM010367.D
 Acq On : 01 Jun 2017 22:11
 Operator : SJ/MA
 Sample : I3163-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSG4

Quant Time: Jun 02 03:23:10 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 02 01:55:54 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	370189	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	1321814	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	801536	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	1872689	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	2774337	20.00	ng/ul	0.00
83) Perylene-d12	23.81	264	2816641	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.38	96	24197	2.68	ng/uL	0.00
5) Phenol-d5	7.10	99	502354	17.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	292382	18.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	428370	19.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.64	113	396660	17.53	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	199887	20.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	248906	22.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	475881	20.65	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	13.97	166	1553328	23.32	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	1741935	22.42	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	131996	13.25	ng/ul	0.00
57) Fluorene-d10	15.54	176	1321325	22.57	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	243509	18.36	ng/ul	0.00
70) Anthracene-d10	17.40	188	1999679	21.94	ng/ul	0.00
76) Pyrene-d10	19.69	212	2676940	23.33	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.66	264	2915705	22.23	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	14.02	163	252253	3.852	ng/ul	98
81) Bis(2-ethylhexyl)phthalate	21.33	149	145341	1.977	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
Data File : BM010367.D
Acq On : 01 Jun 2017 22:11
Operator : SJ/MA
Sample : I3163-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSG4

Quant Time: Jun 02 03:23:10 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 02 01:55:54 2017
Response via : Initial Calibration




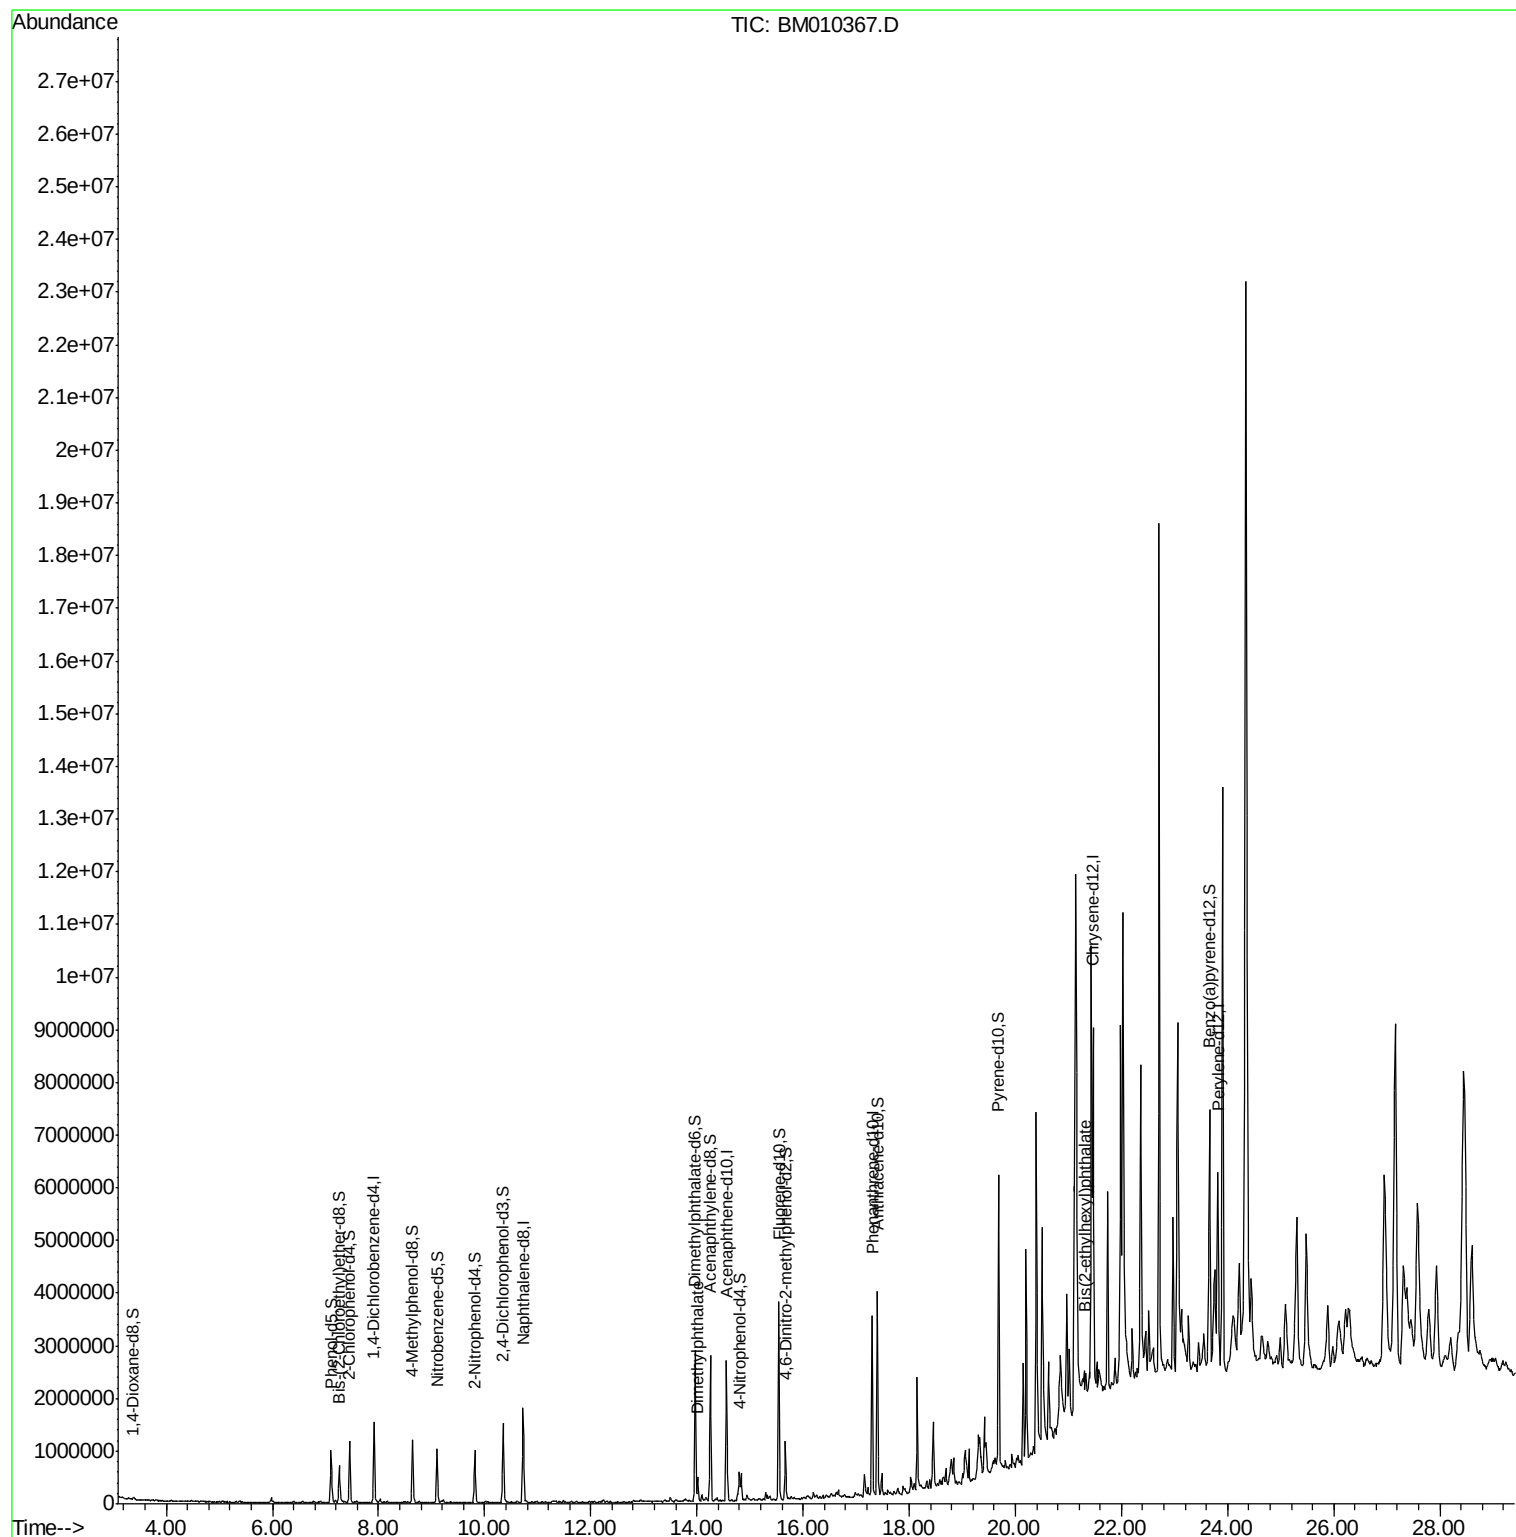


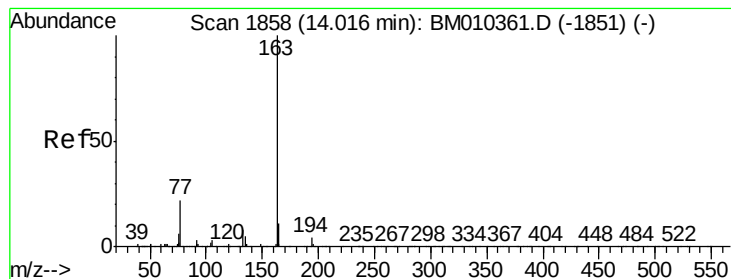

#44
Dimethylphthalate
Concen: 3.852 ng/ul
RT: 14.02 min Scan# 1858
Delta R.T. -0.00 min
Lab File: BM010367.D
Acq: 01 Jun 2017 22:11

Instrument :
BNA_M
ClientSampleId :
JHSG4

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.5	5.3
164	9.5	8.2	12.4

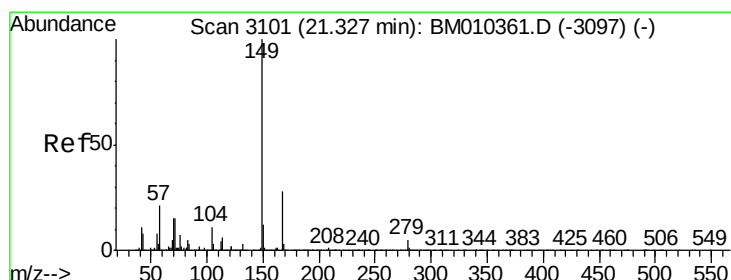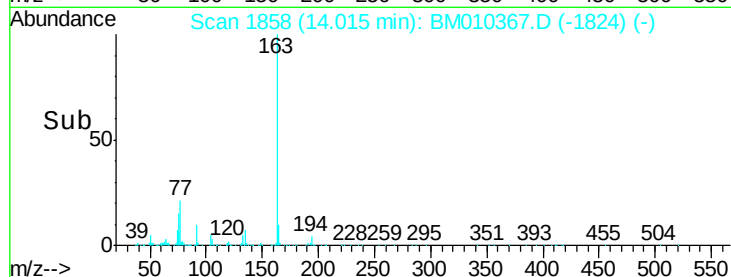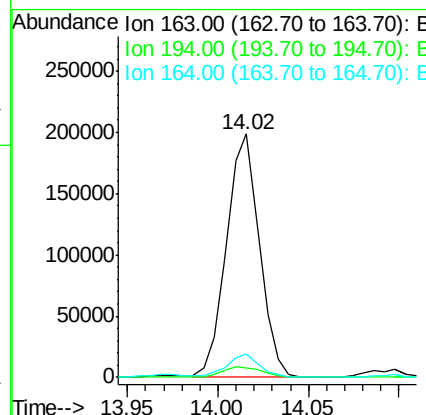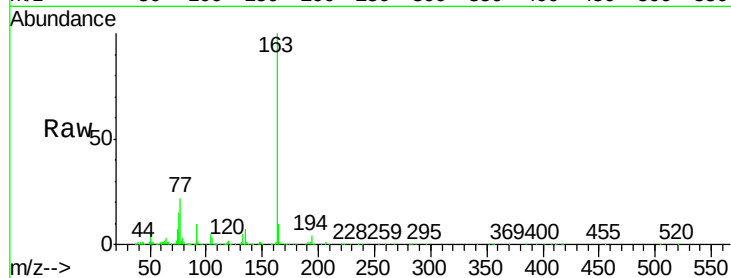

#81
Bis(2-ethylhexyl)phthalate
Concen: 1.977 ng/ul
RT: 21.33 min Scan# 3101
Delta R.T. -0.00 min
Lab File: BM010367.D
Acq: 01 Jun 2017 22:11

Tgt Ion	Ratio	Lower	Upper
149	100		
167	26.7	22.8	34.2
279	4.8	4.9	7.3#

