

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
 Data File : BM010371.D
 Acq On : 02 Jun 2017 00:35
 Operator : SJ/MA
 Sample : I3163-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSG9

Quant Time: Jun 02 01:58:06 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 02 01:55:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	360705	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	1272651	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.55	164	765057	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	1821083	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	2613875	20.00	ng/ul	0.00
83) Perylene-d12	23.81	264	2685038	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.38	96	25294	2.88	ng/uL	0.00
5) Phenol-d5	7.10	99	398026	14.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	238210	15.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	351655	16.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.65	113	321818	14.59	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	162008	17.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	187540	17.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	367951	16.59	ng/ul	0.00
29) 4-Chloroaniline-d4	10.89	131	65184	3.05	ng/ul	0.00
43) Dimethylphthalate-d6	13.97	166	1175942	18.50	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	1325190	17.87	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	92005	9.67	ng/ul	0.00
57) Fluorene-d10	15.55	176	994285	17.79	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	168655	13.07	ng/ul	0.00
70) Anthracene-d10	17.40	188	1517298	17.12	ng/ul	0.00
76) Pyrene-d10	19.69	212	2006056	18.56	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.66	264	2266538	18.13	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	14.02	163	332592	5.320 ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
Data File : BM010371.D
Acq On : 02 Jun 2017 00:35
Operator : SJ/MA
Sample : I3163-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSG9

Quant Time: Jun 02 01:58:06 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 02 01:55:54 2017
Response via : Initial Calibration

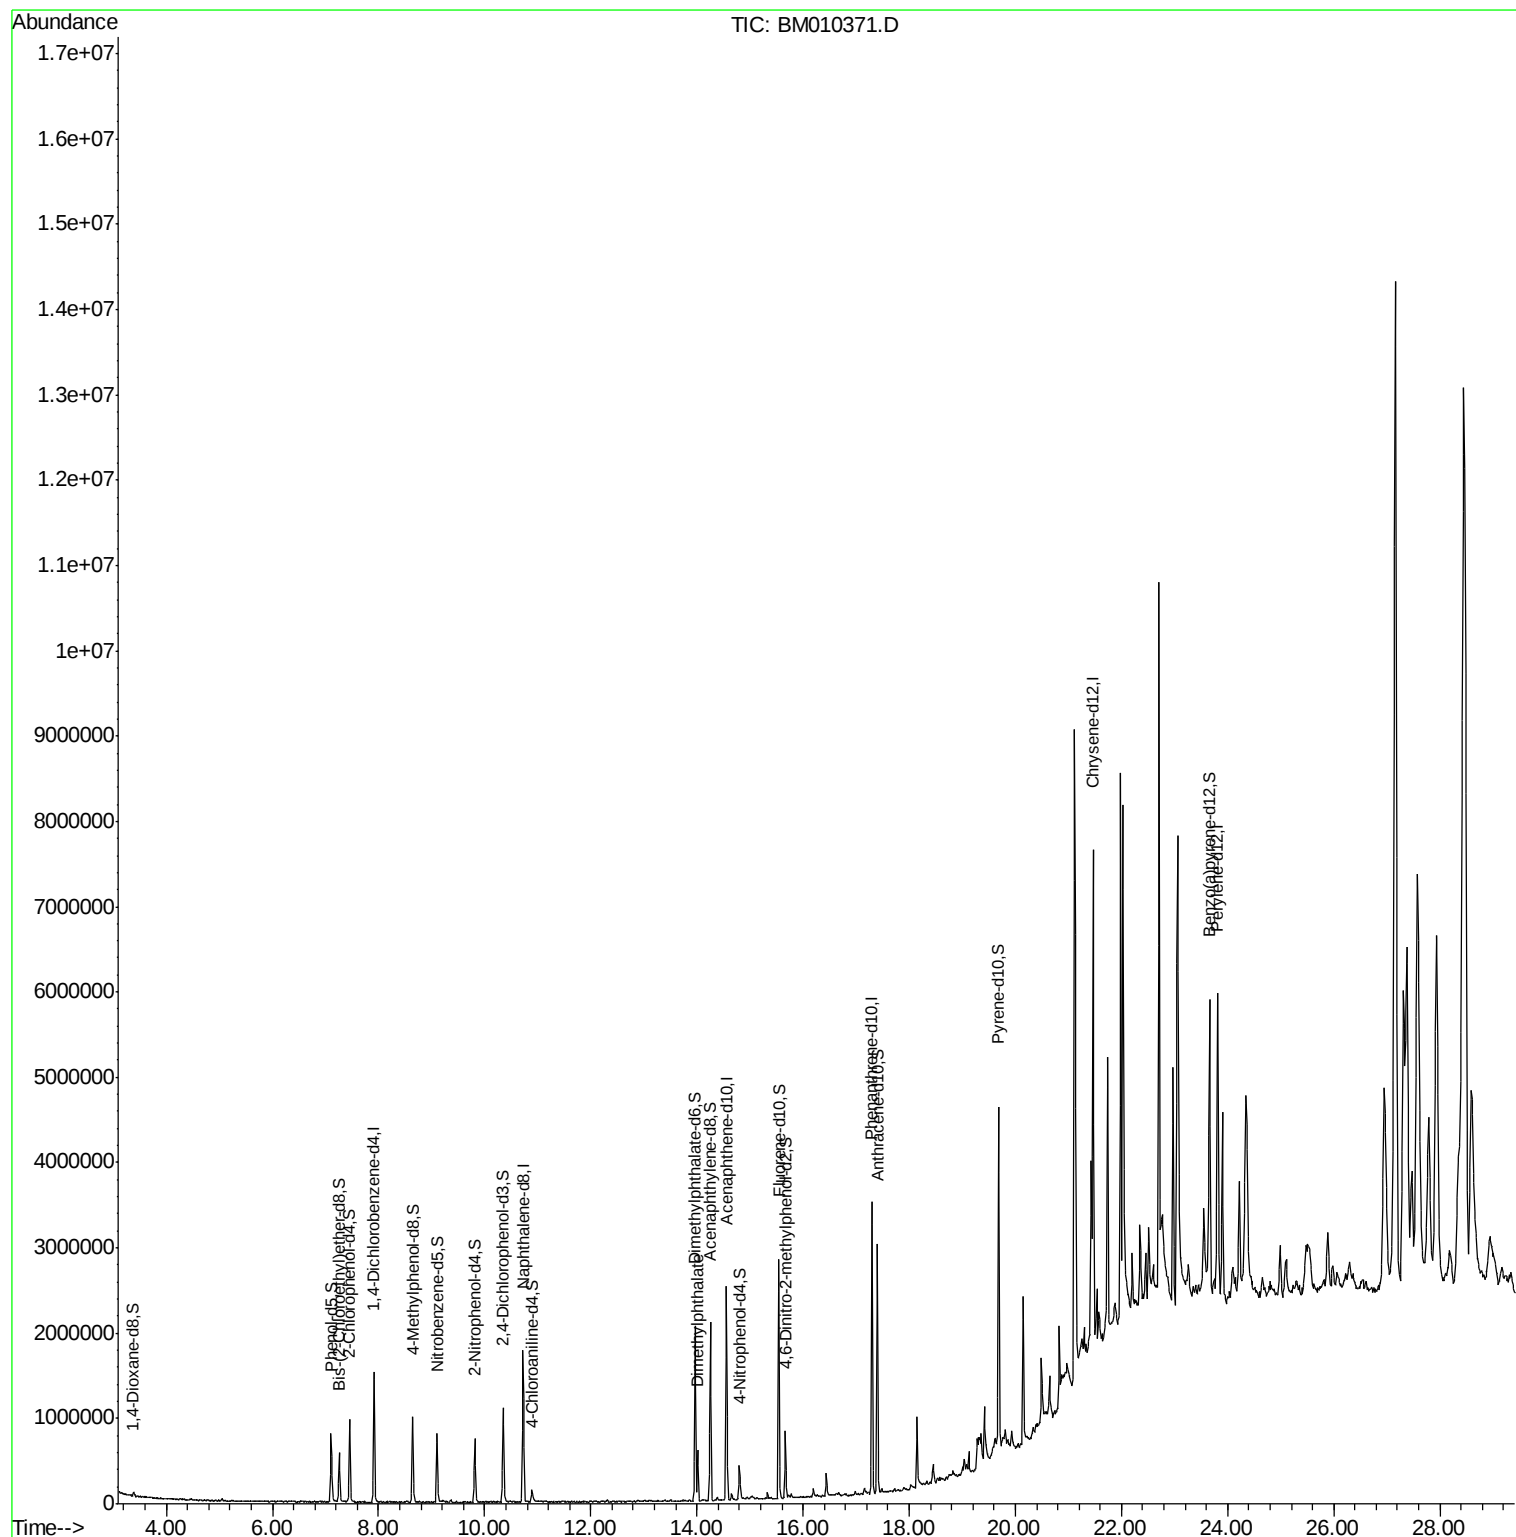

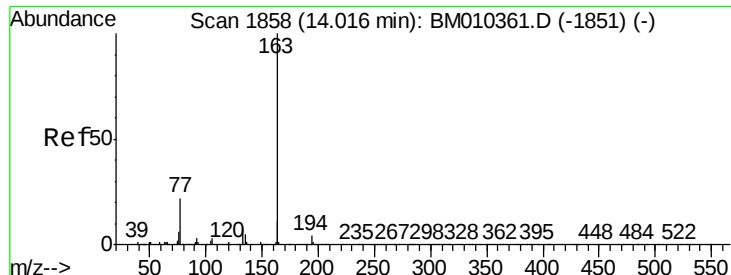

#44

Dimethylphthalate

Concen: 5.320 ng/ul

RT: 14.02 min Scan# 1858

Delta R.T. 0.00 min

Lab File: BM010371.D

Acq: 02 Jun 2017 00:35

Instrument :

BNA_M

ClientSampleId :

JHSG9

Tgt Ion:163 Resp: 332592

Ion Ratio Lower Upper

163 100

194 3.4 3.5 5.3#

164 8.6 8.2 12.4

