

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
 Data File : BM010372.D
 Acq On : 02 Jun 2017 01:10
 Operator : SJ/MA
 Sample : I3163-20
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSH0

Quant Time: Jun 02 01:58:16 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 02 01:55:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	352759	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	1245052	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	765490	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	1798012	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	2656599	20.00	ng/ul	0.00
83) Perylene-d12	23.81	264	2739152	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.38	96	21709	2.52	ng/uL	0.00
5) Phenol-d5	7.10	99	411917	15.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	241609	16.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	359720	16.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.65	113	336040	15.58	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	172506	18.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	202627	19.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	386924	17.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.90	131	9861	0.47	ng/ul	0.01
43) Dimethylphthalate-d6	13.97	166	1248499	19.63	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	1387599	18.70	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	111125	11.68	ng/ul	0.00
57) Fluorene-d10	15.54	176	1042829	18.65	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	190394	14.95	ng/ul	0.00
70) Anthracene-d10	17.40	188	1604701	18.34	ng/ul	0.00
76) Pyrene-d10	19.69	212	2278662	20.74	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.66	264	2600873	20.39	ng/ul	0.00


Target Compounds					Qvalue	
44) Dimethylphthalate	14.02	163	225676	3.608	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
Data File : BM010372.D
Acq On : 02 Jun 2017 01:10
Operator : SJ/MA
Sample : I3163-20
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSH0

Quant Time: Jun 02 01:58:16 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 02 01:55:54 2017
Response via : Initial Calibration

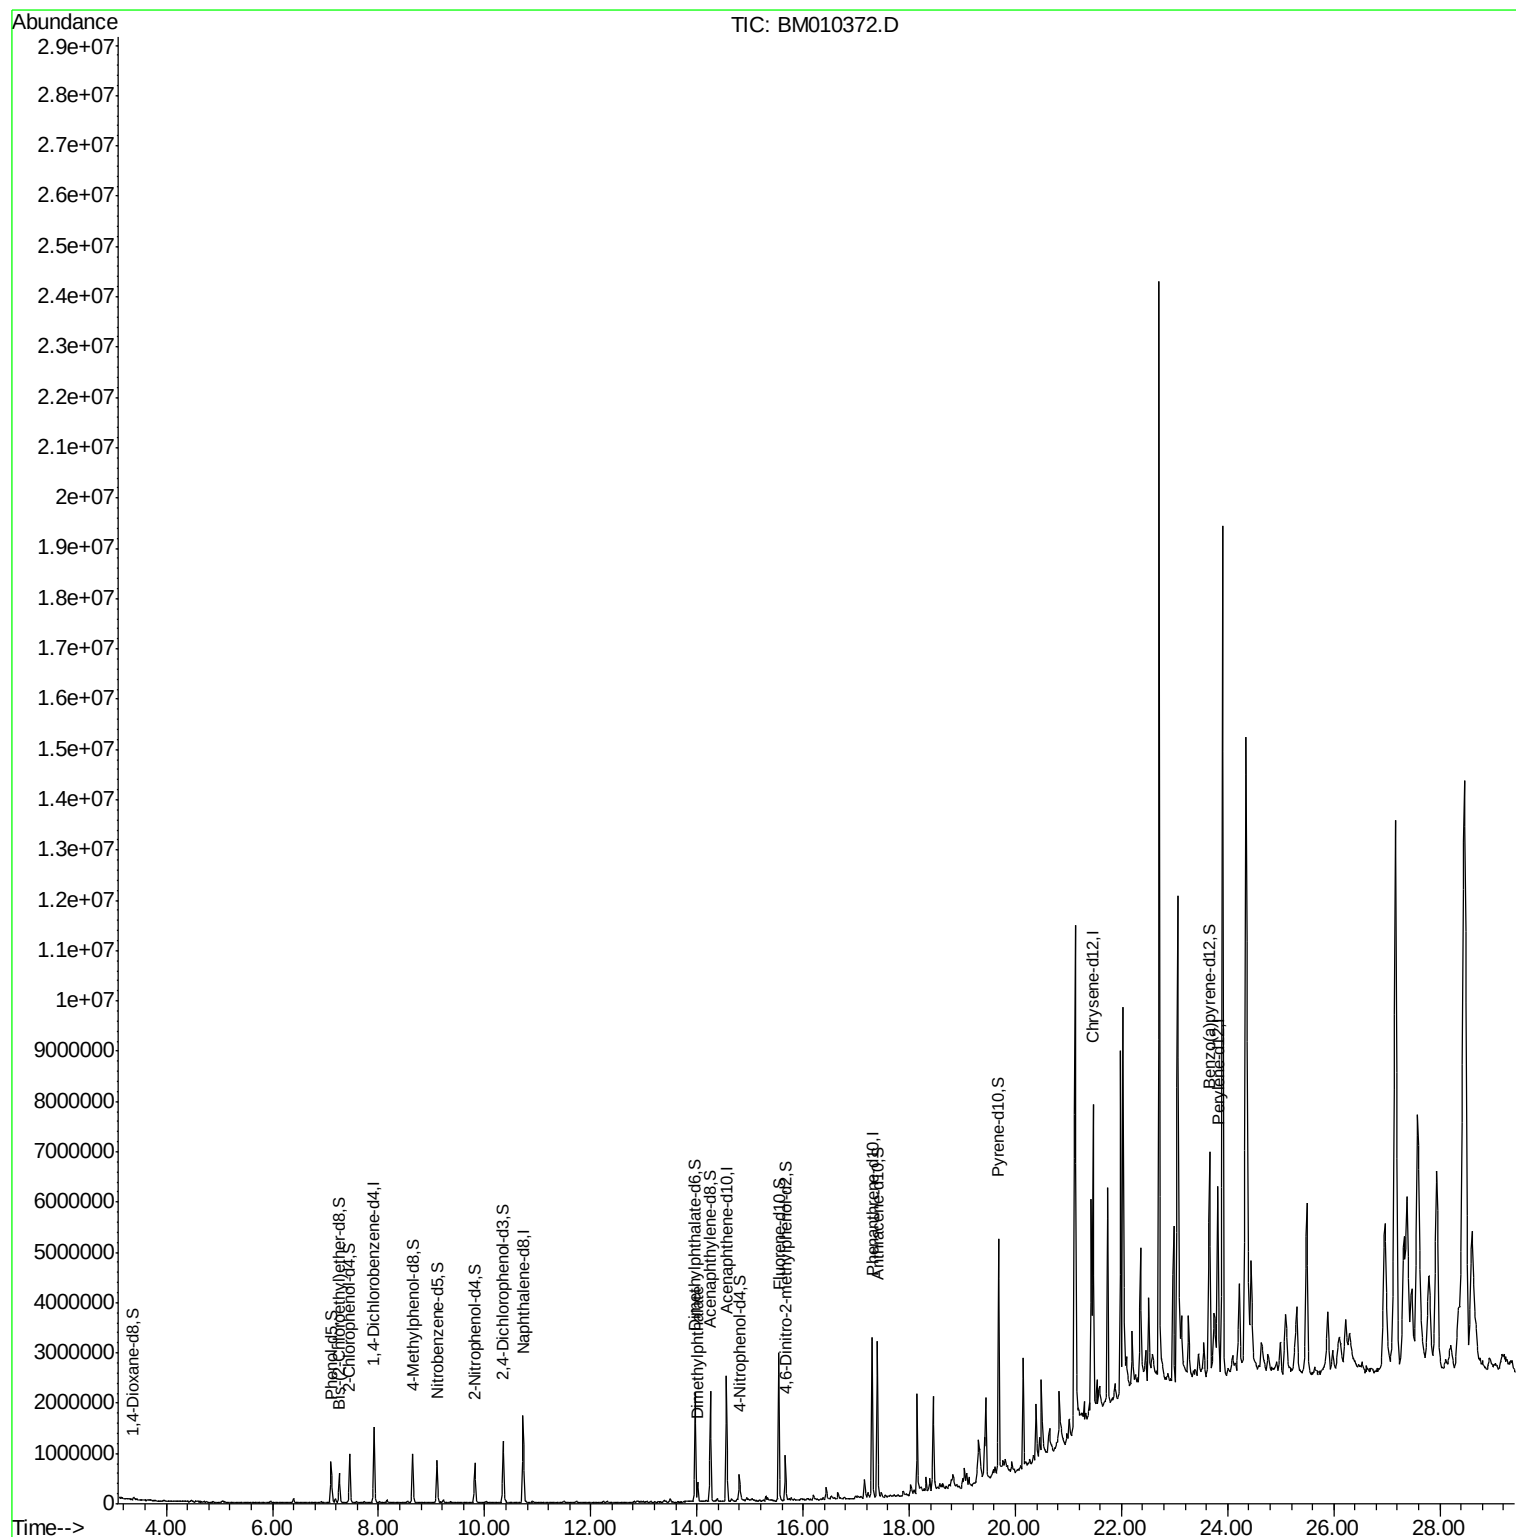

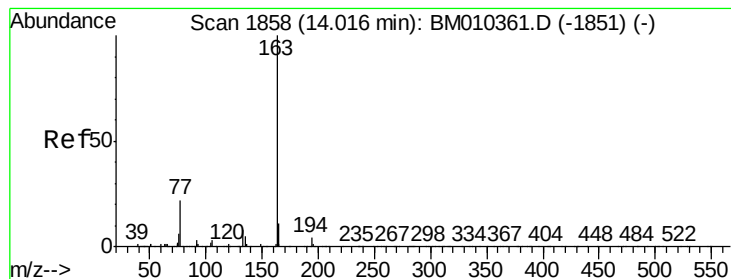

#44

Dimethylphthalate

Concen: 3.608 ng/ul

RT: 14.02 min Scan# 1858

Delta R.T. -0.00 min

Lab File: BM010372.D

Acq: 02 Jun 2017 01:10

Instrument :

BNA_M

ClientSampleId :

JHSH0

Tgt Ion:163 Resp: 225676

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 9.3 8.2 12.4

