

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
 Data File : BM010373.D
 Acq On : 02 Jun 2017 01:46
 Operator : SJ/MA
 Sample : I3163-21
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSH1

Quant Time: Jun 02 04:08:06 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 02 01:55:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.92	152	335396	20.00	ng/ul	0.00
18) Naphthalene-d8	10.72	136	1218224	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.56	164	733707	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.30	188	1734483	20.00	ng/ul	0.00
75) Chrysene-d12	21.46	240	2609453	20.00	ng/ul	0.00
83) Perylene-d12	23.82	264	2652707	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.38	96	20056	2.45	ng/uL	0.00
5) Phenol-d5	7.11	99	383683	15.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.26	67	233203	16.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.46	132	340558	16.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.65	113	230792	11.25	ng/ul	0.00
19) Nitrobenzene-d5	9.10	128	164895	18.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.82	143	194774	18.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.35	165	365098	17.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.90	131	3219	0.16	ng/ul	0.01
43) Dimethylphthalate-d6	13.97	166	1211587	19.87	ng/ul	0.00
46) Acenaphthylene-d8	14.25	160	1384985	19.48	ng/ul	0.00
51) 4-Nitrophenol-d4	14.80	143	75547	8.28	ng/ul	0.01
57) Fluorene-d10	15.55	176	1058973	19.76	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.67	200	171549	13.96	ng/ul	0.00
70) Anthracene-d10	17.40	188	1561240	18.50	ng/ul	0.00
76) Pyrene-d10	19.69	212	2124259	19.69	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.66	264	2308303	18.69	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	14.02	163	211521	3.528 ng/ul	98
81) Bis(2-ethylhexyl)phthalate	21.33	149	73331	1.061 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060117\
Data File : BM010373.D
Acq On : 02 Jun 2017 01:46
Operator : SJ/MA
Sample : I3163-21
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSH1

Quant Time: Jun 02 04:08:06 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM052717.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 02 01:55:54 2017
Response via : Initial Calibration




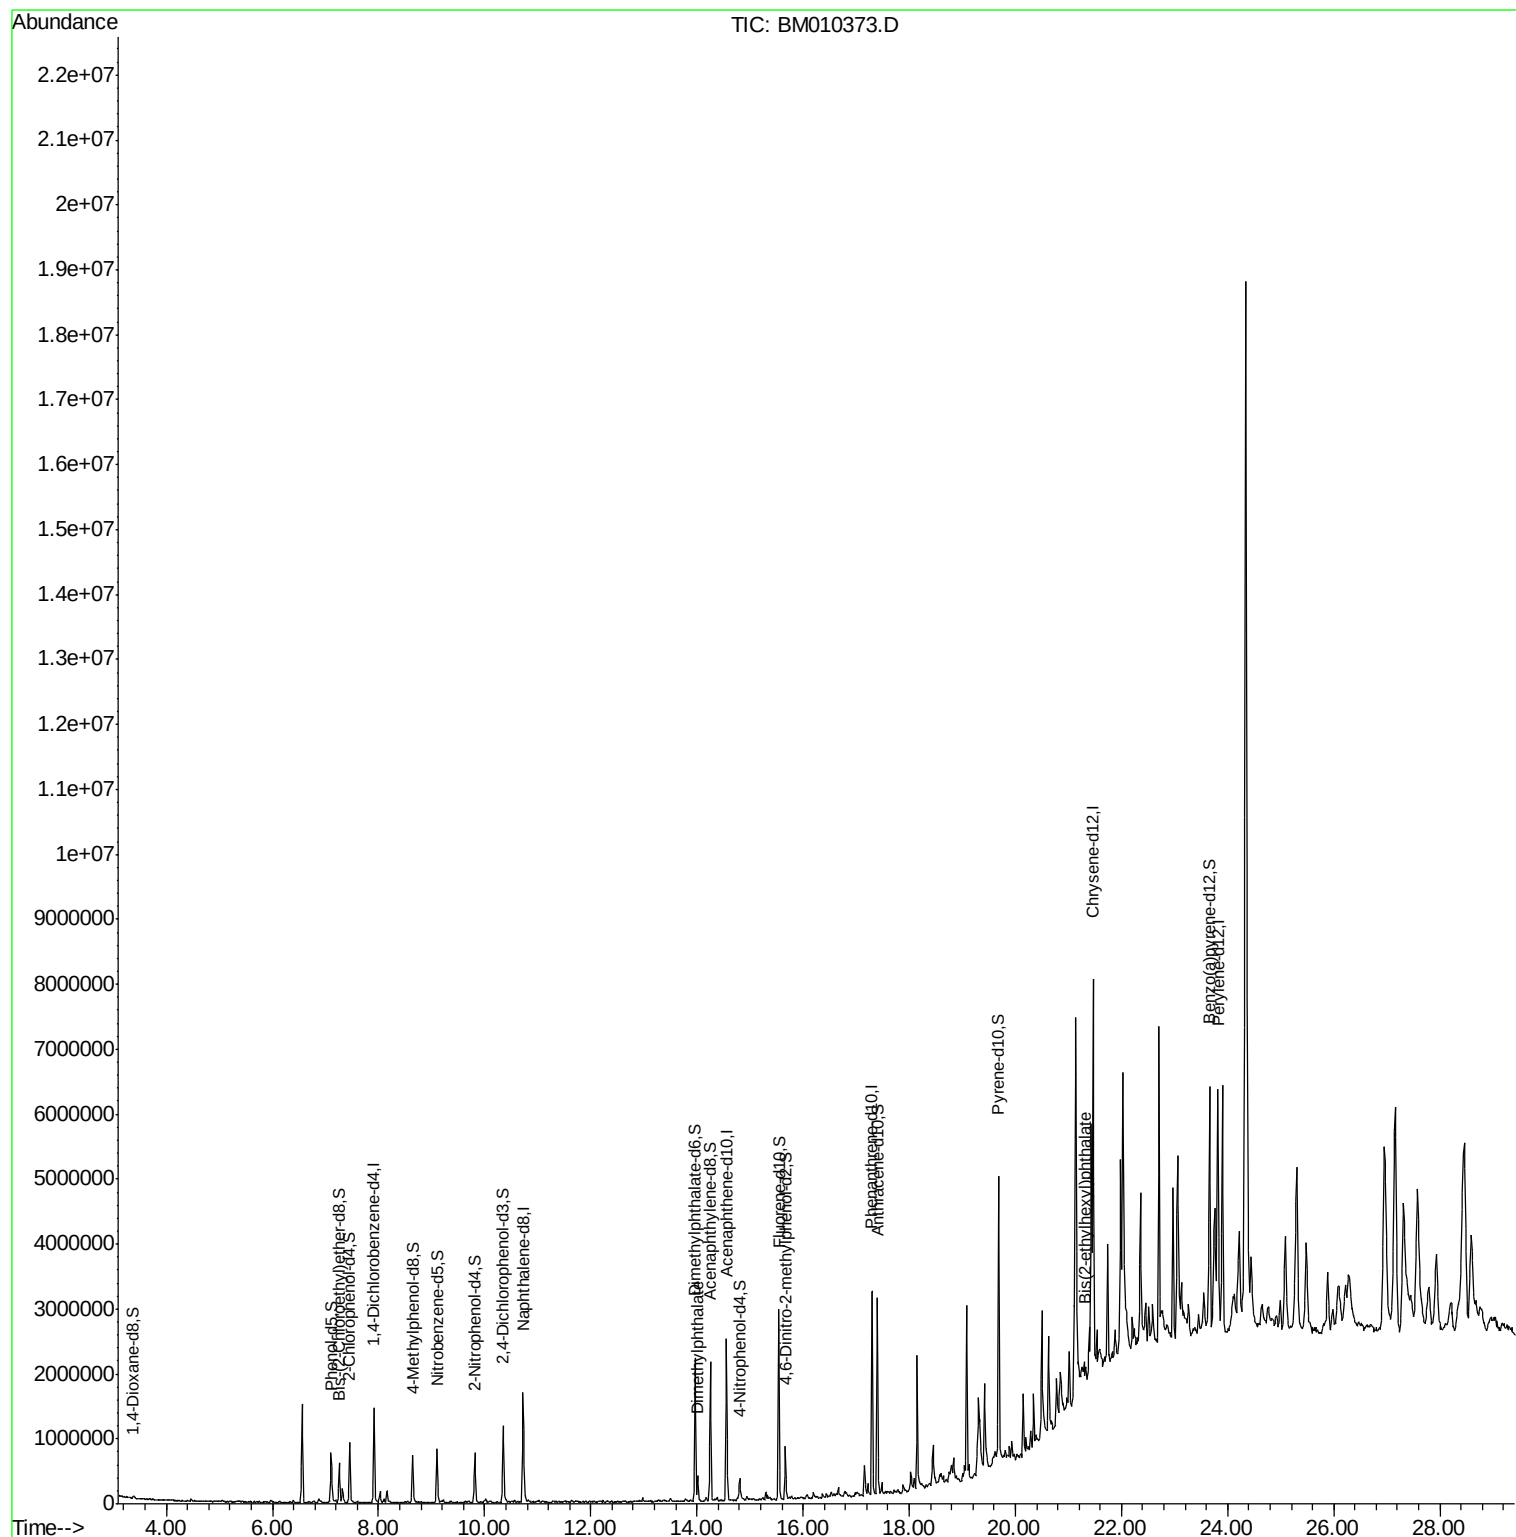


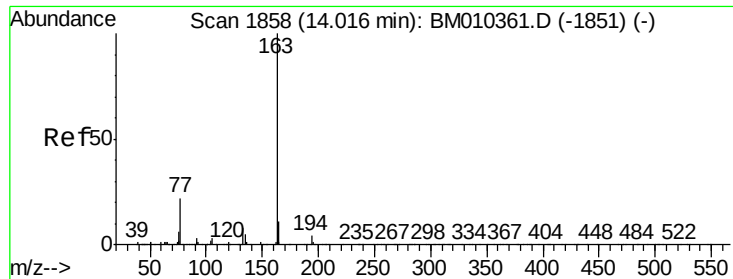

#44
 Dimethylphthalate
 Concen: 3.528 ng/ul
 RT: 14.02 min Scan# 1858
 Delta R.T. 0.00 min
 Lab File: BM010373.D
 Acq: 02 Jun 2017 01:46

Instrument :
 BNA_M
 ClientSampleId :
 JHSH1

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.5	3.5	5.3
164	11.1	8.2	12.4

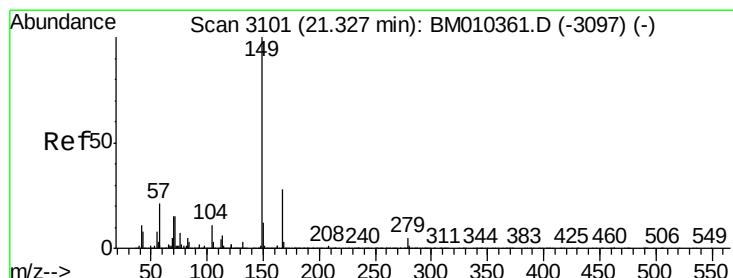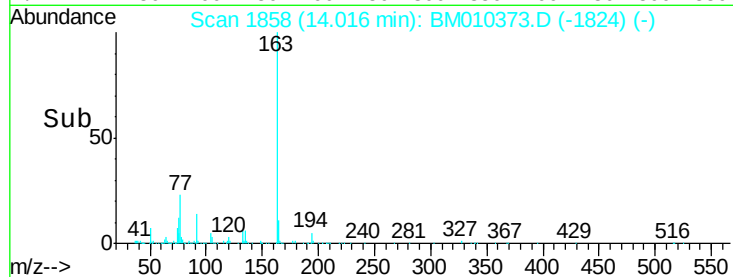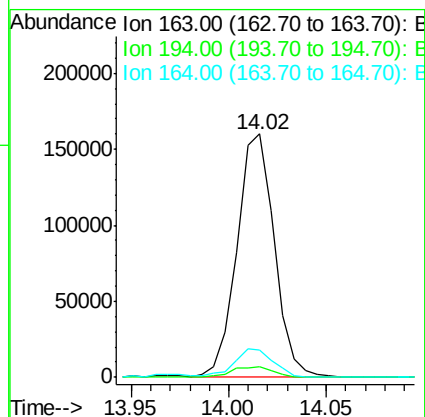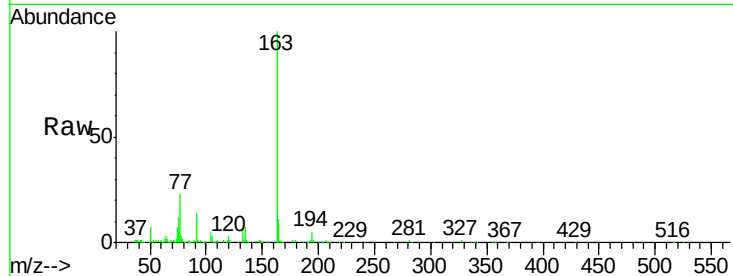

#81
 Bis(2-ethylhexyl)phthalate
 Concen: 1.061 ng/ul
 RT: 21.33 min Scan# 3102
 Delta R.T. 0.01 min
 Lab File: BM010373.D
 Acq: 02 Jun 2017 01:46

Tgt Ion	Ratio	Lower	Upper
149	100		
167	29.3	22.8	34.2
279	6.6	4.9	7.3

