


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060121\
Data File : BM030239.D
Acq On : 01 Jun 2021 16:03
Operator : CG/JU
Sample : PB136659BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK659

Manual Integrations
APPROVED

mohammad
6/2/2021 10:53:33 AM

Quant Time: Jun 01 16:35:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 01 15:22:57 2021
Response via : Initial Calibration

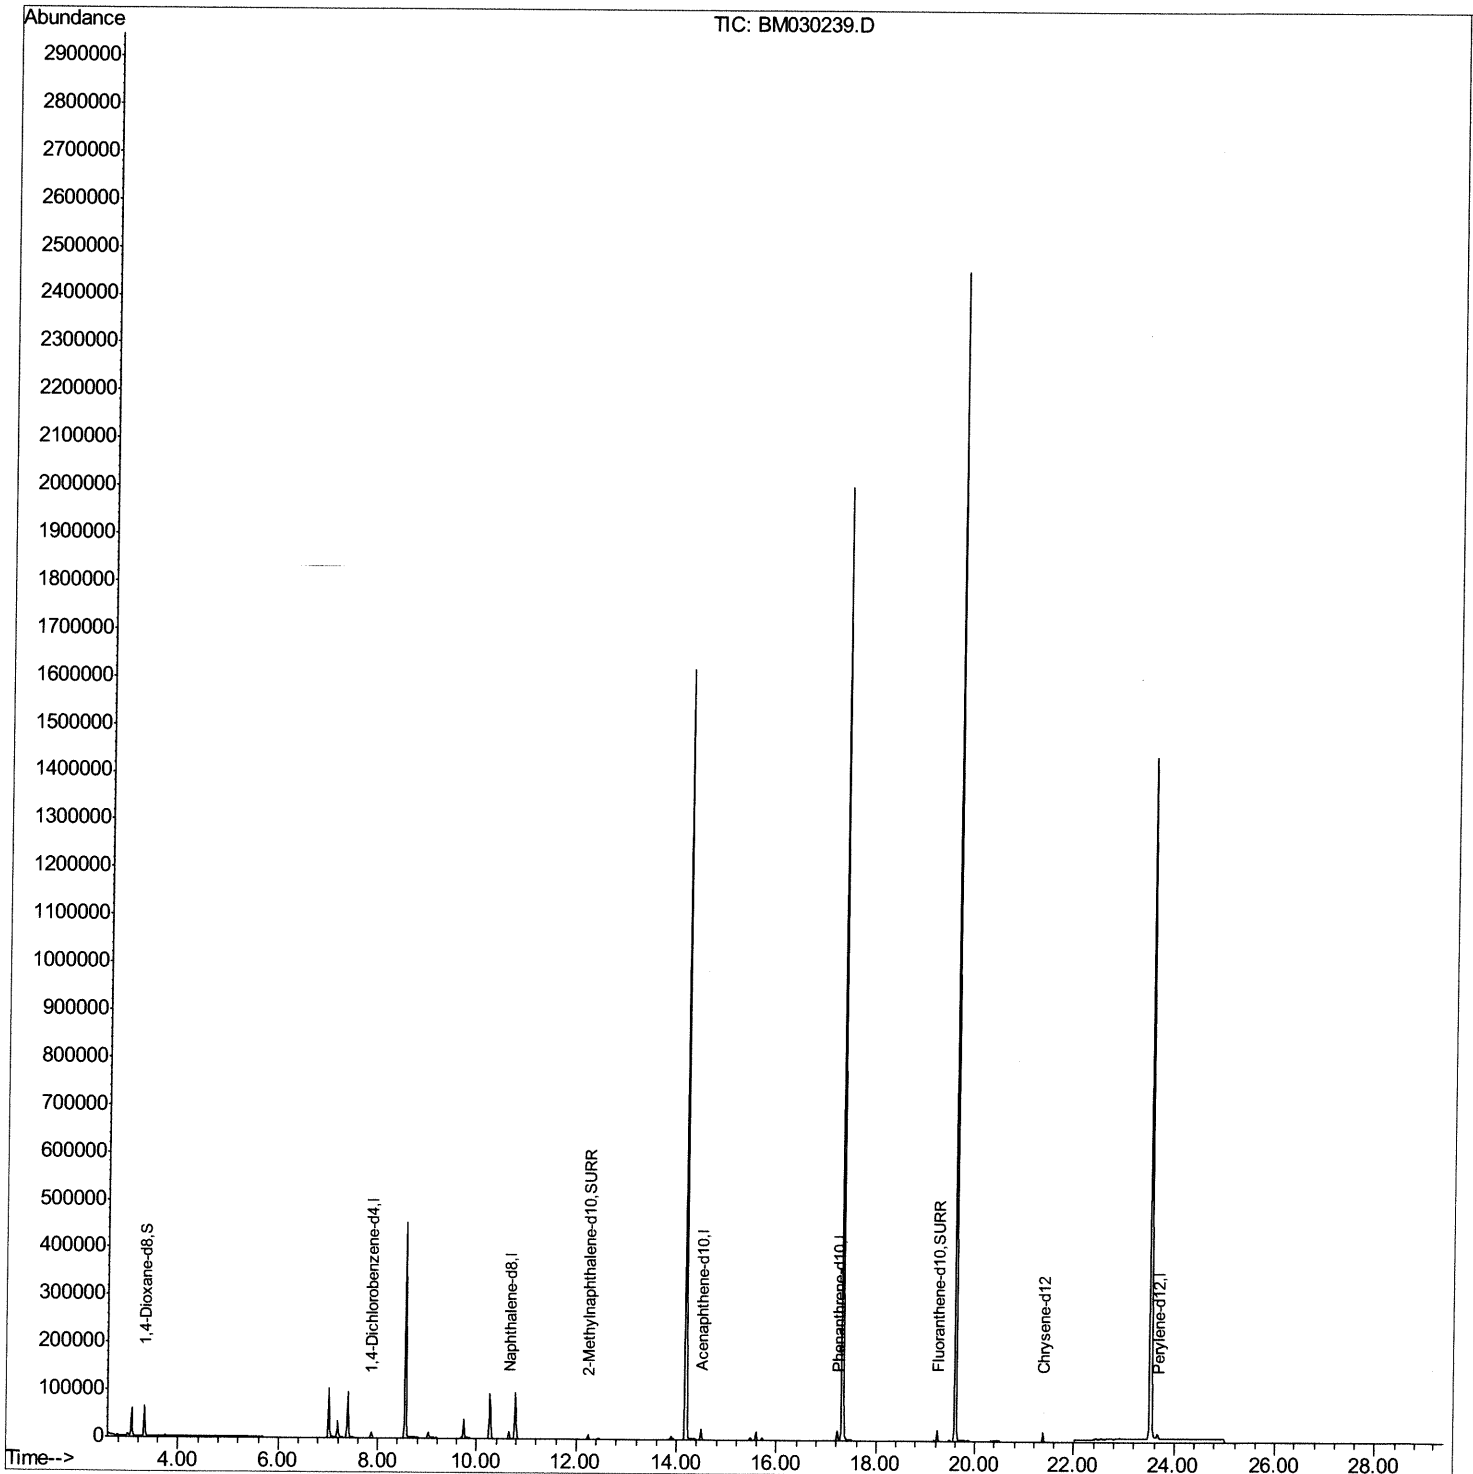

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060121\
 Data File : BM030239.D
 Acq On : 01 Jun 2021 16:03
 Operator : CG/JU
 Sample : PB136659BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK659

Manual Integrations
APPROVED

mohammad
 6/2/2021 10:53:33 AM

Quant Time: Jun 01 16:34:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 01 15:22:57 2021
 Response via : Initial Calibration

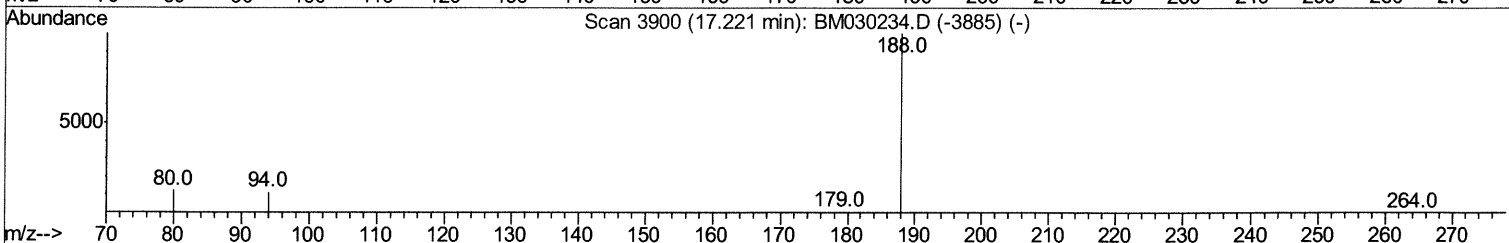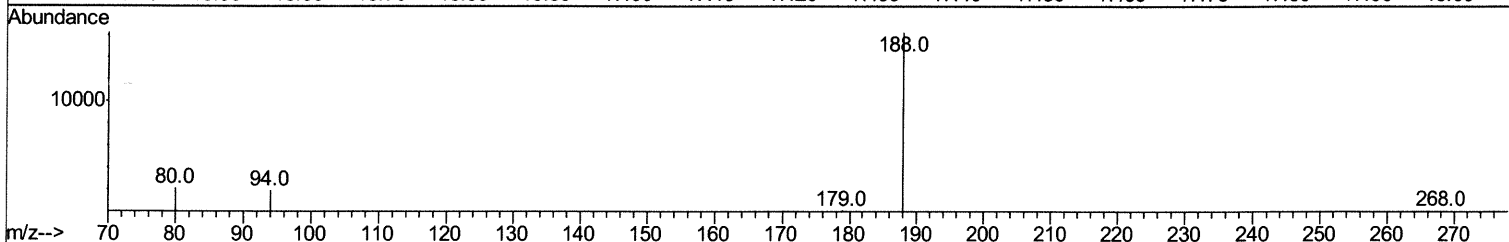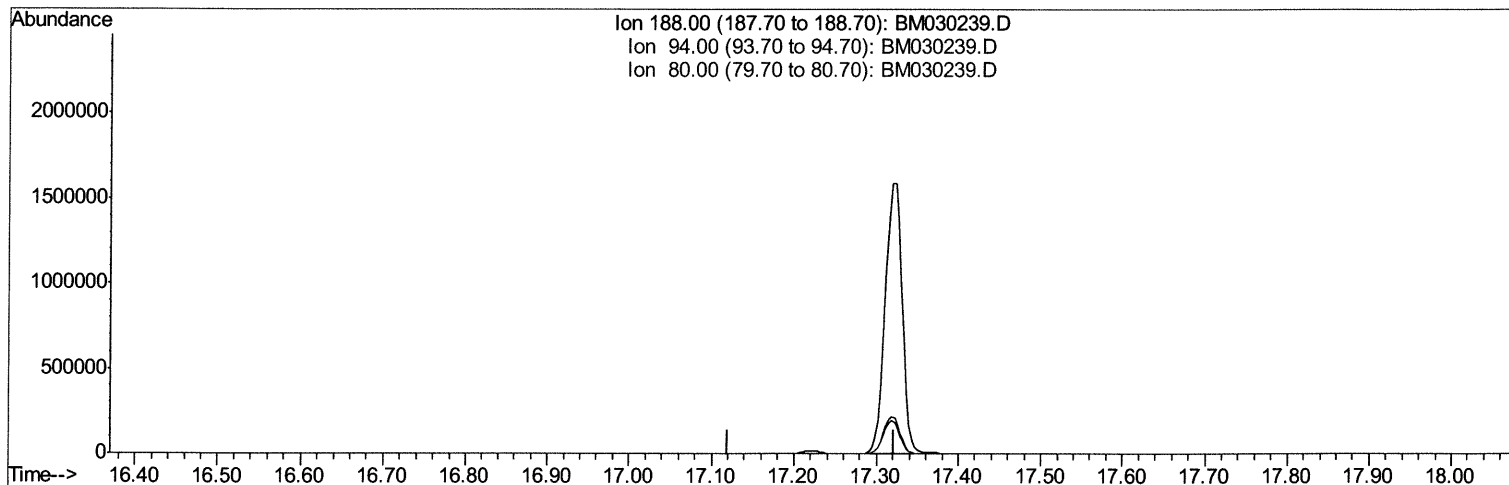

TIC: BM030239.D

(13) Phenanthrene-d10 (I)

17.221min (-17.221) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.80	0.00#
80.00	12.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060121\
 Data File : BM030239.D
 Acq On : 01 Jun 2021 16:03
 Operator : CG/JU
 Sample : PB136659BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK659

Manual Integrations
 APPROVED

mohammad
 6/2/2021 10:53:33 AM

Quant Time: Jun 01 16:34:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 01 15:22:57 2021
 Response via : Initial Calibration

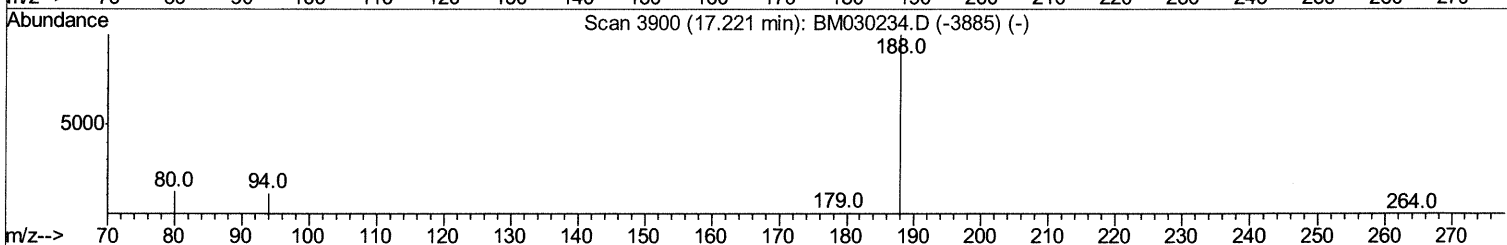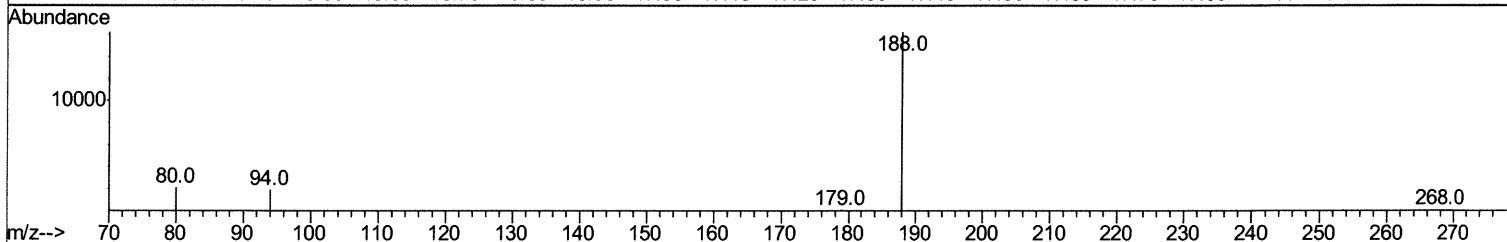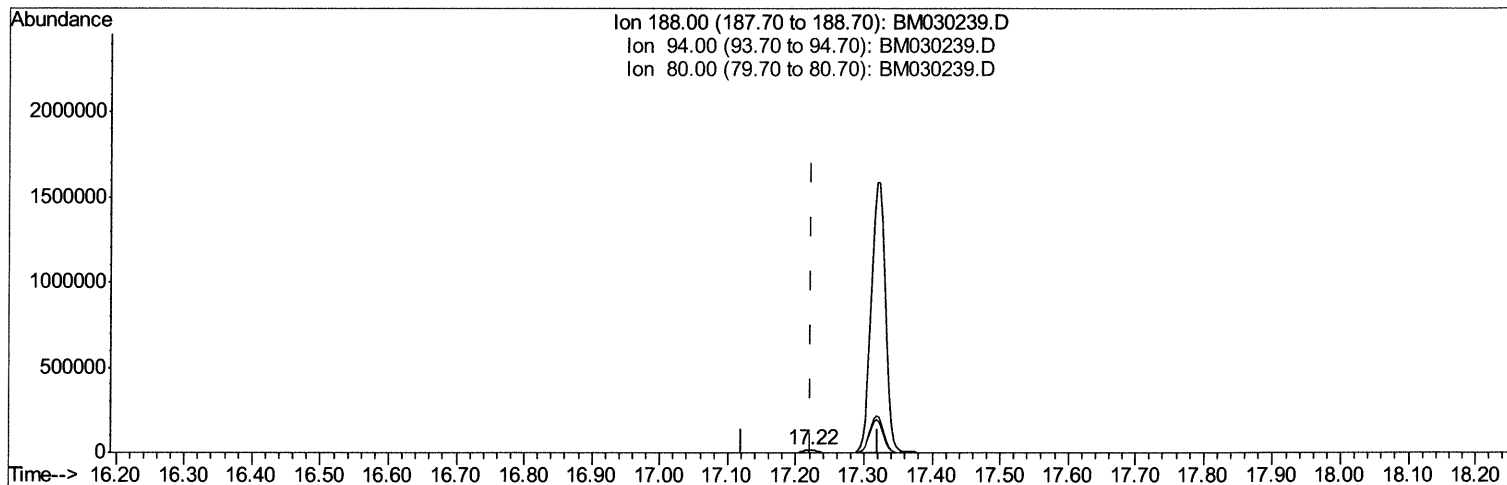

TIC: BM030239.D

(13) Phenanthrene-d10 (I)

17.221min (+0.000) 0.40ng/ul m 06/03/21 JU

response 22703

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	11.68
80.00	12.90	13.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060121\
Data File : BM030239.D
Acq On : 01 Jun 2021 16:03
Operator : CG/JU
Sample : PB136659BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK659

Manual Integrations
APPROVED

mohammad
6/2/2021 10:53:33 AM

Quant Time: Jun 01 16:35:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 01 15:22:57 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	5380	0.40	ng/ul	0.00
4) Naphthalene-d8	10.66	136	19842	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.49	164	12285	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.22	188	22703m>	0.40	ng/ul>	0.00 6/6/21 JU
17) Chrysene-d12	21.38	240	16182	0.40	ng/ul	0.00
23) Perylene-d12	23.67	264	16298	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.33	96	39635	7.51	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.24	152	12372	0.44	ng/ul	0.00
18) Fluoranthene-d10	19.24	212	23767	0.44	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed