


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
Data File : BM030244.D
Acq On : 01 Jun 2021 19:45
Operator : CG/JU
Sample : PB136685BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK685

Manual Integrations
APPROVED

mohammad
6/2/2021 10:53:41 AM

Quant Time: Jun 02 01:14:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 01 15:22:57 2021
Response via : Initial Calibration

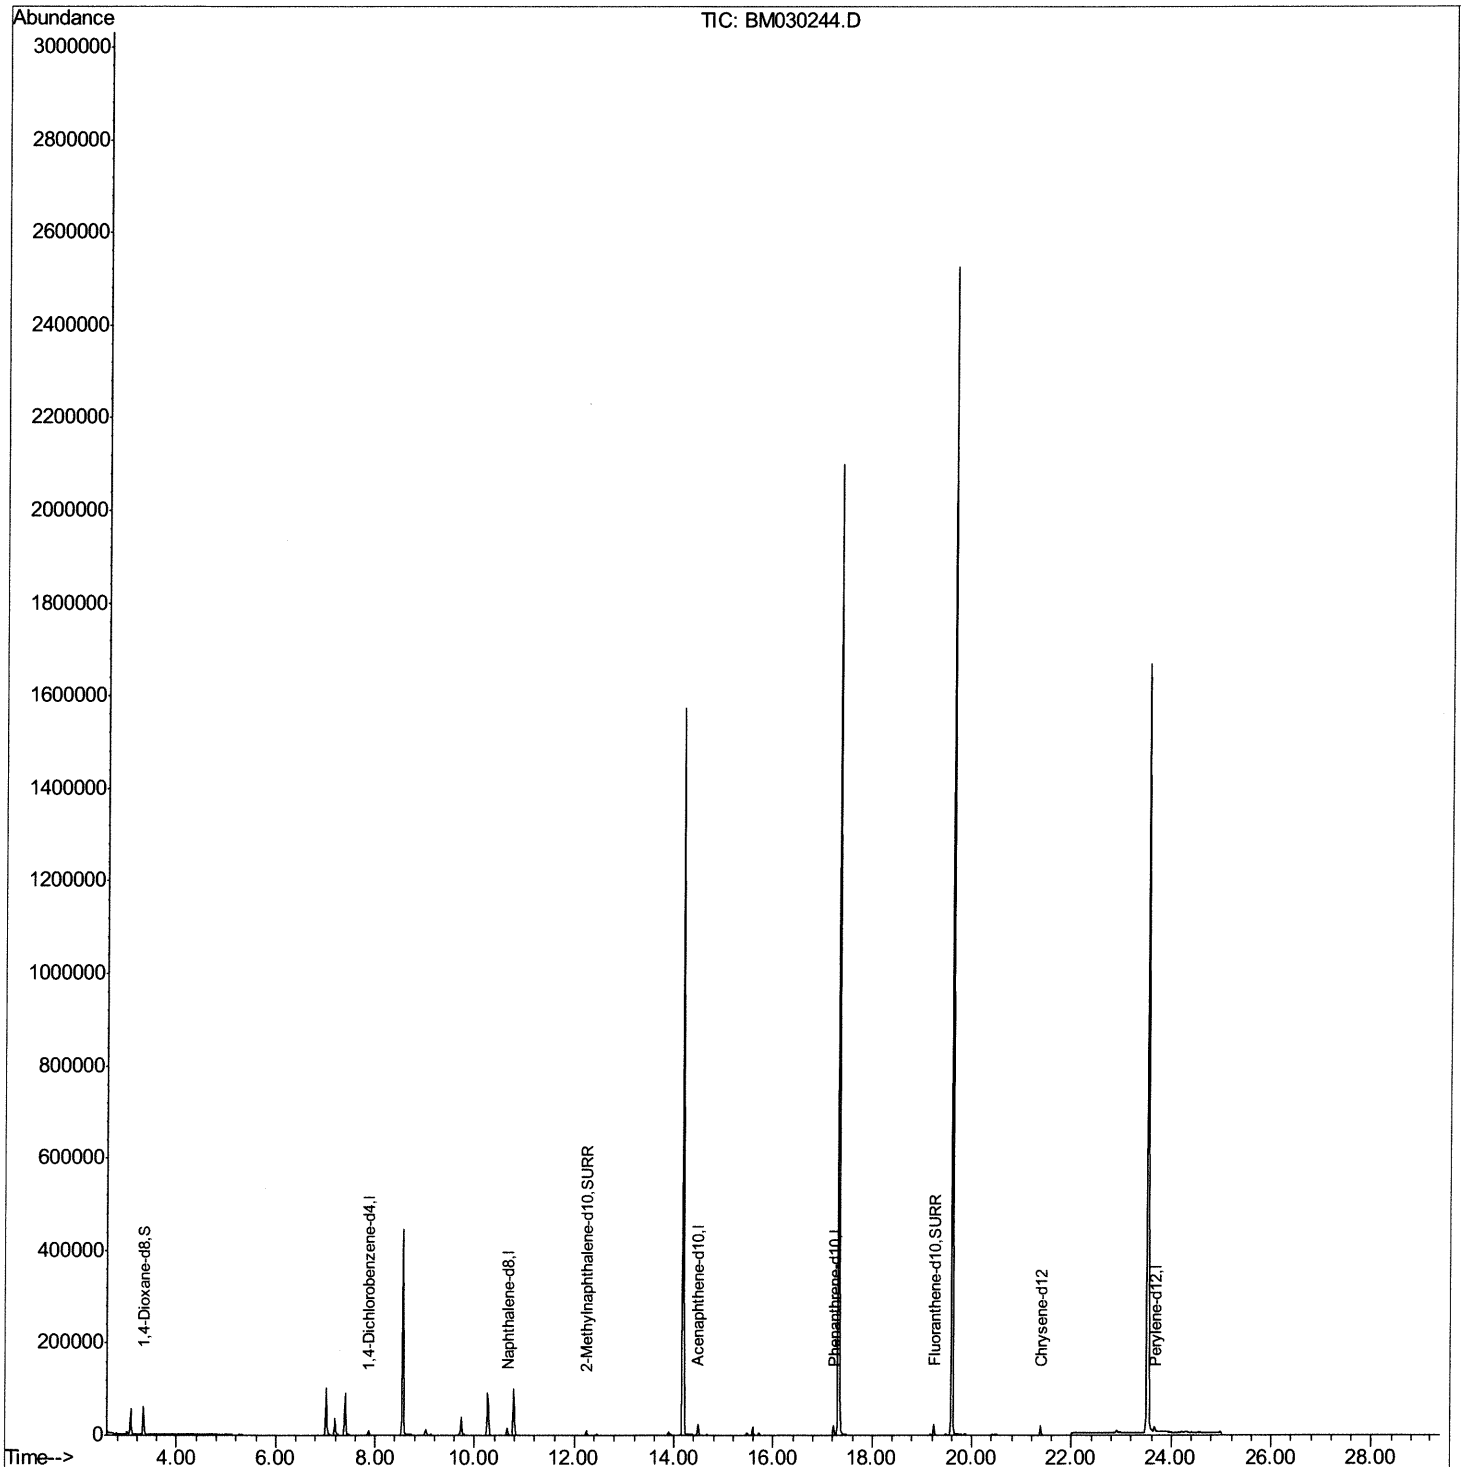

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
 Data File : BM030244.D
 Acq On : 01 Jun 2021 19:45
 Operator : CG/JU
 Sample : PB136685BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK685

Manual Integrations
APPROVED

mohammad
 6/2/2021 10:53:41 AM

Quant Time: Jun 02 01:10:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 01 15:22:57 2021
 Response via : Initial Calibration

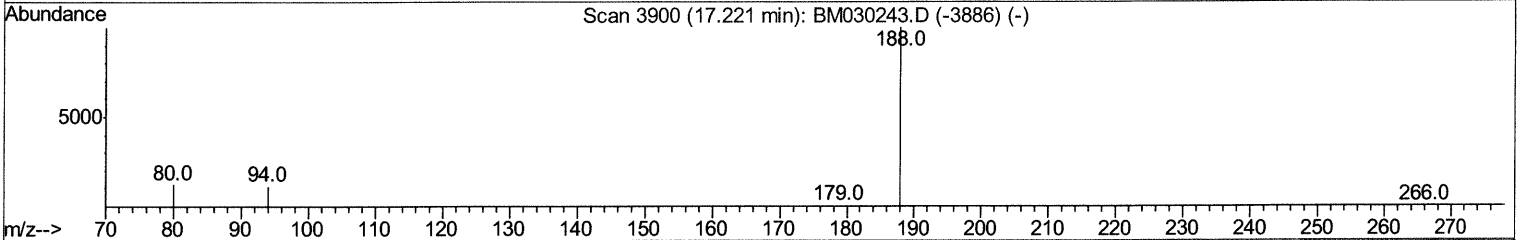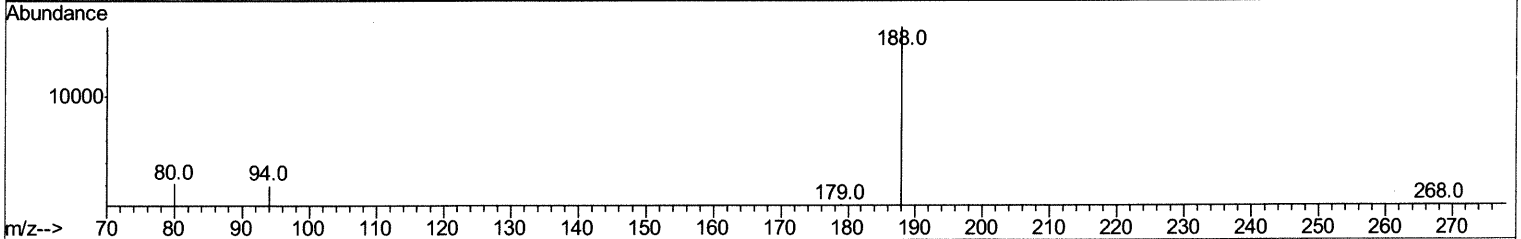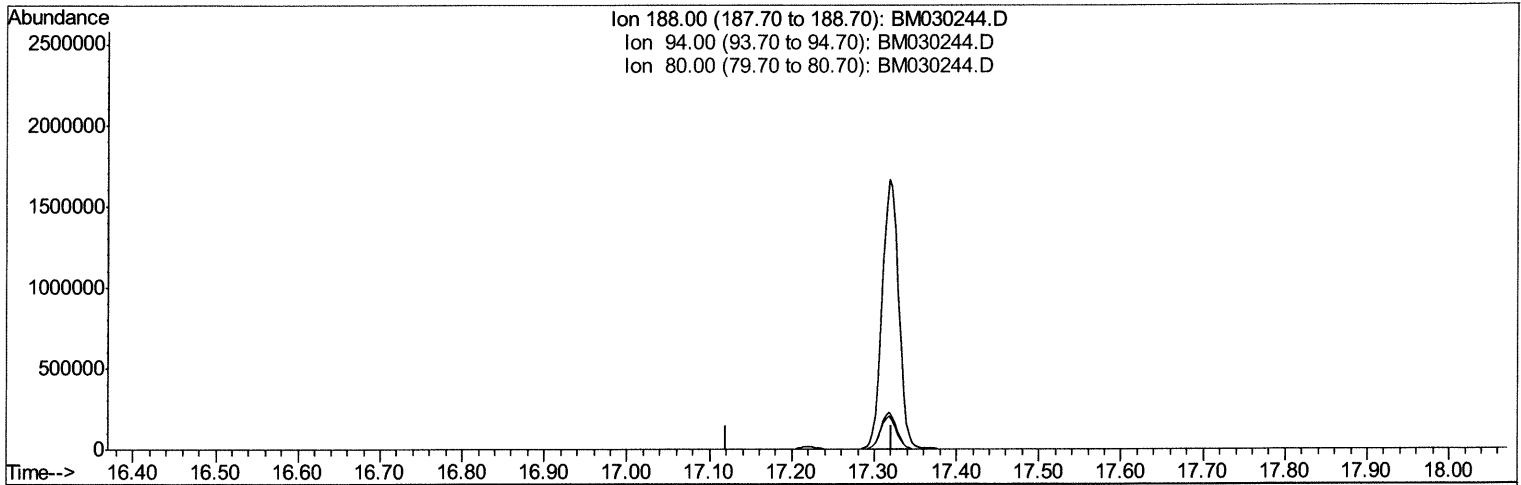

TIC: BM030244.D

(13) Phenanthrene-d10 (I)
 17.221min (-17.221) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.80	0.00#
80.00	12.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
Data File : BM030244.D
Acq On : 01 Jun 2021 19:45
Operator : CG/JU
Sample : PB136685BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK685

Manual Integrations
APPROVED

mohammad
6/2/2021 10:53:41 AM

Quant Time: Jun 02 01:12:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 01 15:22:57 2021
Response via : Initial Calibration

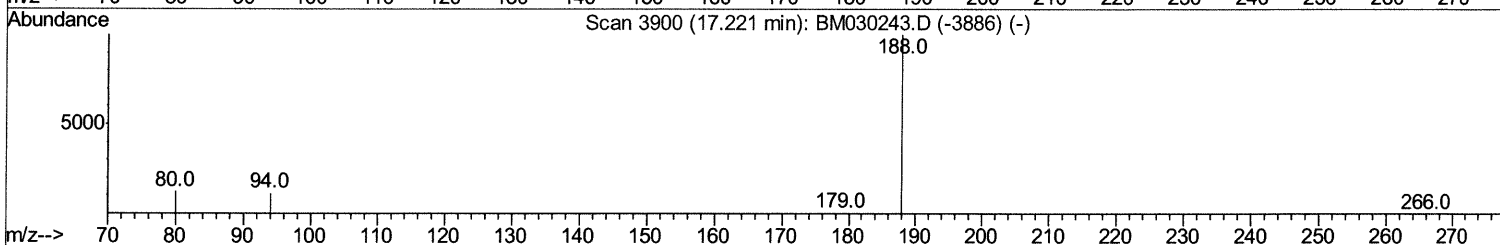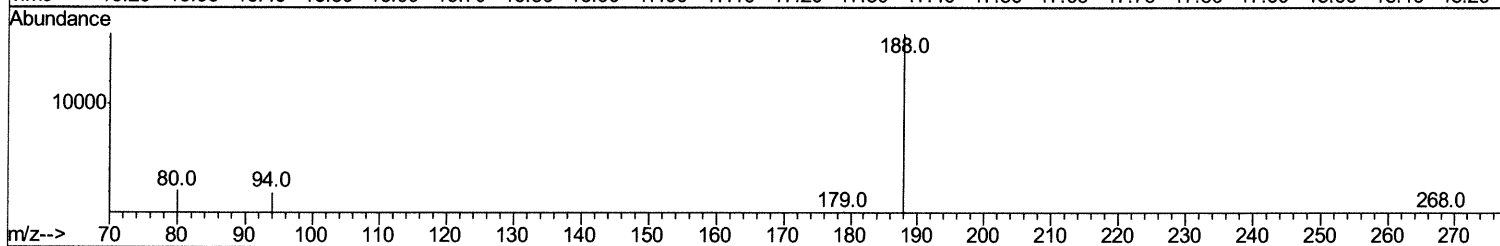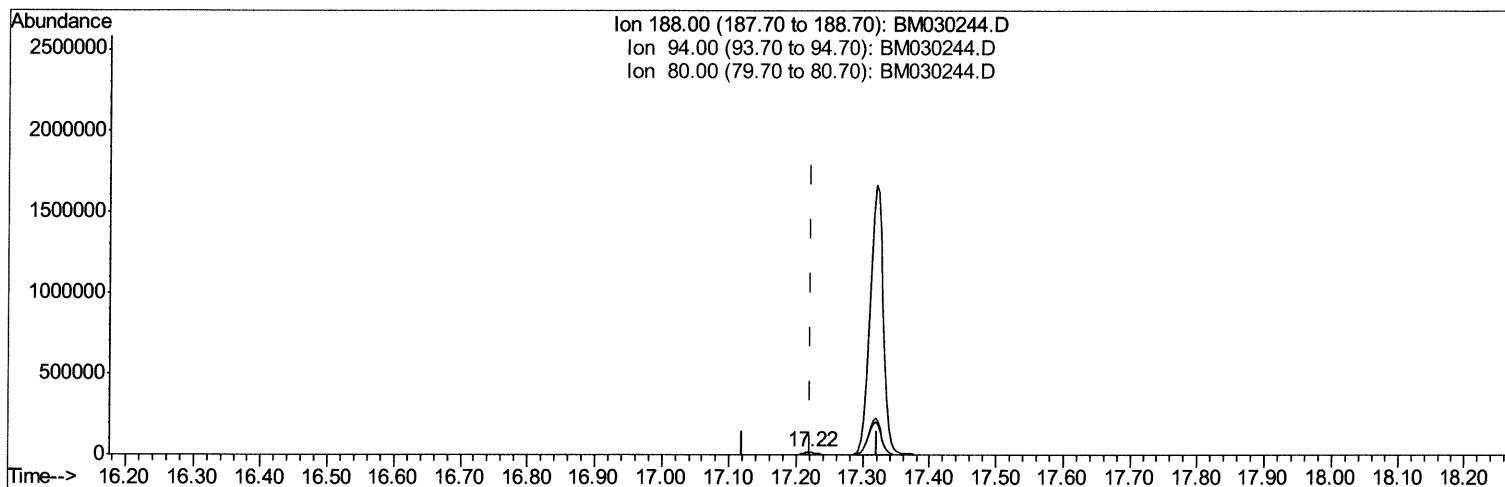

TIC: BM030244.D

(13) Phenanthrene-d10 (I)

17.221min (-0.000) 0.40ng/ul m 06/02/21 JU

response 22930

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	11.35
80.00	12.90	12.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
Data File : BM030244.D
Acq On : 01 Jun 2021 19:45
Operator : CG/JU
Sample : PB136685BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK685

Manual Integrations
APPROVED

mohammad
6/2/2021 10:53:41 AM

Quant Time: Jun 02 01:14:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 01 15:22:57 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	5158	0.40	ng/ul	0.00
4) Naphthalene-d8	10.66	136	19456	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.49	164	12139	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.22	188	22930m>	0.40	ng/ul>	0.00
17) Chrysene-d12	21.38	240	17351	0.40	ng/ul	0.00
23) Perylene-d12	23.67	264	18429	0.40	ng/ul	0.00

06/03/21 JU

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	38060	7.52	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.24	152	12136	0.44	ng/ul	0.00
18) Fluoranthene-d10	19.24	212	24909	0.43	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed