


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
Data File : BM030246.D
Acq On : 01 Jun 2021 20:58
Operator : CG/JU
Sample : M2528-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARK5

Manual Integrations
APPROVED

mohammad
6/2/2021 10:53:44 AM

Quant Time: Jun 02 01:18:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 02 01:10:46 2021
Response via : Initial Calibration

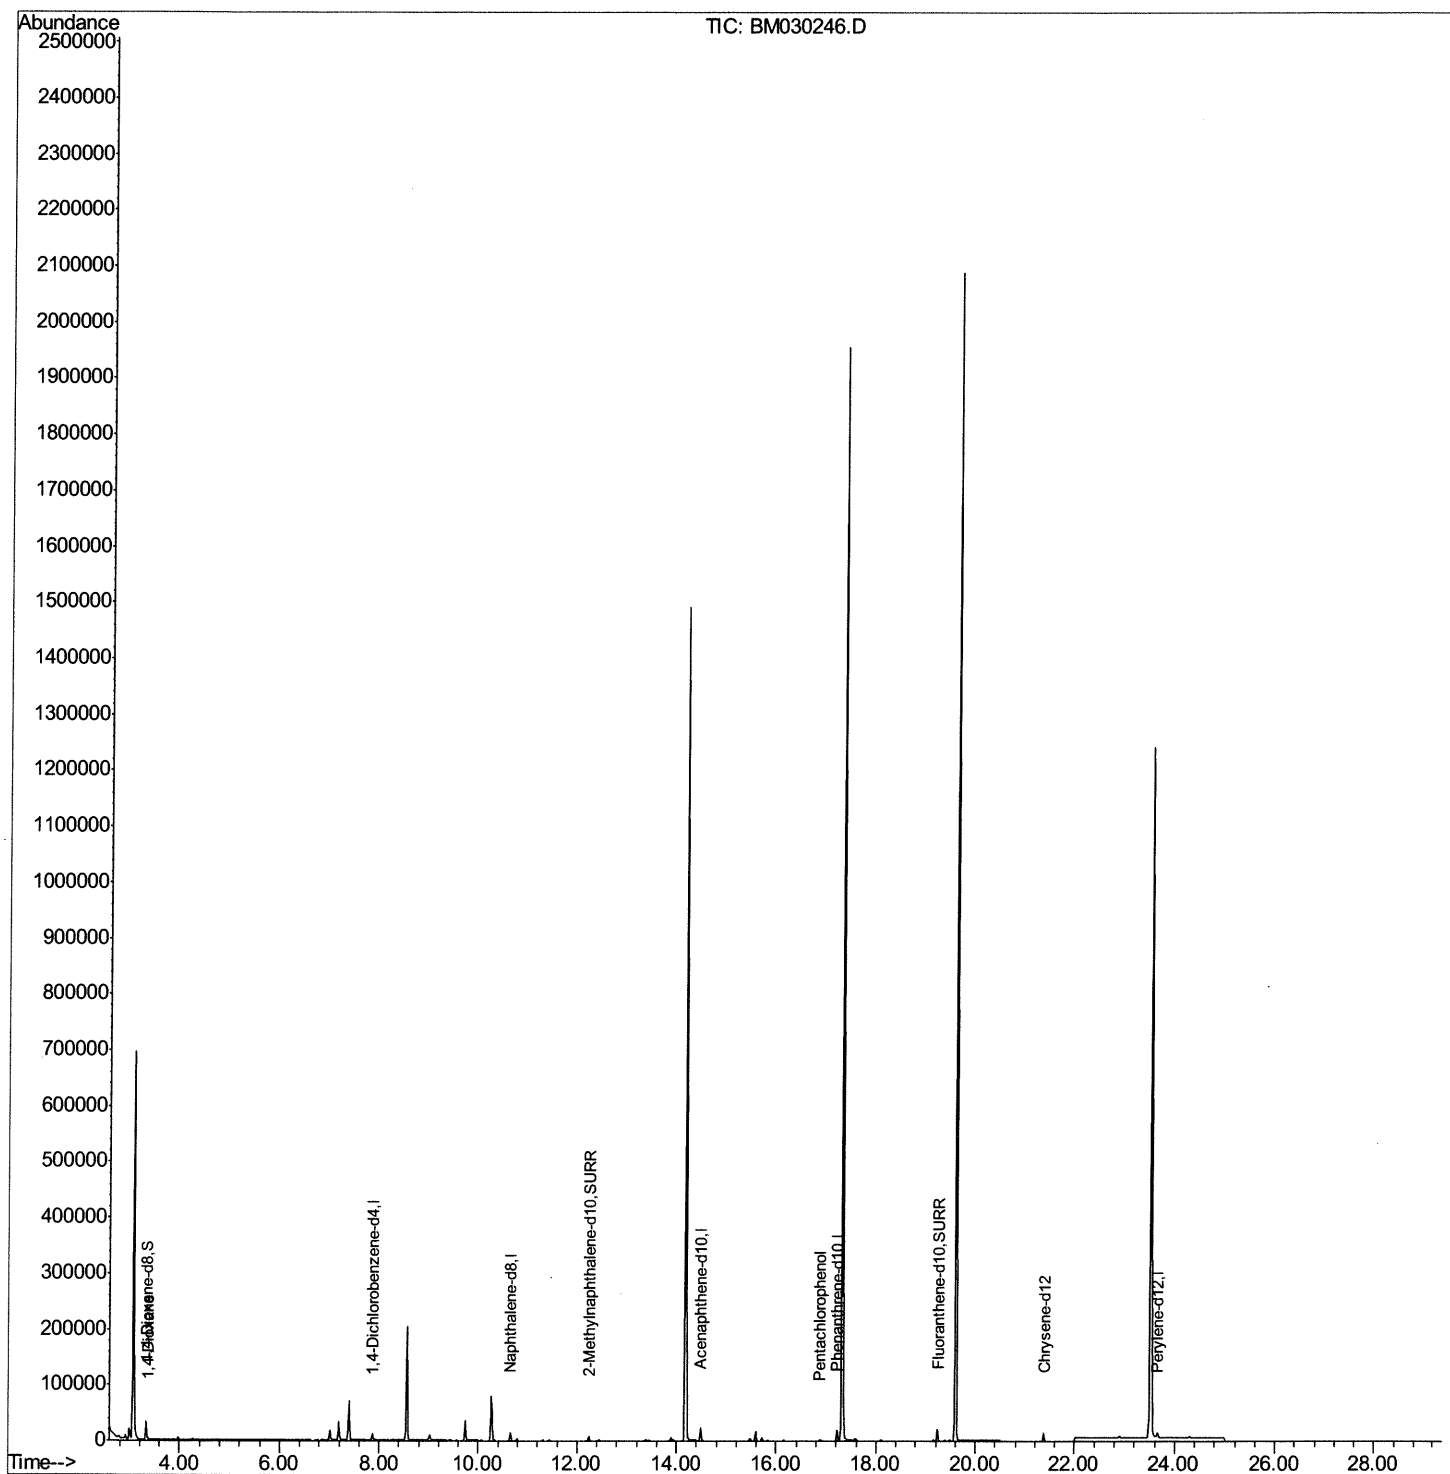

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
 Data File : BM030246.D
 Acq On : 01 Jun 2021 20:58
 Operator : CG/JU
 Sample : M2528-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARK5

Manual Integrations
 APPROVED

mohammad
 6/2/2021 10:53:44 AM

Quant Time: Jun 02 01:11:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 02 01:10:46 2021
 Response via : Initial Calibration

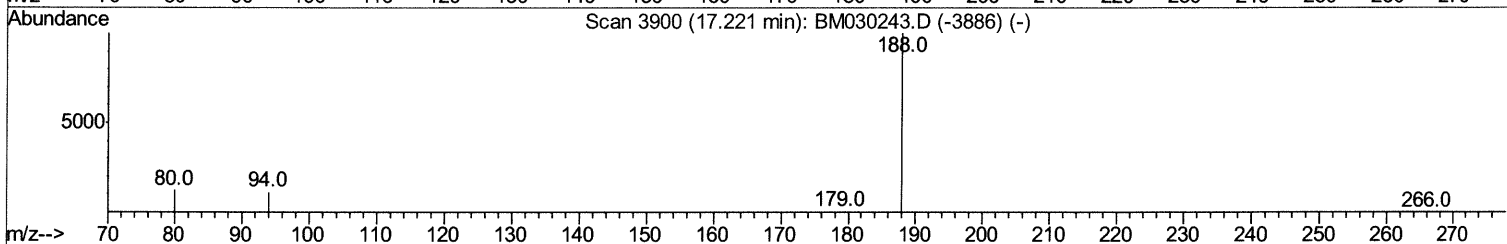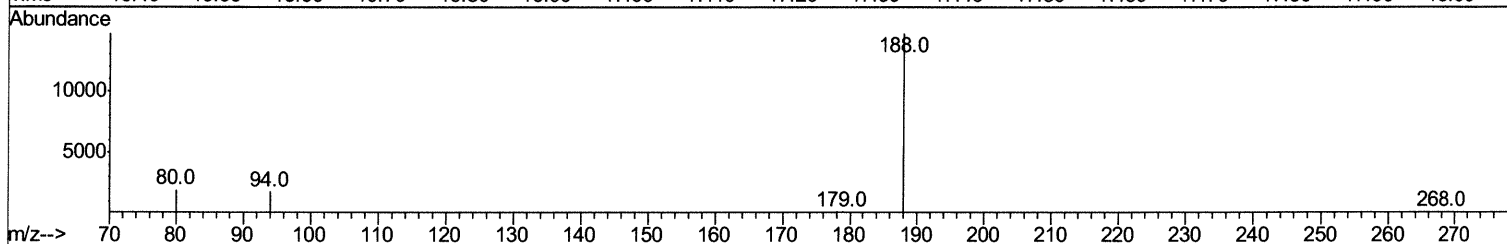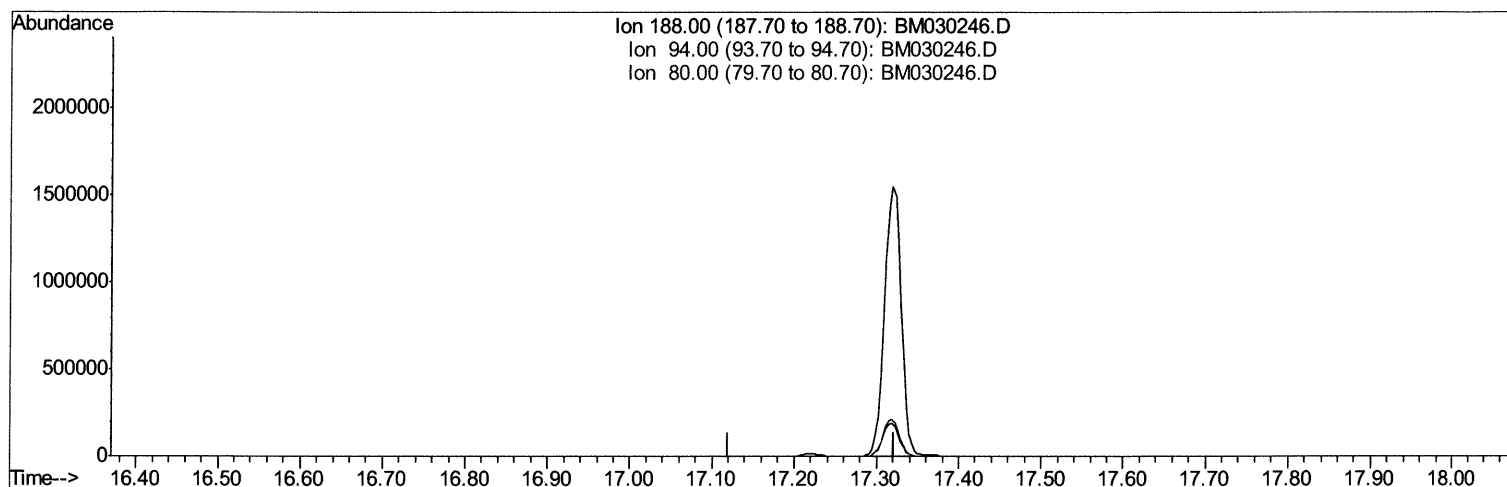

TIC: BM030246.D

(13) Phenanthrene-d10 (I)

17.221min (-17.221) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.80	0.00#
80.00	12.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
 Data File : BM030246.D
 Acq On : 01 Jun 2021 20:58
 Operator : CG/JU
 Sample : M2528-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARK5

Manual Integrations
 APPROVED

mohammad
 6/2/2021 10:53:44 AM

Quant Time: Jun 02 01:11:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 02 01:10:46 2021
 Response via : Initial Calibration

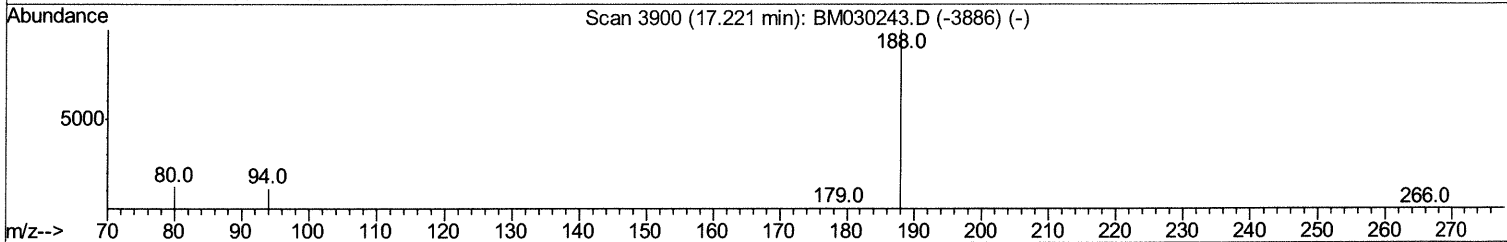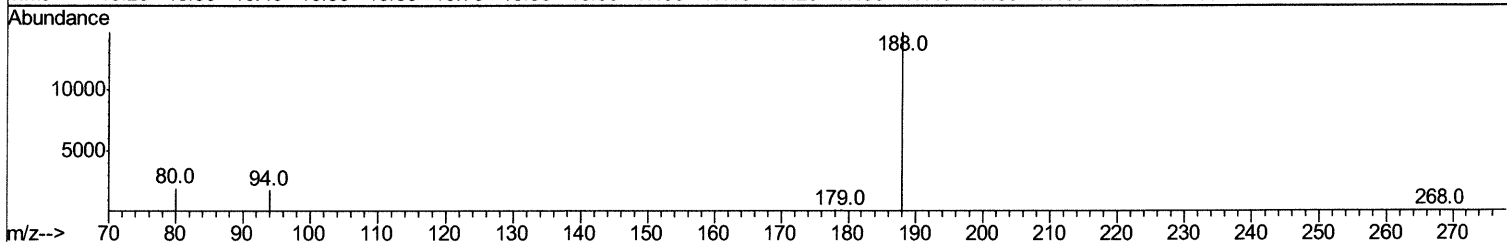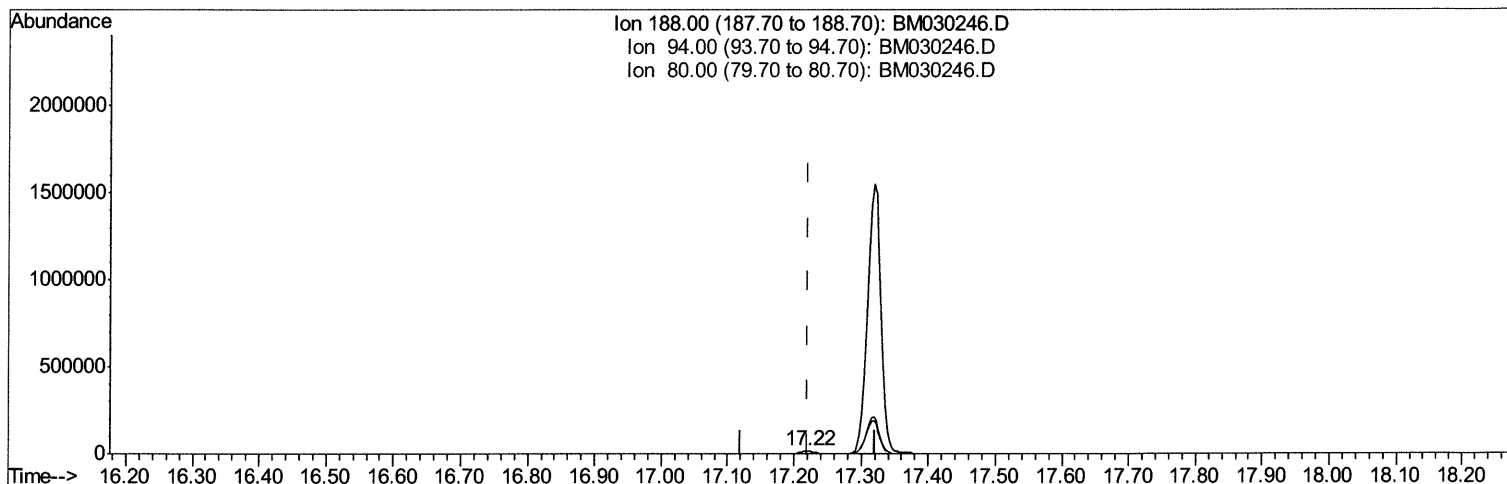

TIC: BM030246.D

(13) Phenanthrene-d10 (I)

17.221min (-0.000) 0.40ng/ul m 06/03/21 ju

response 20822

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	11.62
80.00	12.90	12.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
 Data File : BM030246.D
 Acq On : 01 Jun 2021 20:58
 Operator : CG/JU
 Sample : M2528-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARK5

Manual Integrations
 APPROVED

mohammad
 6/2/2021 10:53:44 AM

Quant Time: Jun 02 01:18:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 02 01:10:46 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	5638	0.40	ng/ul	0.00
4) Naphthalene-d8	10.65	136	20540	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.49	164	11981	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.22	188	20822m>	0.40	ng/ul>	0.00
17) Chrysene-d12	21.38	240	12927	0.40	ng/ul	0.00
23) Perylene-d12	23.66	264	13354	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.33	96	19003	3.44	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.24	152	11176	0.38	ng/ul	0.00
18) Fluoranthene-d10	19.24	212	22681	0.52	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.37	88	315	0.053	ng/ul#	65
14) Pentachlorophenol	16.87	266	634	0.098	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

06/03/21 JU