


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
Data File : BM030250.D
Acq On : 01 Jun 2021 23:23
Operator : CG/JU
Sample : M2528-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARK7

Manual Integrations
APPROVED

mohammad
6/2/2021 10:53:51 AM

Quant Time: Jun 02 01:26:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 02 01:10:46 2021
Response via : Initial Calibration

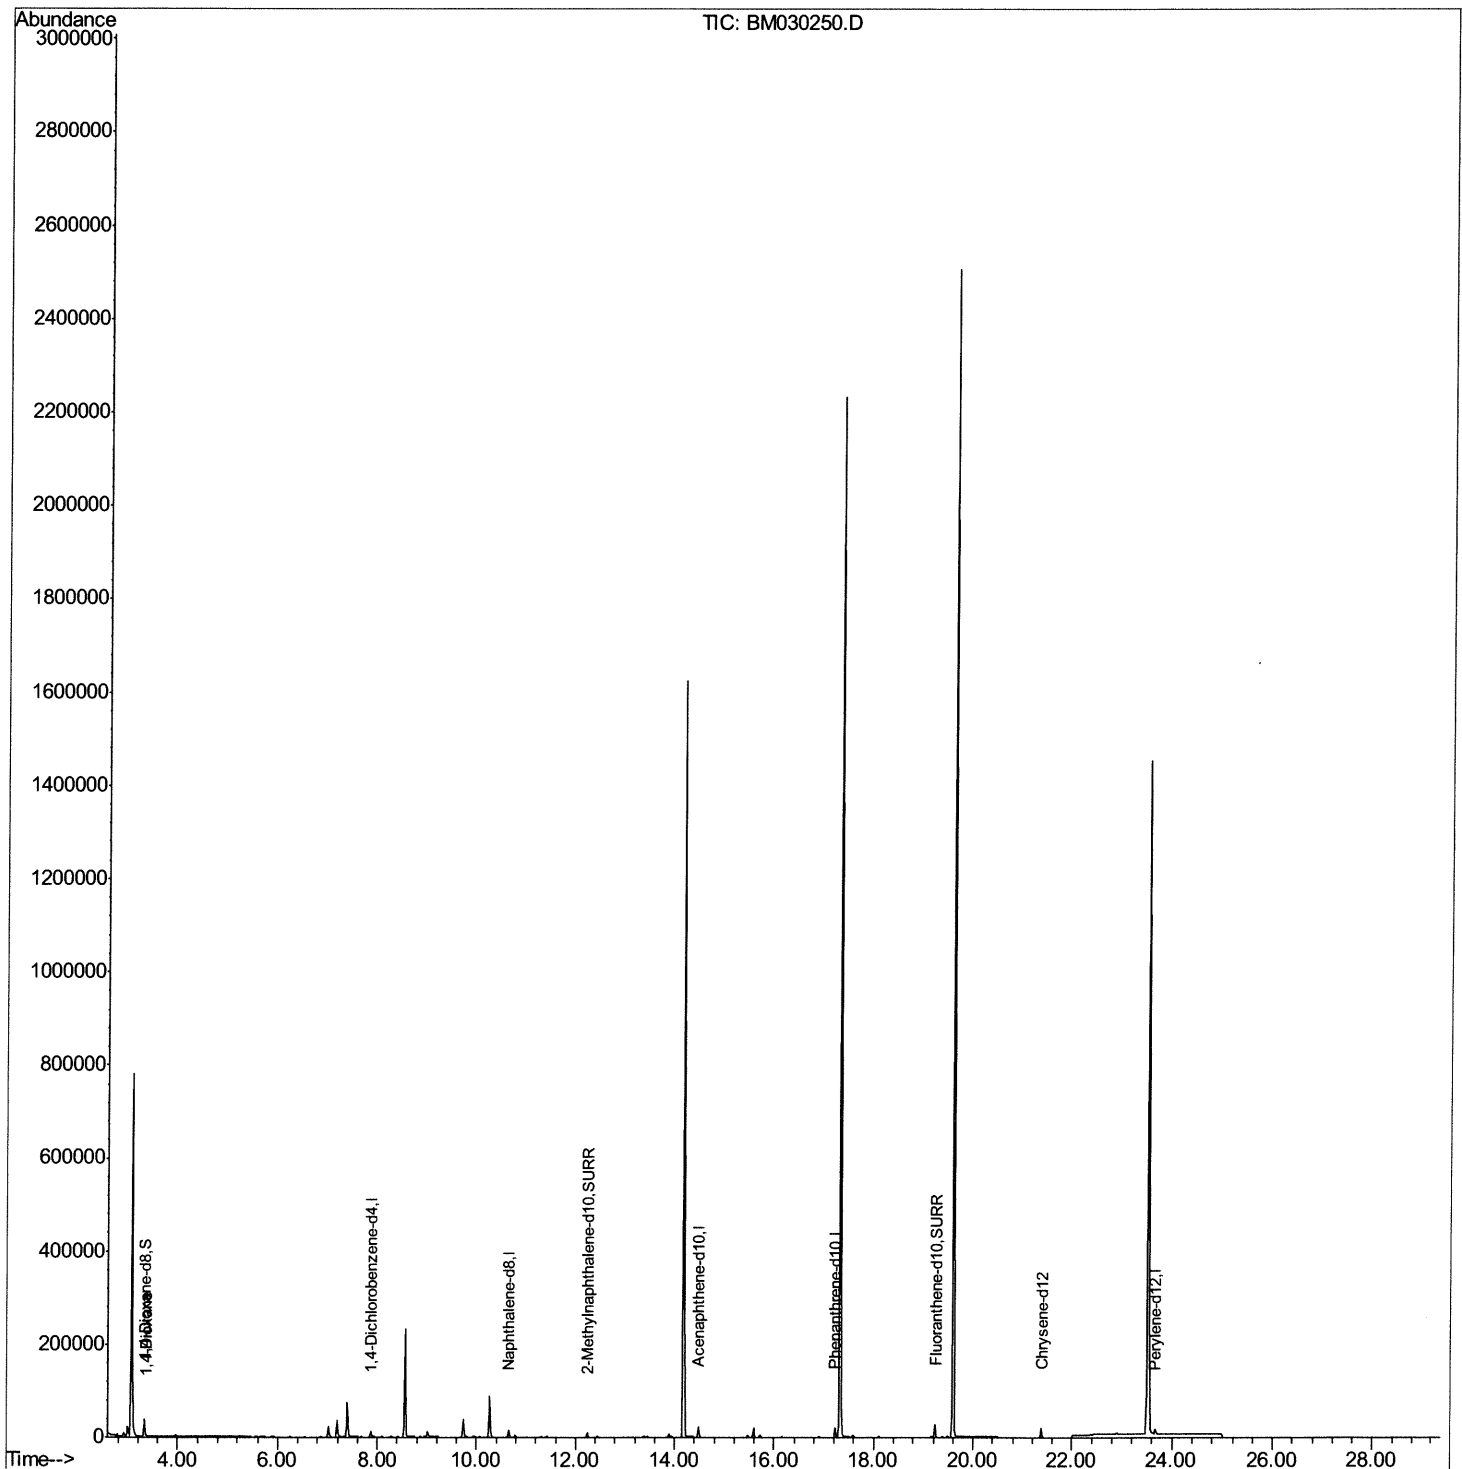

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
 Data File : BM030250.D
 Acq On : 01 Jun 2021 23:23
 Operator : CG/JU
 Sample : M2528-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARK7

Manual Integrations
 APPROVED

mohammad
 6/2/2021 10:53:51 AM

Quant Time: Jun 02 01:11:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 02 01:10:46 2021
 Response via : Initial Calibration

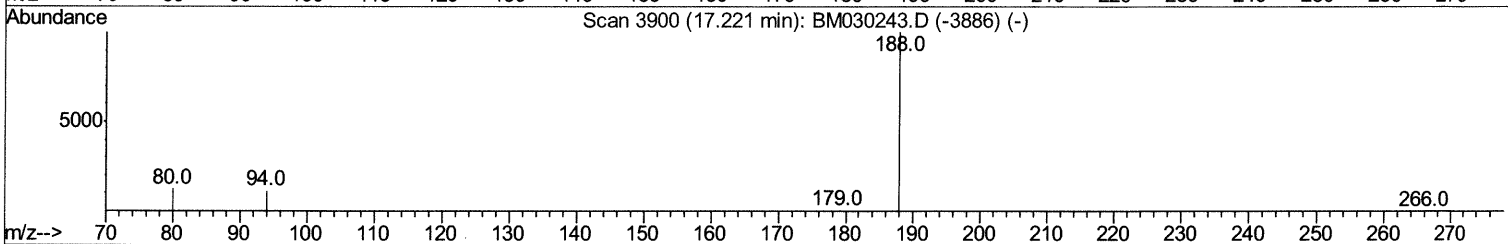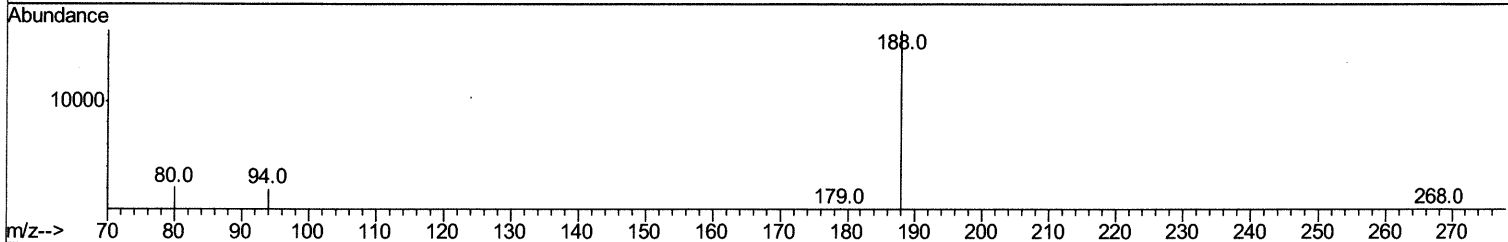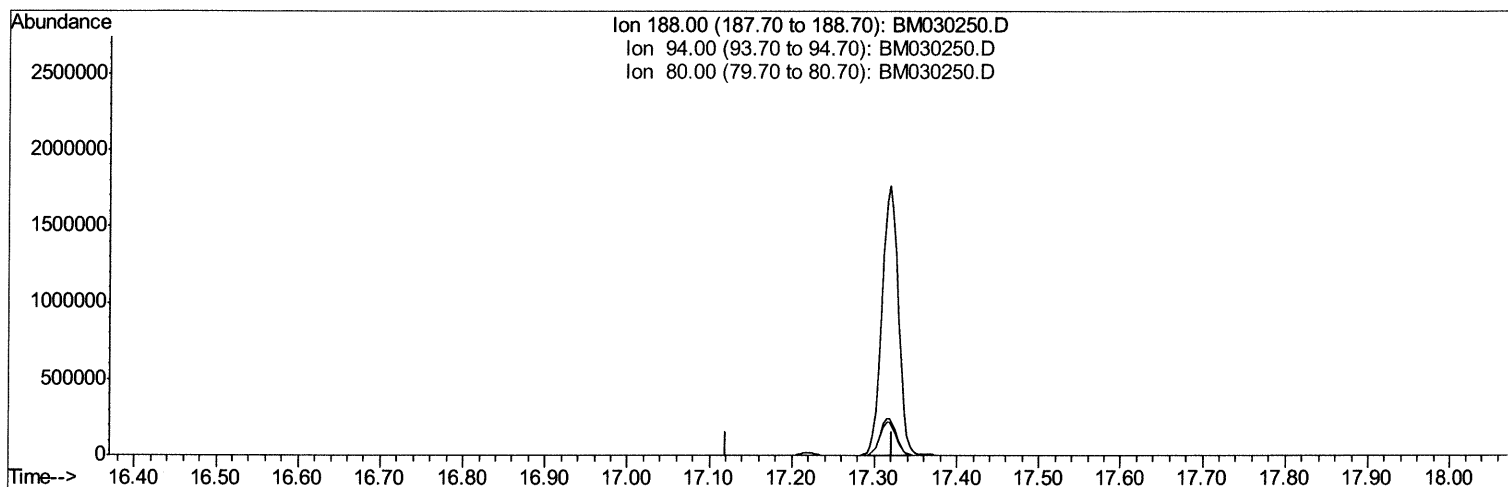

TIC: BM030250.D

(13) Phenanthrene-d10 (I)

17.221min (-17.221) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.80	0.00#
80.00	12.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
Data File : BM030250.D
Acq On : 01 Jun 2021 23:23
Operator : CG/JU
Sample : M2528-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARK7

Manual Integrations
APPROVED

mohammad
6/2/2021 10:53:51 AM

Quant Time: Jun 02 01:11:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 02 01:10:46 2021
Response via : Initial Calibration

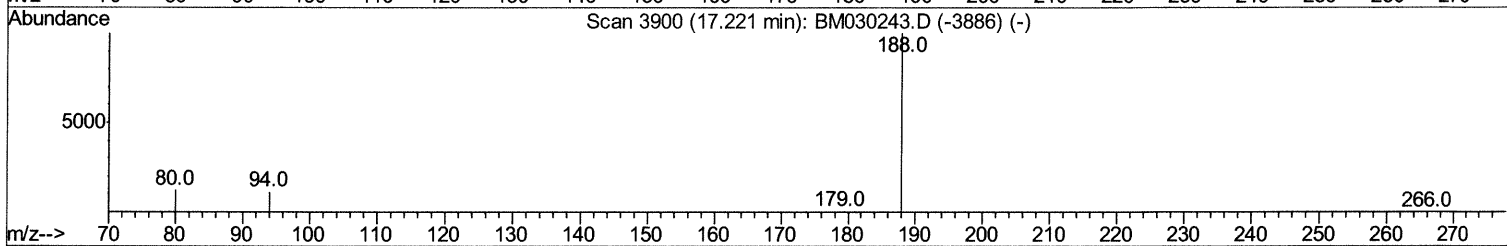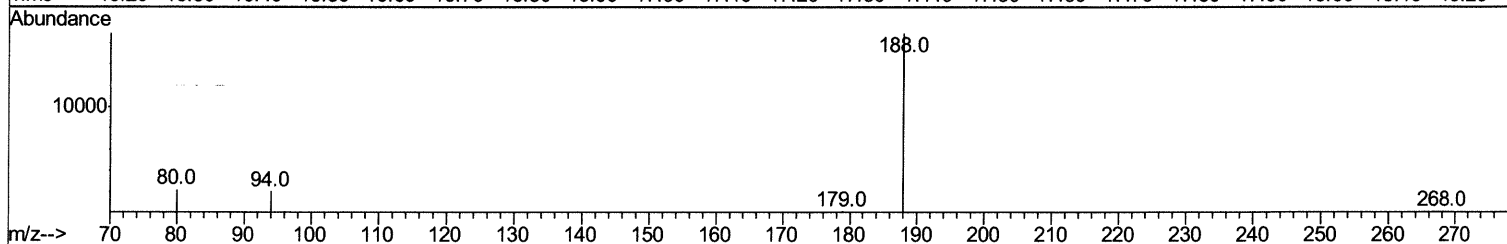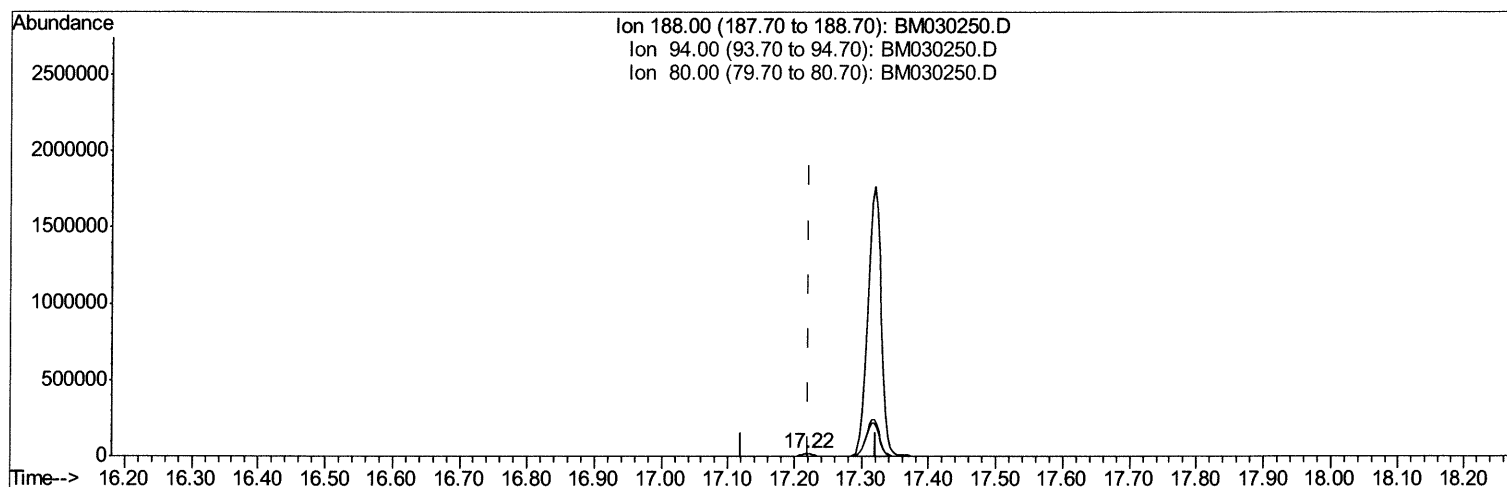

TIC: BM030250.D

(13) Phenanthrene-d10 (I)

17.218min (-0.004) 0.40ng/ul m 6/03/21 JU

response 23695

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	11.71
80.00	12.90	12.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
 Data File : BM030250.D
 Acq On : 01 Jun 2021 23:23
 Operator : CG/JU
 Sample : M2528-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARK7

Manual Integrations
 APPROVED

mohammad
 6/2/2021 10:53:51 AM

Quant Time: Jun 02 01:26:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 02 01:10:46 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	5790	0.40	ng/ul	0.00
4) Naphthalene-d8	10.65	136	21129	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.49	164	12712	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.22	188	23695m>	0.40	ng/ul>	0.00
17) Chrysene-d12	21.38	240	16219	0.40	ng/ul	0.00
23) Perylene-d12	23.66	264	15859	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.33	96	22899	4.03	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.24	152	12308	0.41	ng/ul	0.00
18) Fluoranthene-d10	19.24	212	27871	0.51	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.37	88	248	0.040	ng/ul#	63

(#) = qualifier out of range (m) = manual integration (+) = signals summed