


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
Data File : BM030254.D
Acq On : 02 Jun 2021 11:23
Operator : CG/JU
Sample : M2528-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARK8

Manual Integrations
APPROVED

mohammad
6/2/2021 5:18:42 PM

Quant Time: Jun 02 11:55:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 02 02:39:12 2021
Response via : Initial Calibration

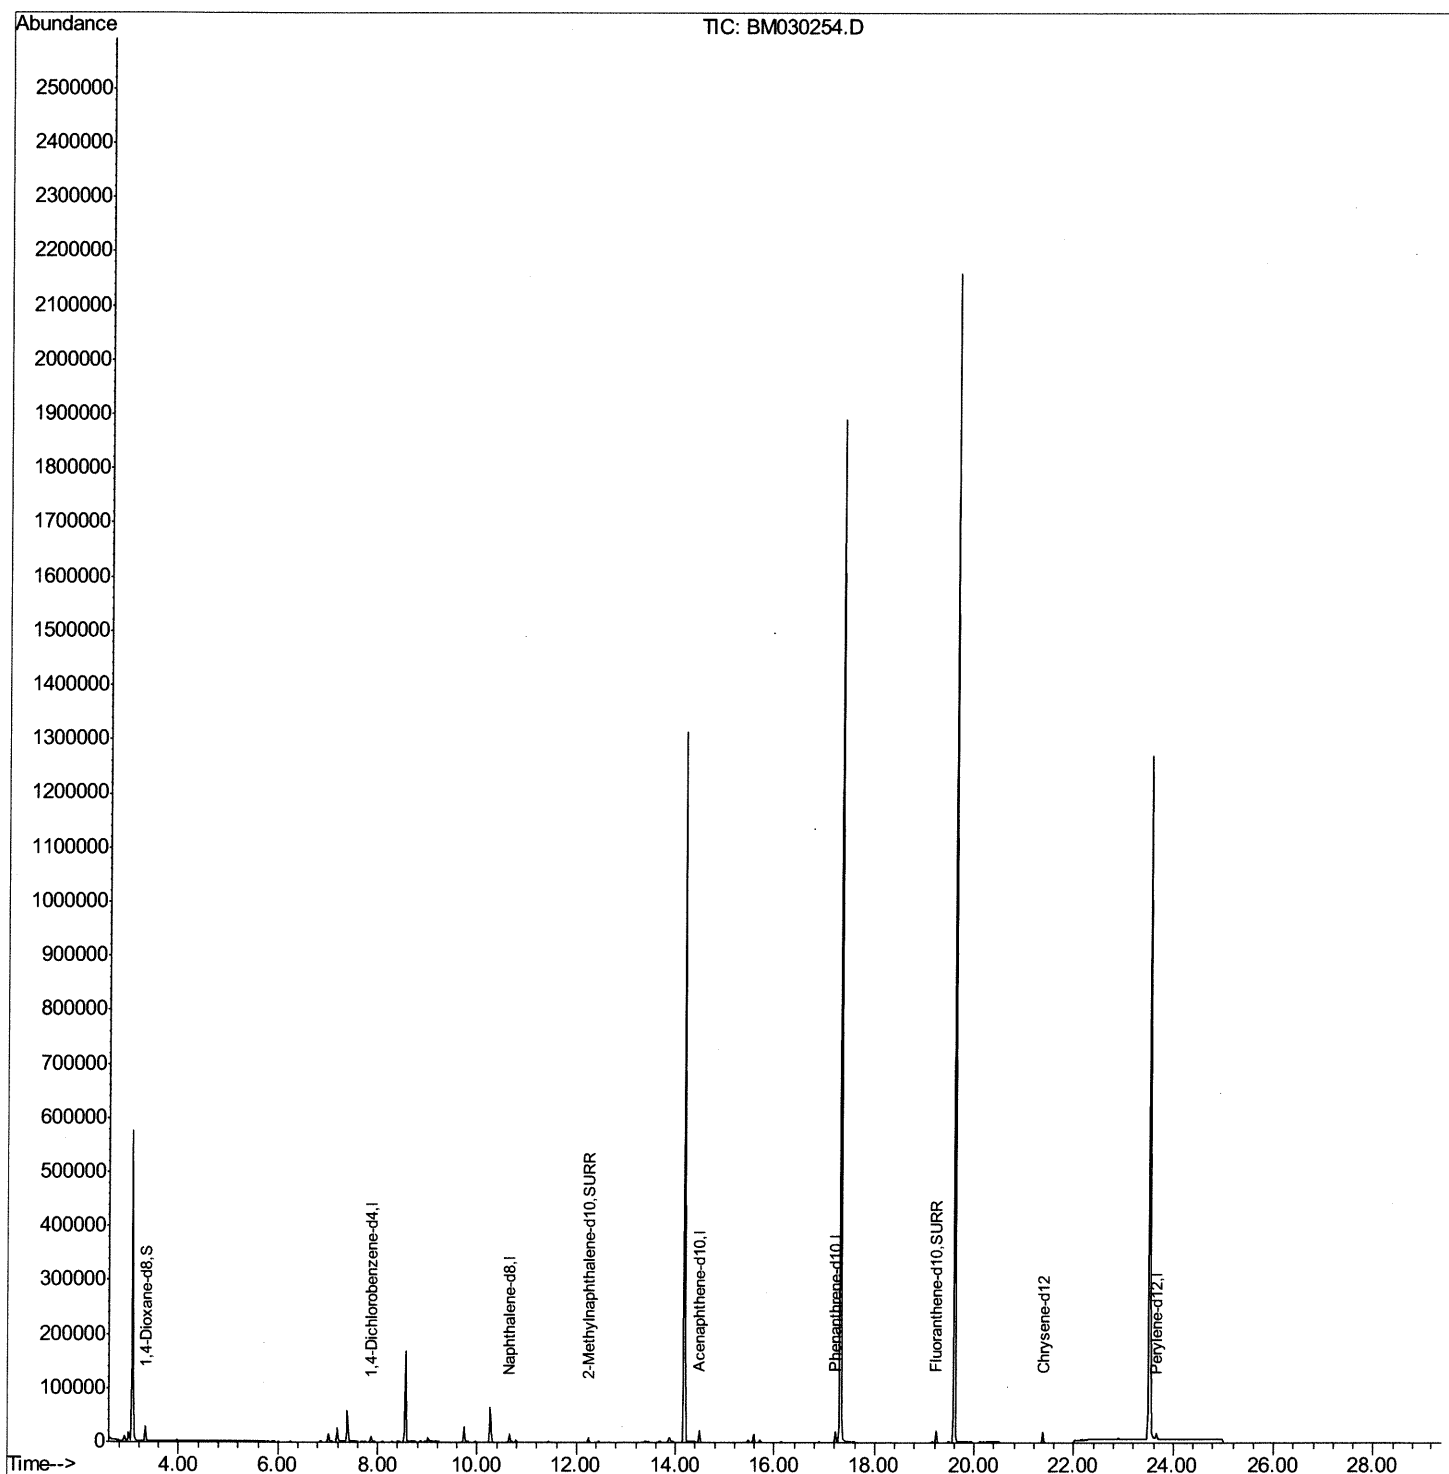

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
Data File : BM030254.D
Acq On : 02 Jun 2021 11:23
Operator : CG/JU
Sample : M2528-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARK8

Manual Integrations
APPROVED

mohammad
6/2/2021 5:18:42 PM

Quant Time: Jun 02 11:54:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 02 02:39:12 2021
Response via : Initial Calibration

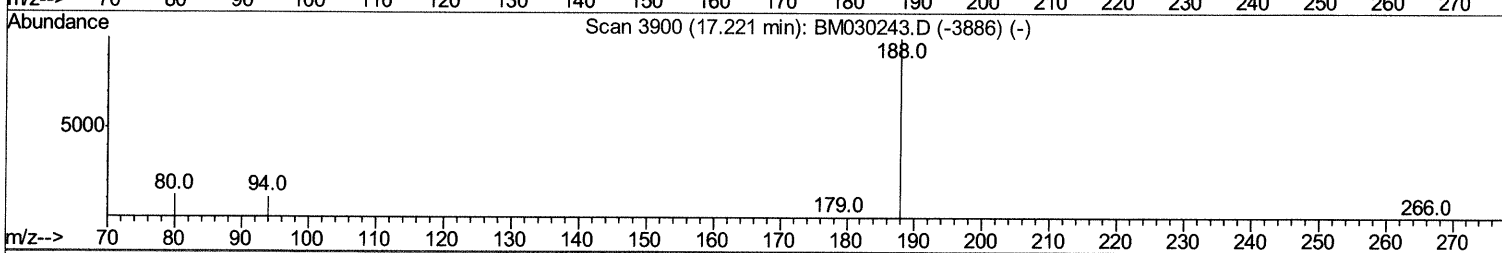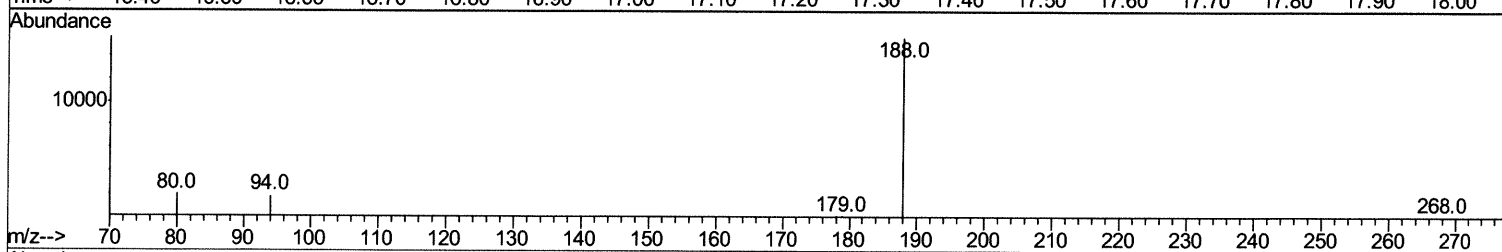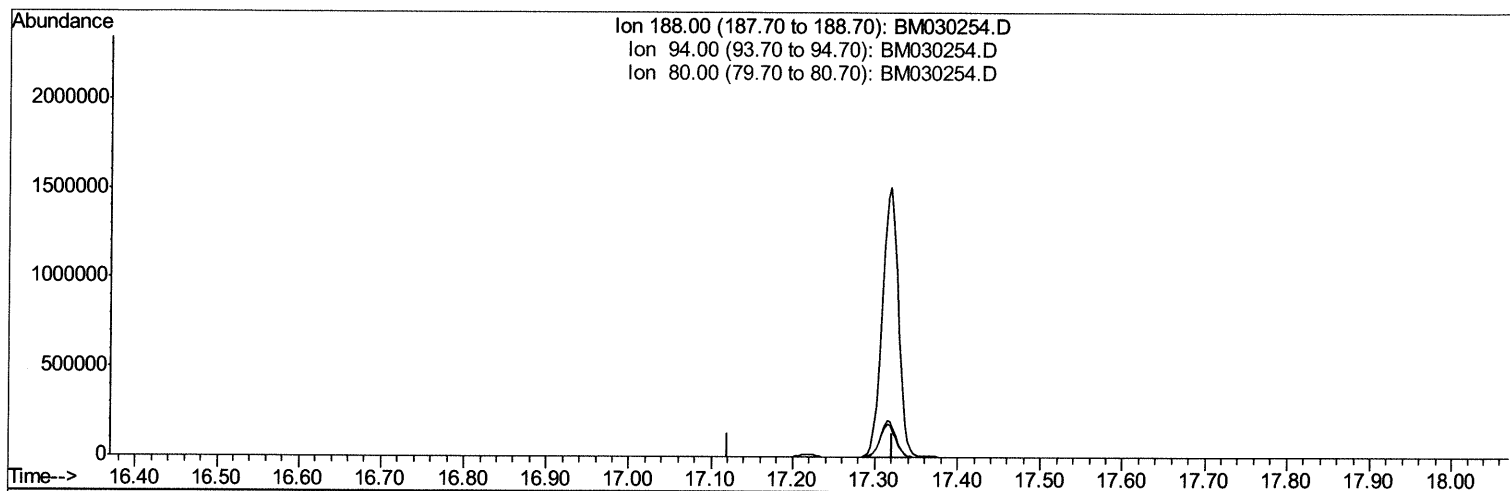

TIC: BM030254.D

(13) Phenanthrene-d10 (I)

17.221min (-17.221) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.80	0.00#
80.00	12.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
 Data File : BM030254.D
 Acq On : 02 Jun 2021 11:23
 Operator : CG/JU
 Sample : M2528-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARK8

Manual Integrations
 APPROVED

mohammad
 6/2/2021 5:18:42 PM

Quant Time: Jun 02 11:54:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 02 02:39:12 2021
 Response via : Initial Calibration

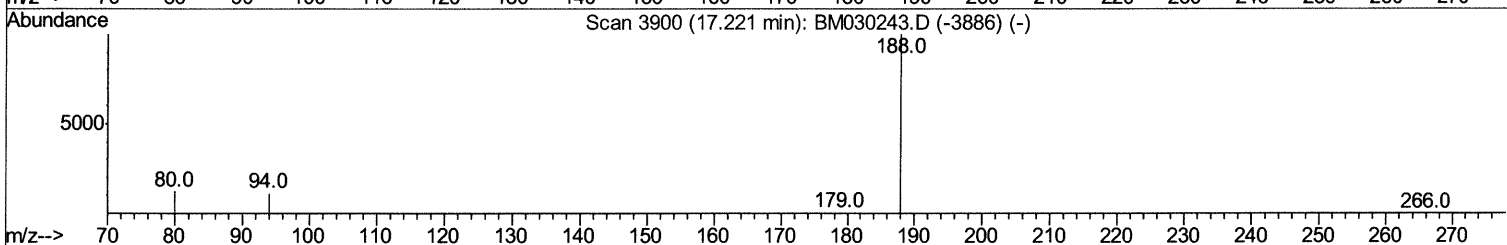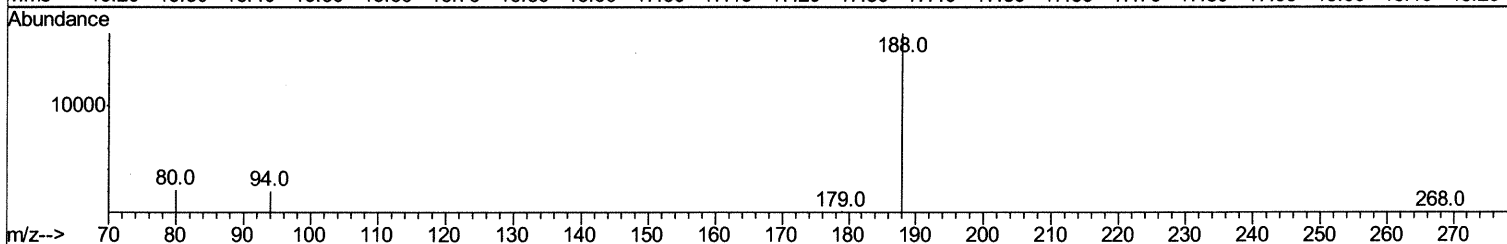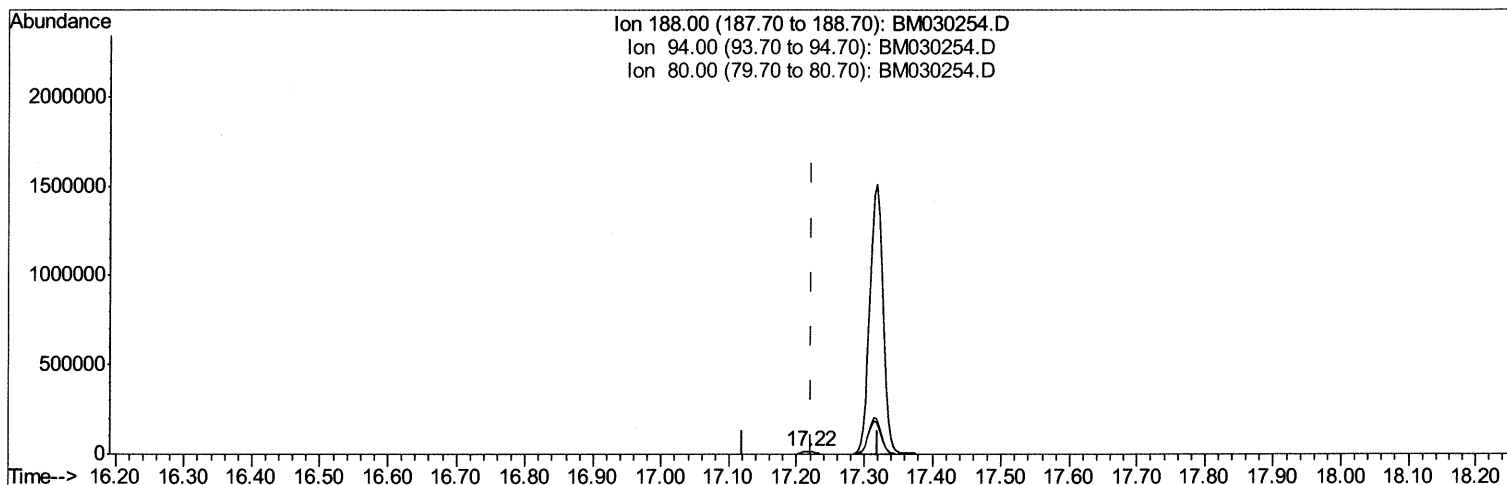

TIC: BM030254.D

(13) Phenanthrene-d10 (I)

17.218min (-0.004) 0.40ng/ul m 06/03/21 JU

response 23040

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	11.96
80.00	12.90	12.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060121\
 Data File : BM030254.D
 Acq On : 02 Jun 2021 11:23
 Operator : CG/JU
 Sample : M2528-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARK8

Manual Integrations
 APPROVED

mohammad
 6/2/2021 5:18:42 PM

Quant Time: Jun 02 11:55:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 02 02:39:12 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	5168	0.40	ng/ul	0.00
4) Naphthalene-d8	10.65	136	19265	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.49	164	12054	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.22	188	23040m >	0.40	ng/ul >	0.00
17) Chrysene-d12	21.38	240	16102	0.40	ng/ul	0.00
23) Perylene-d12	23.66	264	15589	0.40	ng/ul	0.00

66103/2150

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	16896	3.33	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.24	152	9761	0.35	ng/ul	0.00
18) Fluoranthene-d10	19.23	212	23027	0.43	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed