

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060121\
 Data File : BM030250.D
 Acq On : 01 Jun 2021 23:23
 Operator : CG/JU
 Sample : M2528-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARK7

Manual Integrations
 APPROVED

mohammad
 6/2/2021 10:53:51 AM

Quant Time: Jun 02 01:11:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 02 01:10:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.867	152	5790	0.40	ng/ul	0.00
4) Naphthalene-d8	10.653	136	21129	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.485	164	12712	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.218	188	23695m	0.40	ng/ul	0.00
17) Chrysene-d12	21.377	240	16219	0.40	ng/ul	0.00
23) Perylene-d12	23.660	264	15859	0.40	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.331	96	22899	4.03	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.241	152	12308	0.41	ng/ul	0.00
18) Fluoranthene-d10	19.237	212	27871	0.51	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.369	88	248	0.04	ng/ul#	63

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060121\
Data File : BM030250.D
Acq On : 01 Jun 2021 23:23
Operator : CG/JU
Sample : M2528-05
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
YARK7

Manual Integrations
APPROVED


mohammad
6/2/2021 10:53:51 AM

Quant Time: Jun 02 01:11:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 02 01:10:46 2021
Response via : Initial Calibration

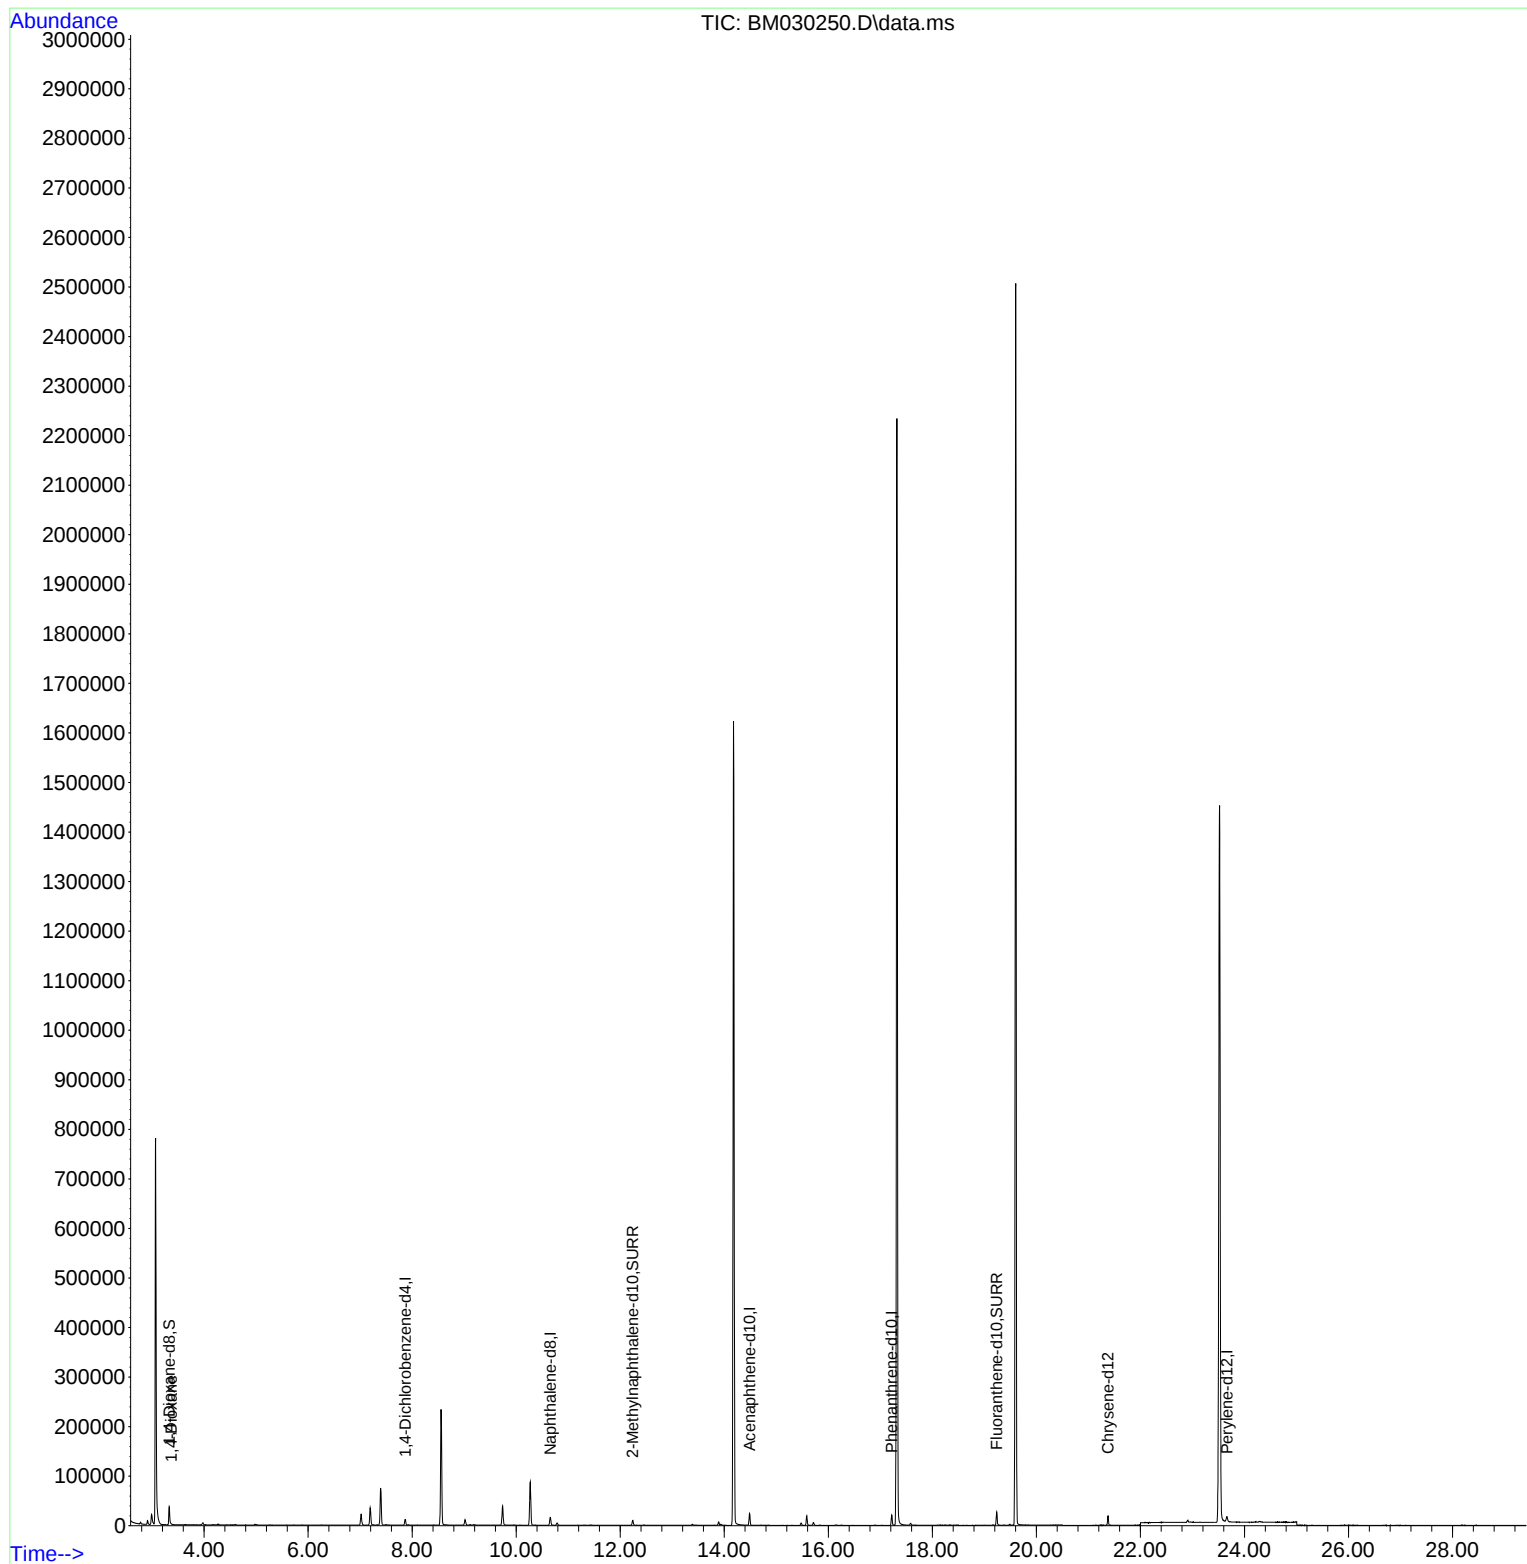


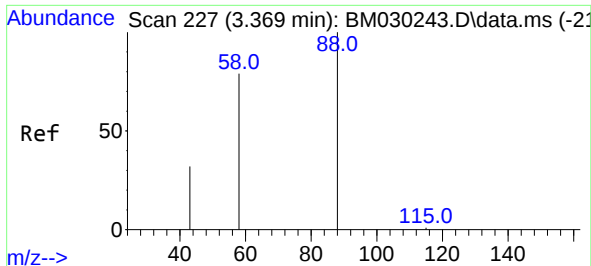


#2
1,4-Dioxane
Concen: 0.04 ng/ul
RT: 3.369 min Scan# 227
Delta R.T. -0.000 min
Lab File: BM030250.D
Acq: 01 Jun 2021 23:23

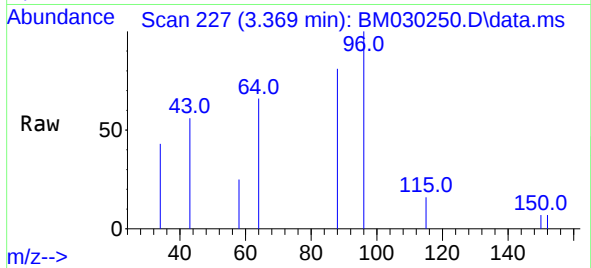

Tgt Ion: 88 Resp: 248

Ion	Ratio	Lower	Upper
88	100		
43	69.0	38.2	57.4#
58	30.9	49.8	74.8#

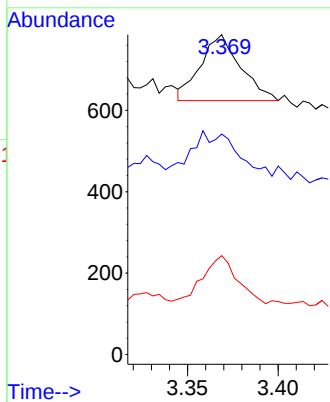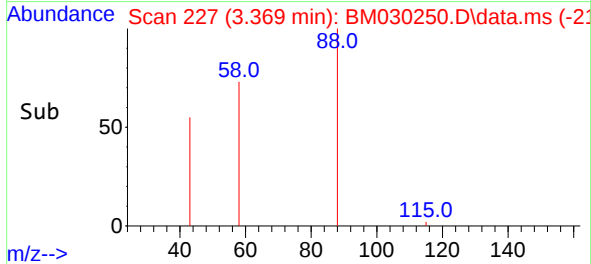

Instrument :
BNA_M
ClientSampleId :
YARK7

Manual Integrations
APPROVED

mohammad
6/2/2021 10:53:51 AM