
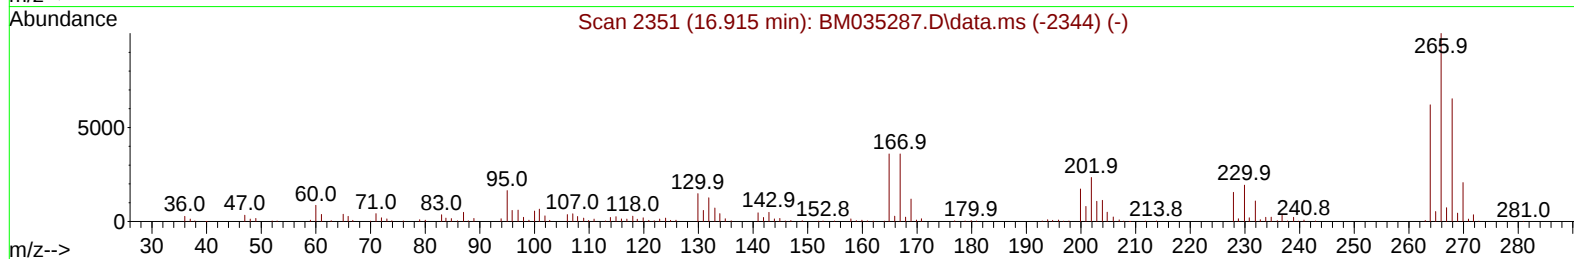
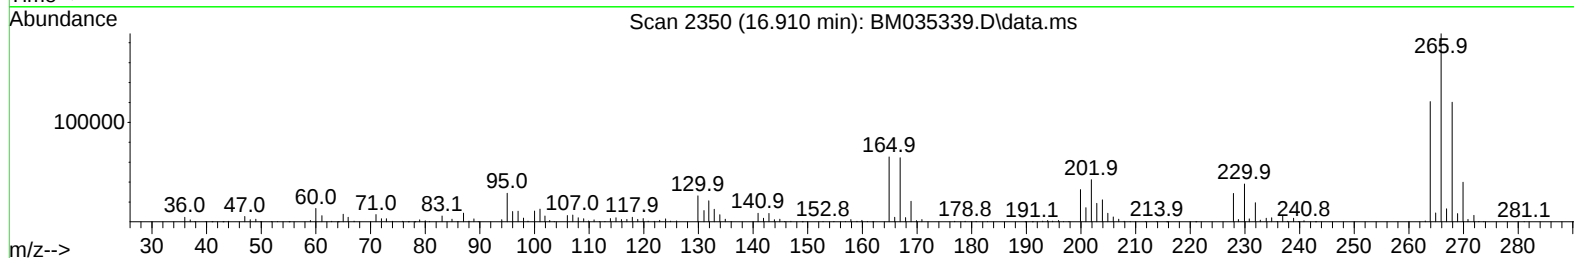


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060122\
Data File : BM035339.D
Acq On : 01 Jun 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 06:06:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 31 15:35:47 2022
Response via : Initial Calibration

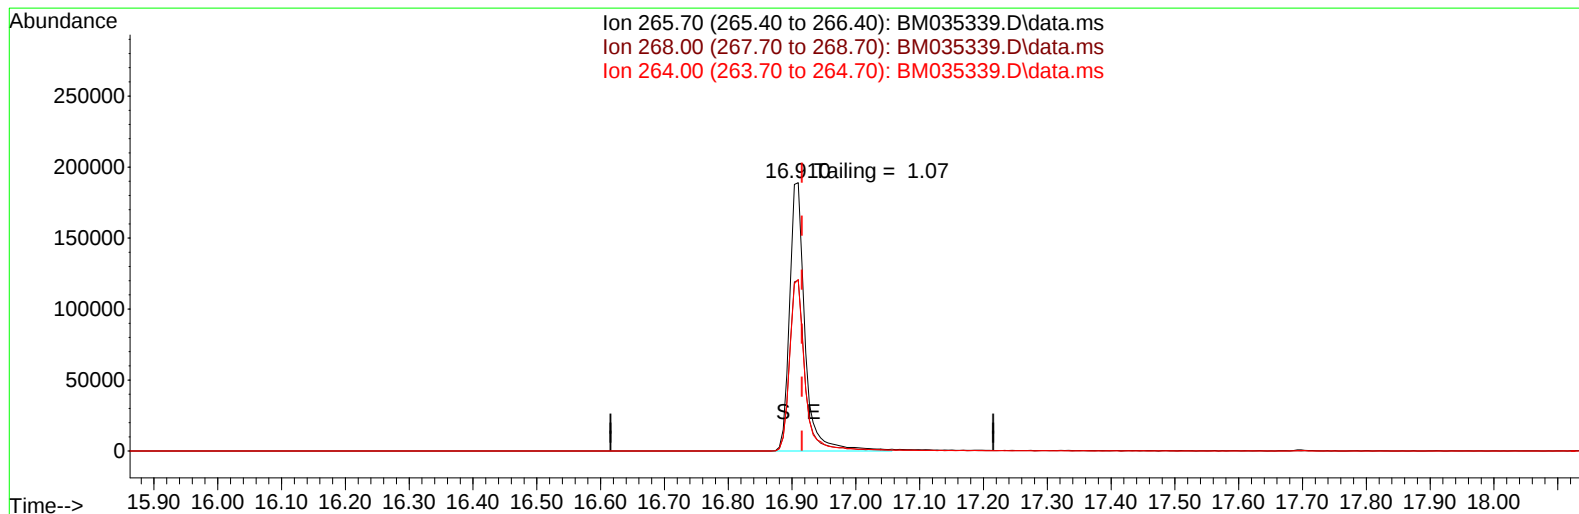

TIC: BM035339.D\data.ms

(70) Pentachlorophenol (C)




16.910min (-0.006) 0.00 ng

response 321403

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.61
264.00	63.30	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060122\
 Data File : BM035339.D
 Acq On : 01 Jun 2022 10:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 06:06:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 31 15:35:47 2022
 Response via : Initial Calibration

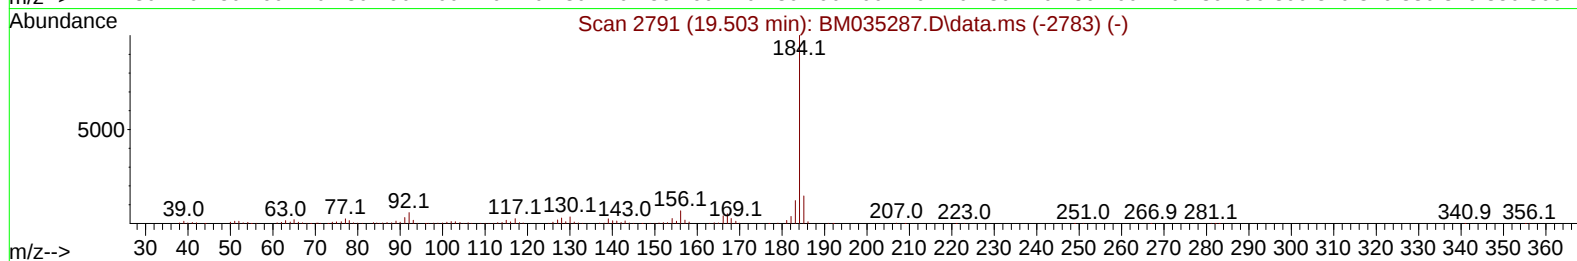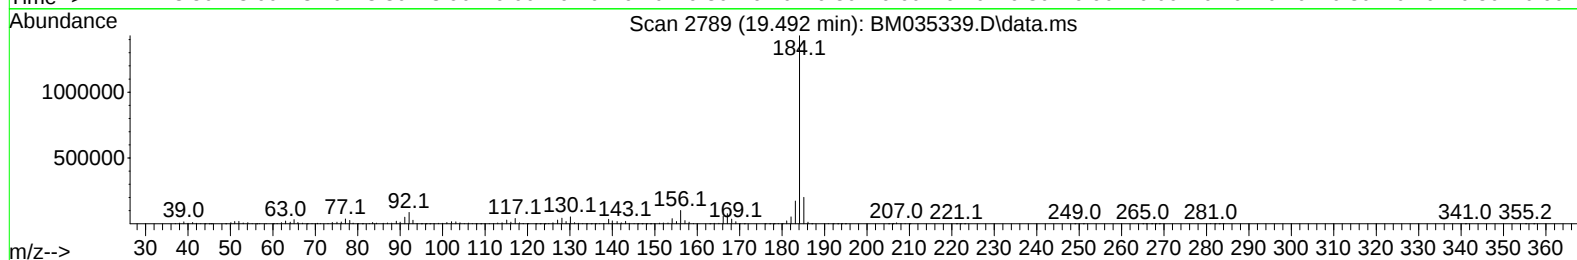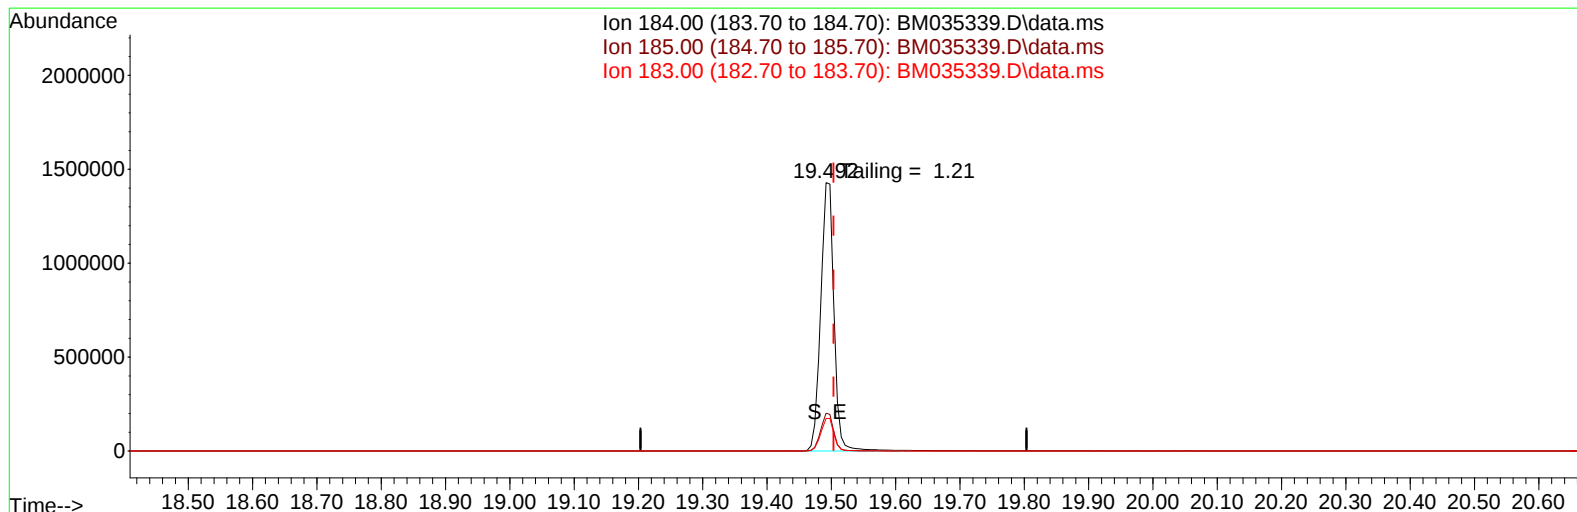

TIC: BM035339.D\data.ms

(77) Benzidine**19.492min (-0.012) 355263.06 ng****response 2058206**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.09
183.00	11.90	12.14
0.00	0.00	0.00