

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060122\
 Data File : BM035341.D
 Acq On : 01 Jun 2022 11:29
 Operator : CG/JU
 Sample : PB145220BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145220BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	395	402	421	rBV	1776746	2611301	30.96%	8.292%
2	7.046	666	673	695	rBV	1662350	2674722	31.71%	8.494%
3	7.863	806	812	826	rVB	335269	531220	6.30%	1.687%
4	9.022	1002	1009	1026	rBV	1016292	1737787	20.60%	5.519%
5	10.663	1281	1288	1306	rBV	424457	739824	8.77%	2.349%
6	13.127	1700	1707	1721	rBV	3294248	4867439	57.71%	15.457%
7	14.504	1933	1941	1956	rBV	750466	1111463	13.18%	3.530%
8	15.992	2187	2194	2218	rBV	2633141	3993768	47.35%	12.683%
9	17.245	2401	2407	2417	rBV	975384	1396689	16.56%	4.435%
10	19.874	2848	2854	2863	rBV	6744072	8434437	100.00%	26.784%
11	21.433	3114	3119	3131	rBV	1351147	1744399	20.68%	5.540%
12	23.797	3515	3521	3530	rVB2	792643	1647000	19.53%	5.230%




Sum of corrected areas: 31490049

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060122\
Data File : BM035341.D
Acq On : 01 Jun 2022 11:29
Operator : CG/JU
Sample : PB145220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

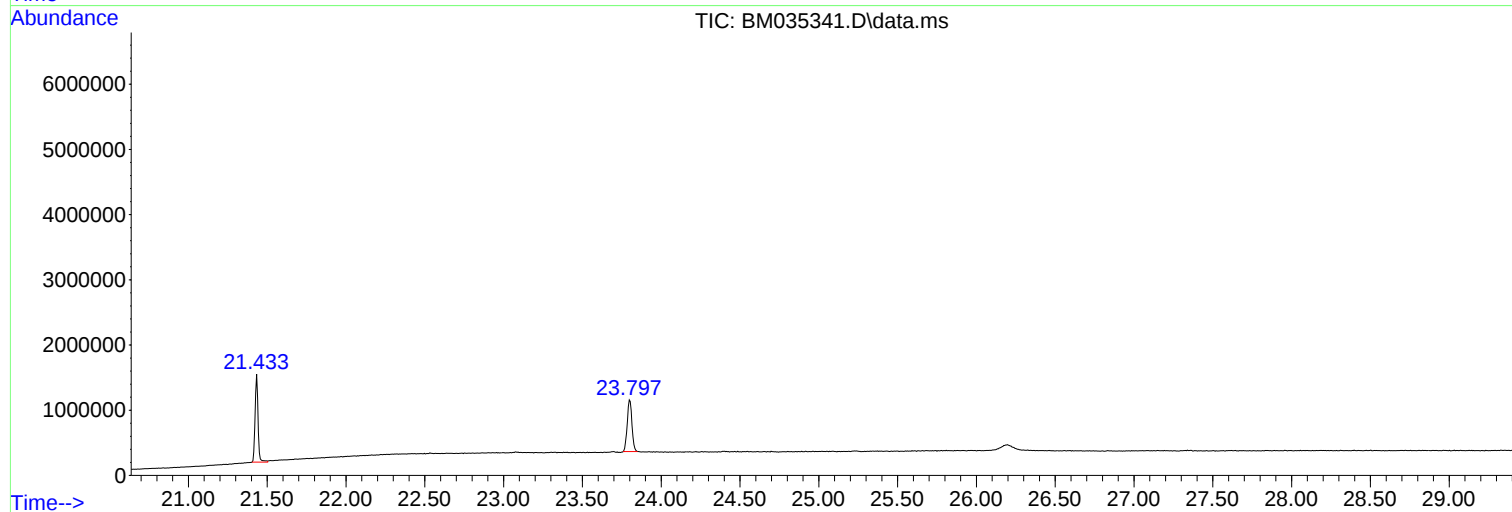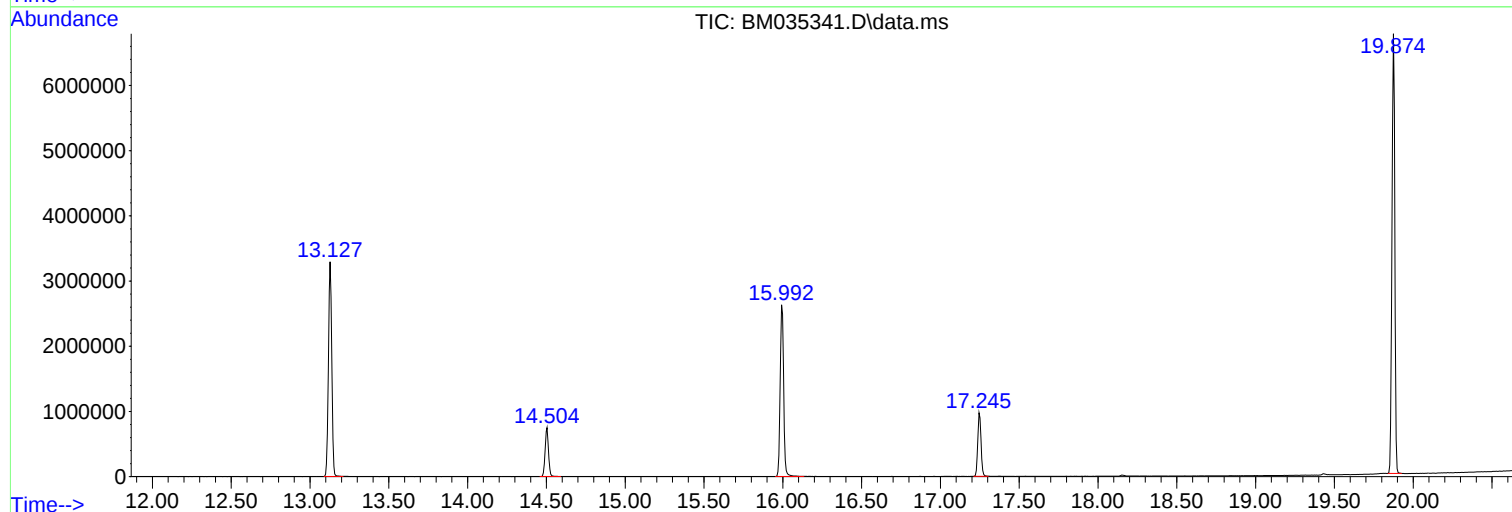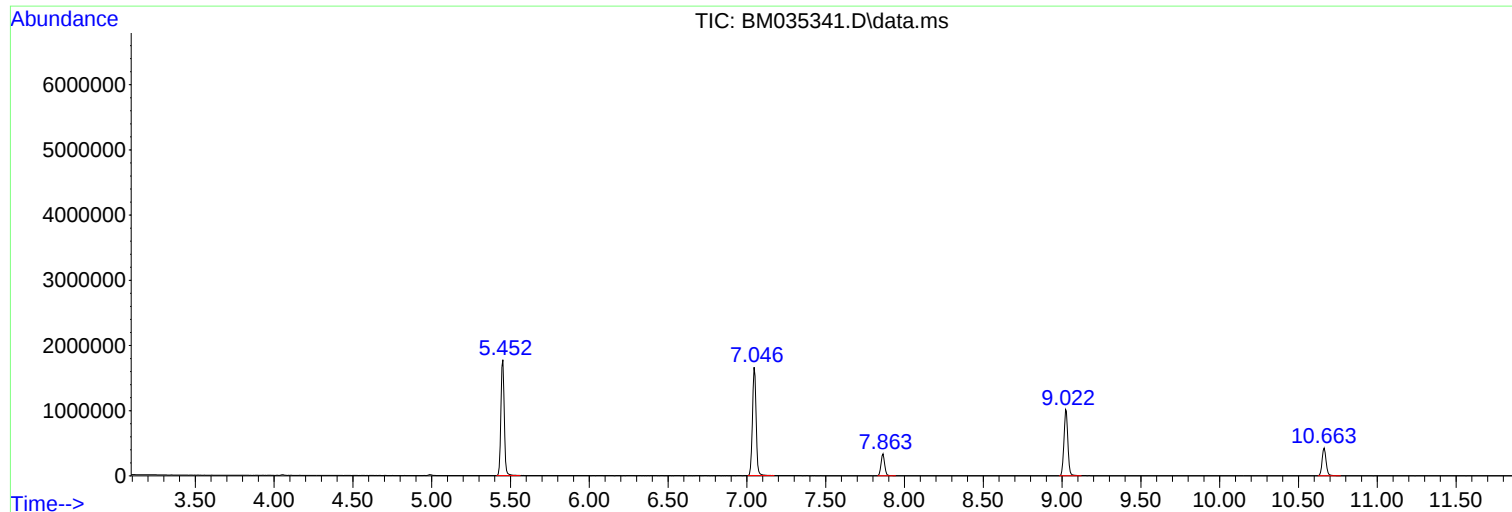

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060122\
Data File : BM035341.D
Acq On : 01 Jun 2022 11:29
Operator : CG/JU
Sample : PB145220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060122\
Data File : BM035341.D
Acq On : 01 Jun 2022 11:29
Operator : CG/JU
Sample : PB145220BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------