
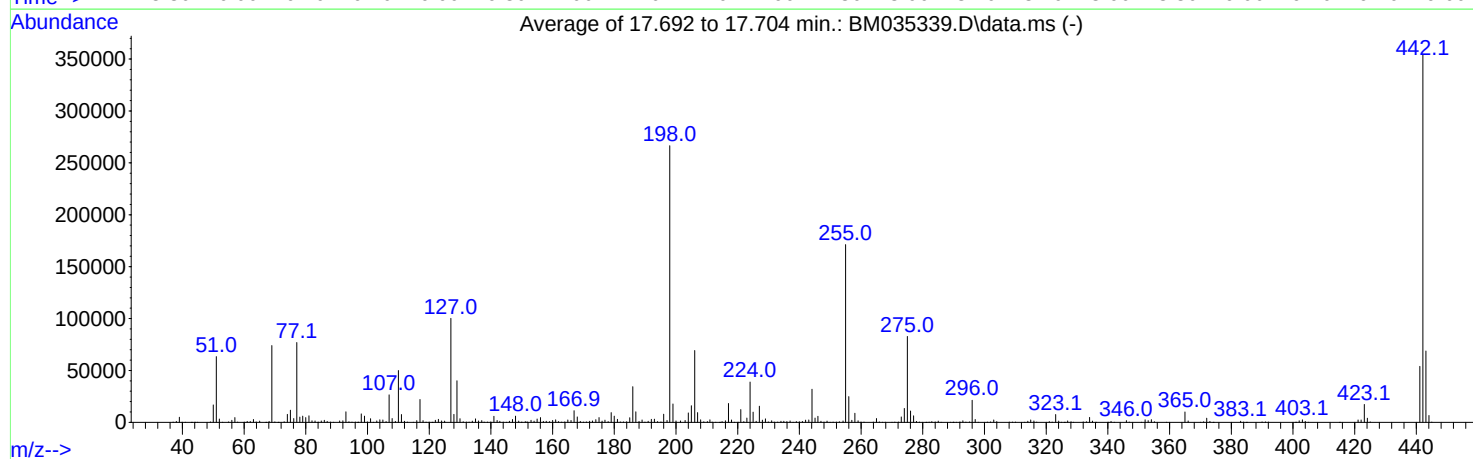


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060122\
 Data File : BM035339.D
 Acq On : 01 Jun 2022 10:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 31 15:35:47 2022

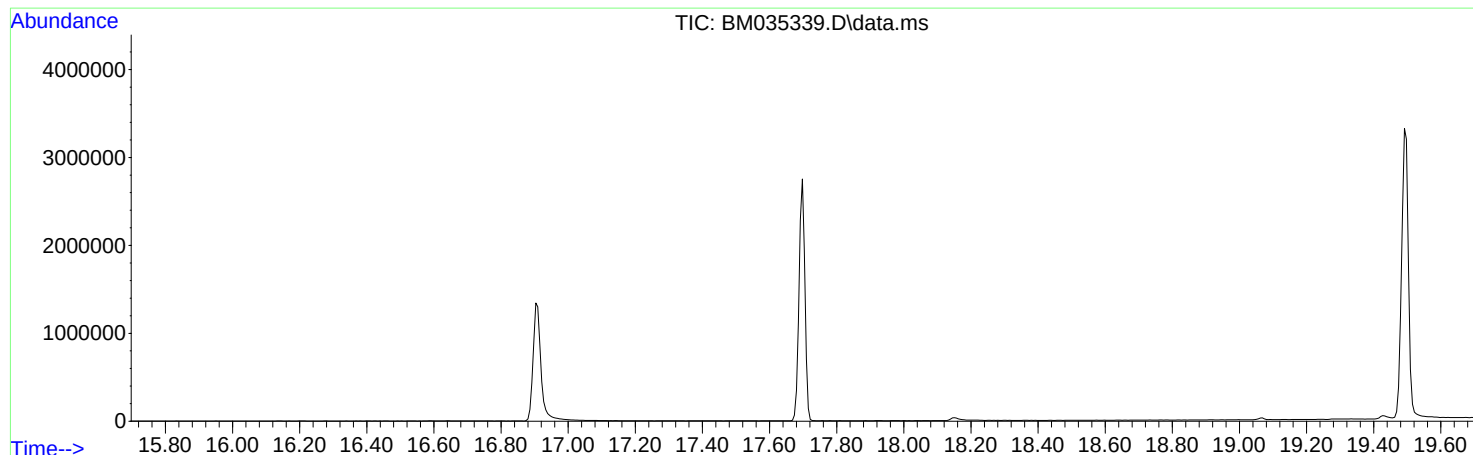




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.8	63347	PASS
68	69	0.00	2	1.3	939	PASS
69	198	0.00	100	27.8	74024	PASS
70	69	0.00	2	0.6	472	PASS
127	198	10	80	37.6	100187	PASS
197	198	0.00	2	0.7	1847	PASS
198	198	100	100	100.0	266539	PASS
199	198	5	9	6.7	17769	PASS
275	198	10	60	31.0	82741	PASS
365	198	1	100	3.8	10072	PASS
441	198	0.01	100	20.2	53907	PASS
442	442	50	100	100.0	354389	PASS
443	442	15	24	19.4	68827	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060122\
 Data File : BM035339.D
 Acq On : 01 Jun 2022 10:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 02 06:06:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 31 15:35:47 2022
 Response via : Initial Calibration

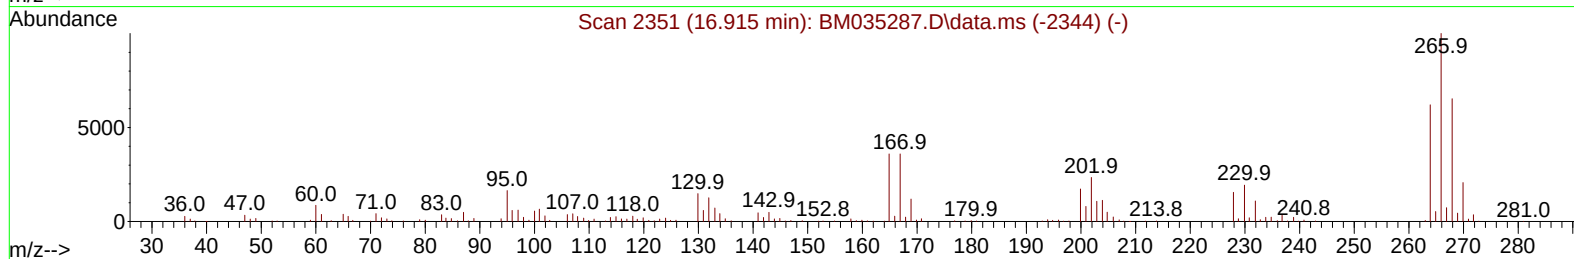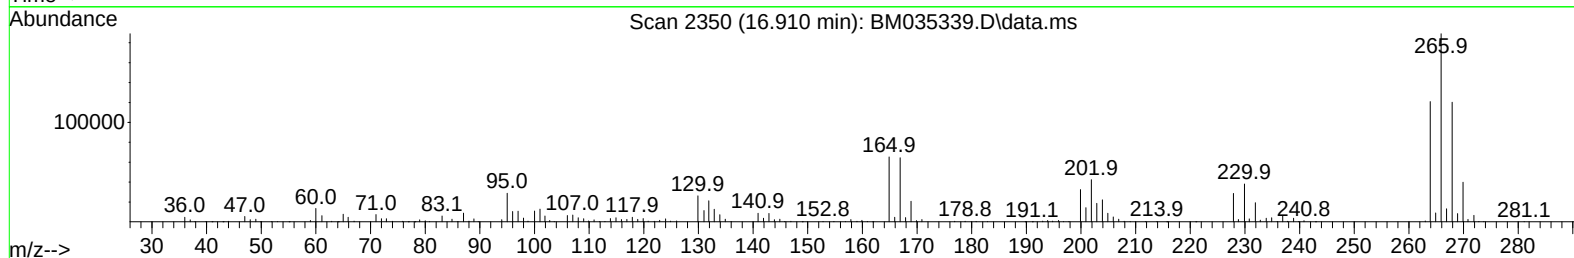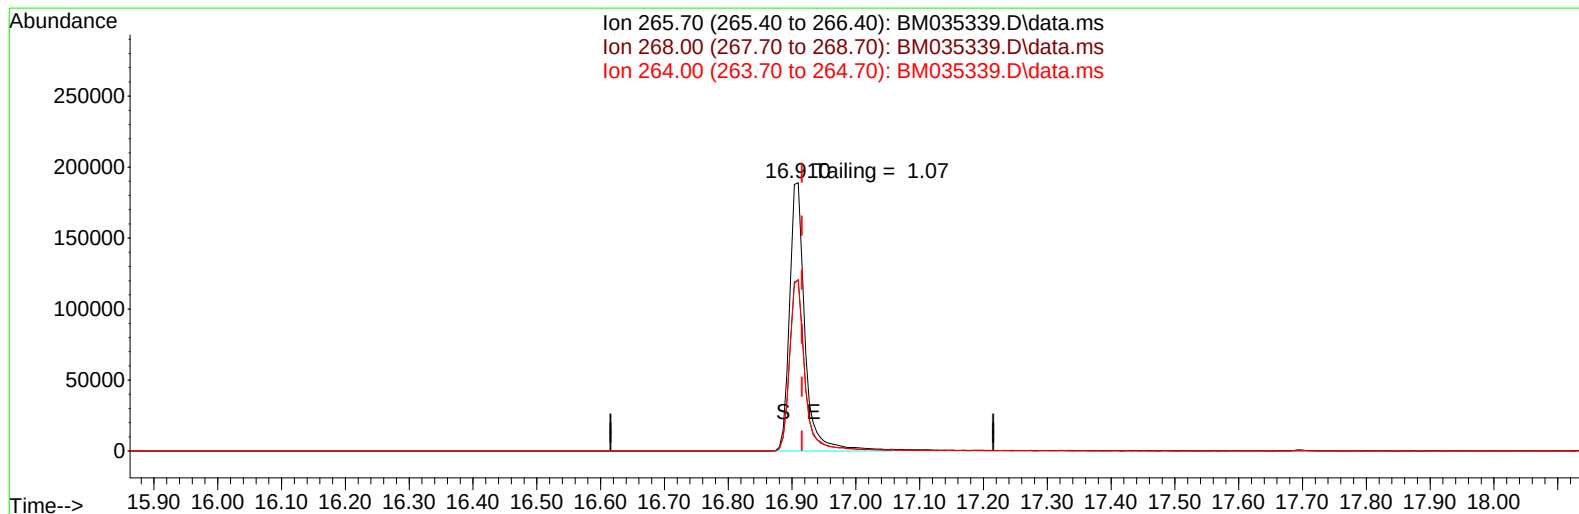

TIC: BM035339.D\data.ms

(70) Pentachlorophenol (C)

16.910min (-0.006) 0.00 ng




response 321403

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.61
264.00	63.30	63.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060122\
 Data File : BM035339.D
 Acq On : 01 Jun 2022 10:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 02 06:06:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM052722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 31 15:35:47 2022
 Response via : Initial Calibration

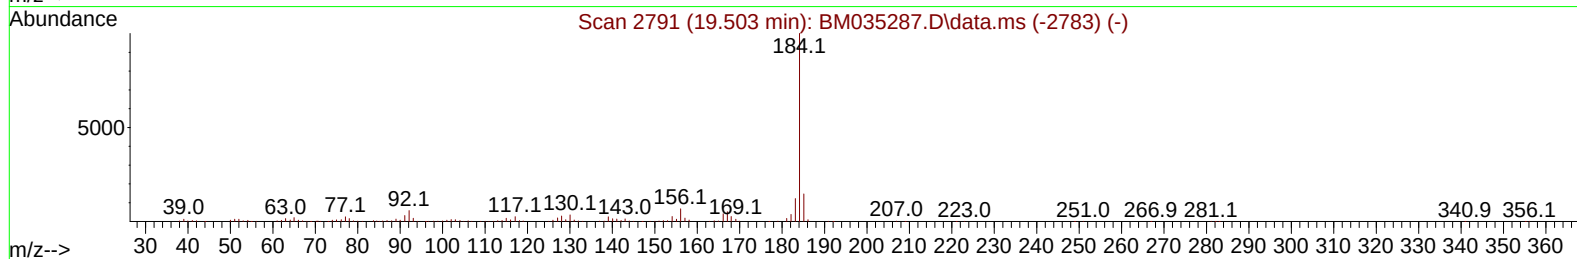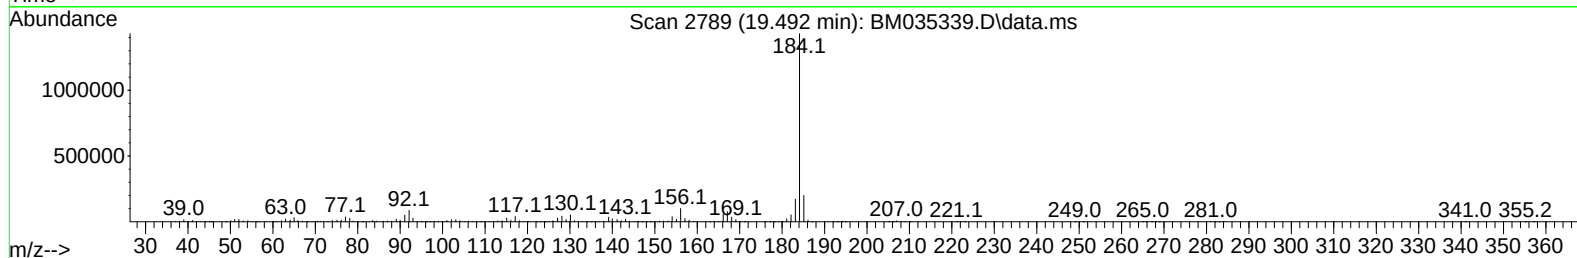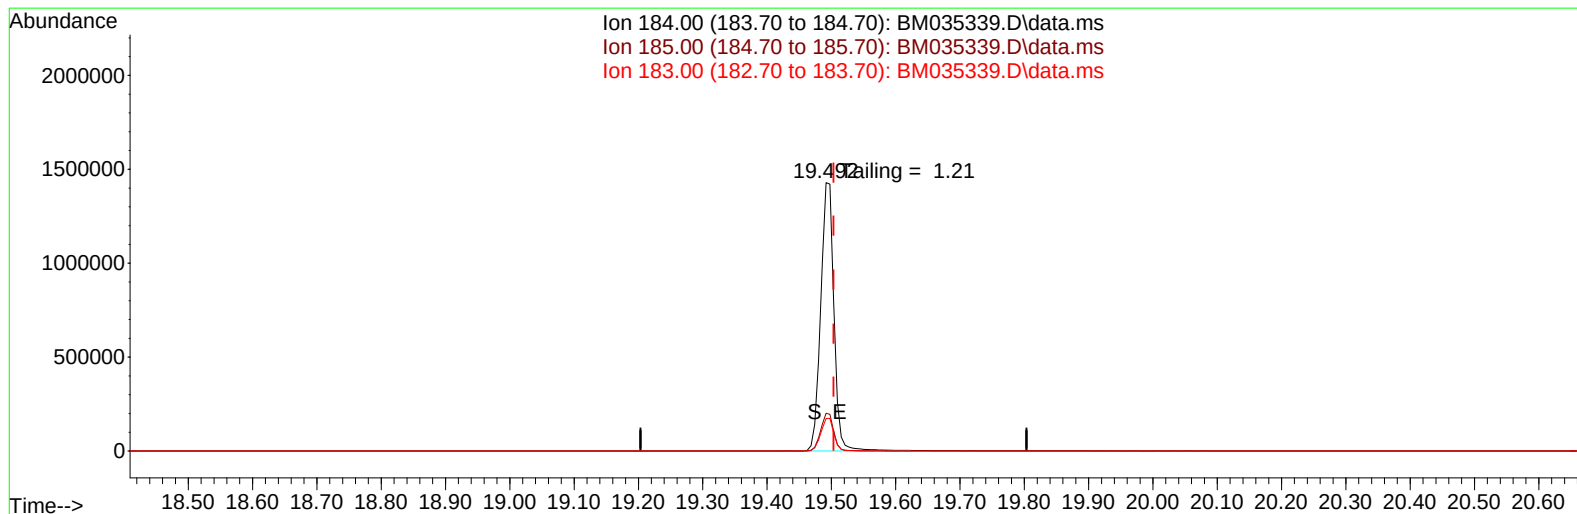

TIC: BM035339.D\data.ms

(77) Benzidine

19.492min (-0.012) 355263.06 ng

response 2058206

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.09
183.00	11.90	12.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/1/2022	BNA_M	<u>BM035339.D</u>
Compound Name	Response	Retention Time
DDT	1110703	20.727
DDD	13141	20.286
DDE	1912	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15053	1125756	1.34

Instrument :
BNA_M
ClientSampleId :
DFTPP