


Data Path : Z:\HPCHEM1\BNA_M\Data\BM060215\
Data File : BM001515.D
Acq On : 02 Jun 2015 16:30
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 03 02:19:00 2015

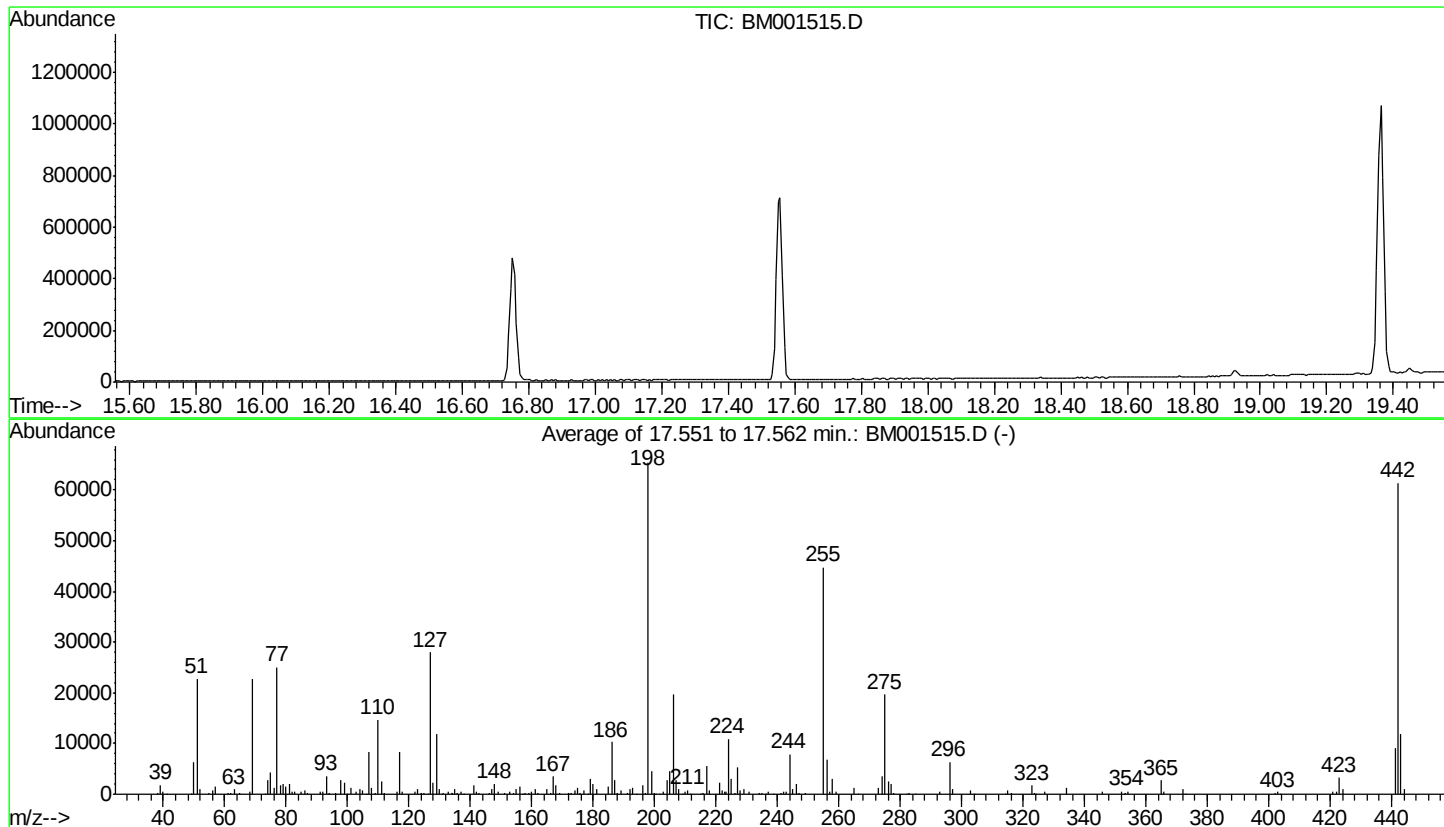

AutoFind: Scans 2527, 2528, 2529; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	22813	PASS
68	69	0.00	2	1.7	398	PASS
69	198	0.00	100	34.9	22792	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.7	27938	PASS
197	198	0.00	2	0.6	376	PASS
198	198	100	100	100.0	65384	PASS
199	198	5	9	6.9	4533	PASS
275	198	10	60	30.0	19607	PASS
365	198	1	100	4.2	2755	PASS
441	442	0.01	24	14.6	8975	PASS
442	198	50	100	93.9	61394	PASS
443	442	15	24	19.3	11824	PASS