


Data Path : Z:\HPCHEM1\BNA_M\Data\BM060215\
Data File : BM001533.D
Acq On : 03 Jun 2015 03:47
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 03 02:19:00 2015

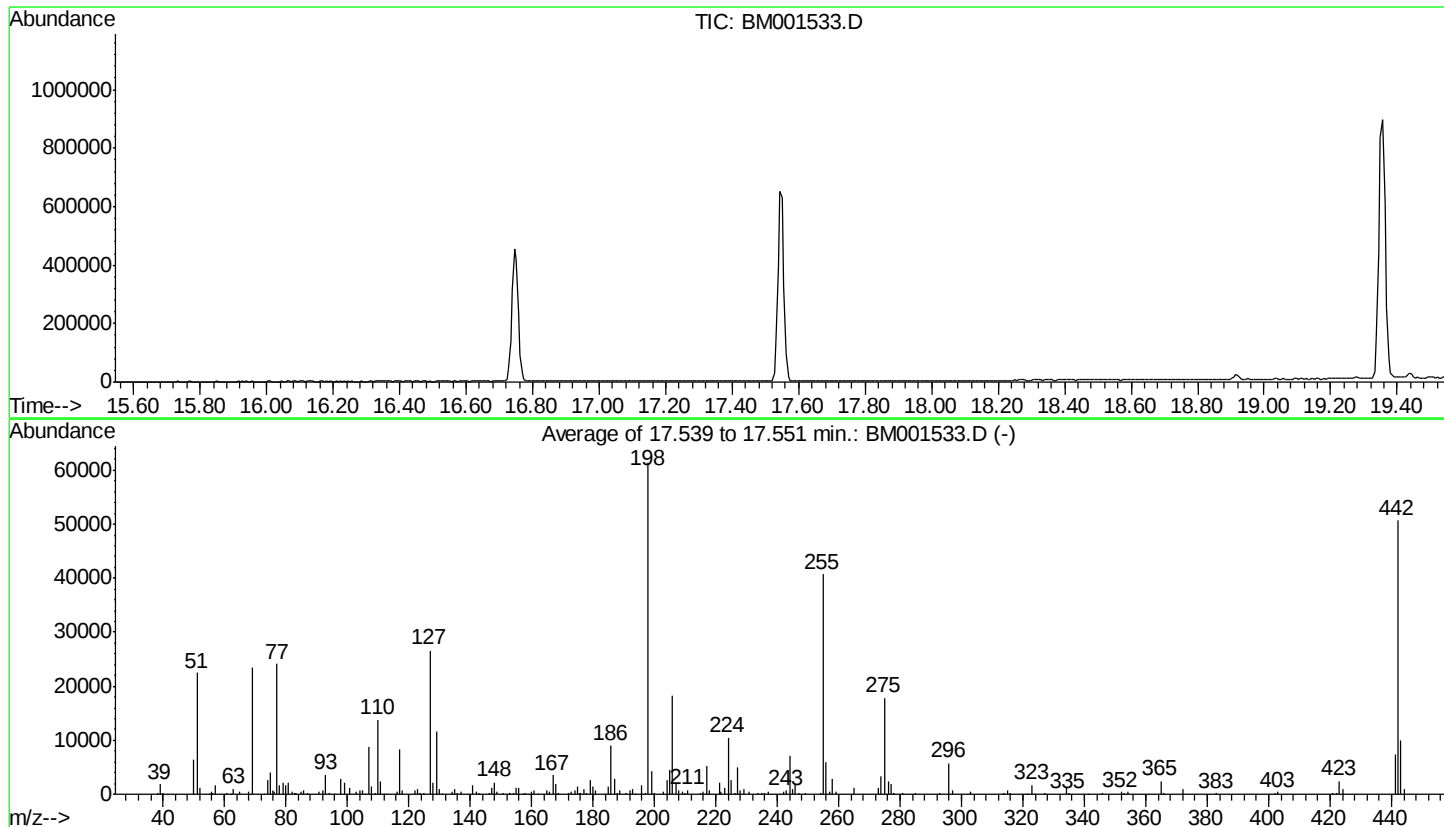

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	22453	PASS
68	69	0.00	2	2.2	511	FAIL*
69	198	0.00	100	38.3	23498	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.3	26578	PASS
197	198	0.00	2	0.5	321	PASS
198	198	100	100	100.0	61408	PASS
199	198	5	9	7.0	4284	PASS
275	198	10	60	29.1	17845	PASS
365	198	1	100	3.9	2410	PASS
441	442	0.01	24	14.5	7375	PASS
442	198	50	100	82.6	50704	PASS
443	442	15	24	19.7	9964	PASS