

Data Path : Z:\HPCHEM1\BNA M\DATA\BM060217\
 Data File : BM010395.D
 Acq On : 02 Jun 2017 19:48
 Operator : SJ/MA
 Sample : I3164-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 03 05:18:03 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 03 05:17:32 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	878	0.40	ng/ul	0.00
2) Naphthalene-d8	10.72	136	2721	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.55	164	1576	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	3205	0.40	ng/ul	0.00
16) Chrysene-d12	21.46	240	2927	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	199993	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.30	152	1083	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.31	212	2364	0.28	ng/ul	0.00
Target Compounds						
9) Fluorene	15.55	166	356	0.05	ng/ul#	28
17) Pyrene	19.69	202	550	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM060217\
Data File : BM010395.D
Acq On : 02 Jun 2017 19:48
Operator : SJ/MA
Sample : I3164-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 03 05:18:03 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 03 05:17:32 2017
Response via : Initial Calibration

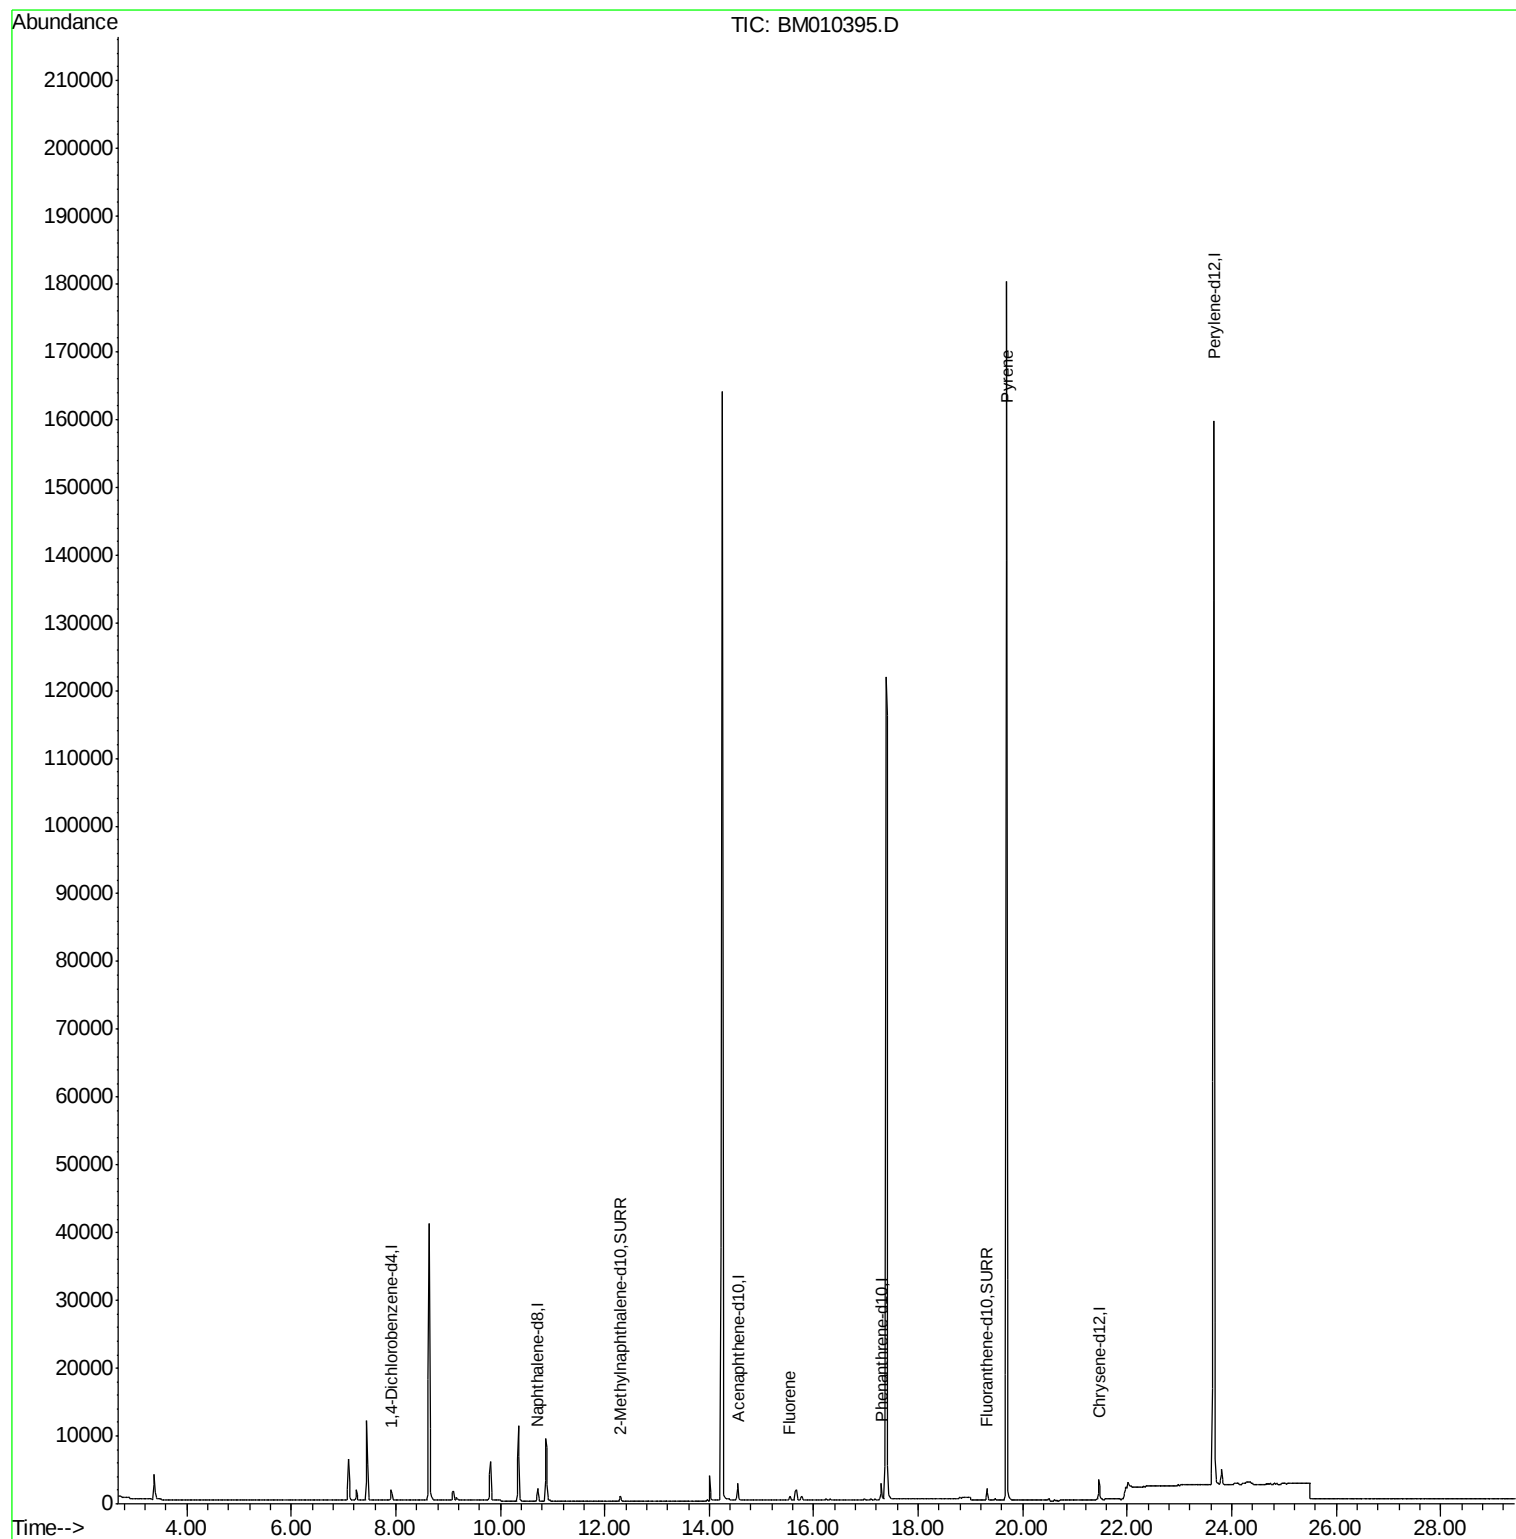

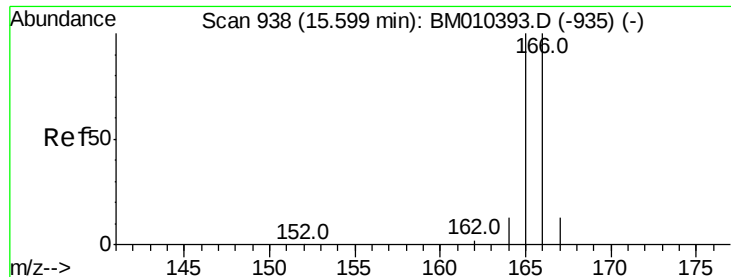

#9

Fluorene

Concen: 0.05 ng/ul

RT: 15.55 min Scan# 935

Delta R.T. -0.05 min

Lab File: BM010395.D

Acq: 02 Jun 2017 19:48

Instrument :

BNA_M

ClientSampleId :


Tot Ion:166 Resp: 356

Ion Ratio Lower Upper

166 100

165 21.6 73.4 110.2#

167 46.1 14.6 22.0#

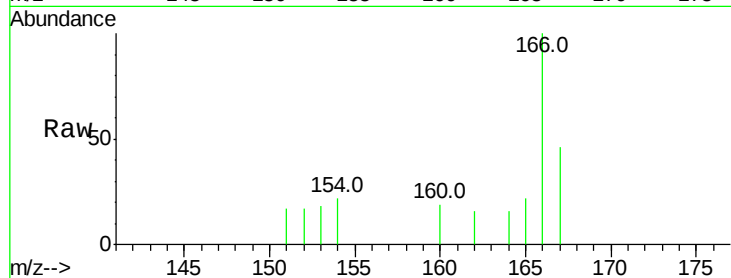

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

15.55

400



300

200

100

0

Time-->

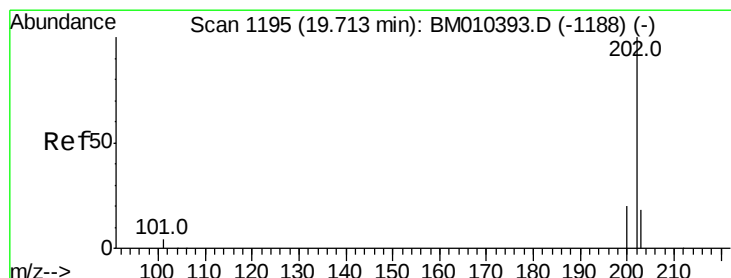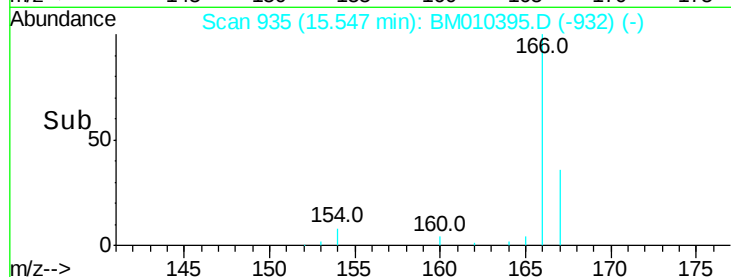

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.69 min Scan# 1193

Delta R.T. -0.02 min

Lab File: BM010395.D

Acq: 02 Jun 2017 19:48


Tgt Ion:202 Resp: 550

Ion Ratio Lower Upper

202 100

200 22.3 18.2 27.4

203 213.2 15.6 23.4#

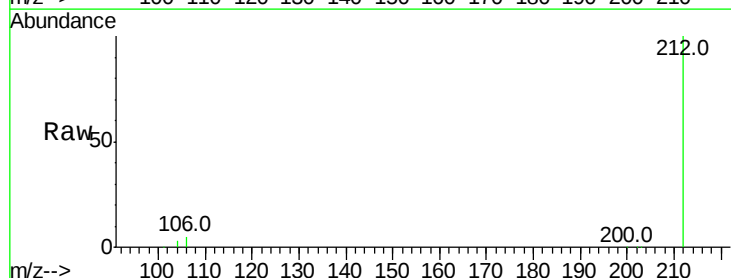

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

19.69

1000

800

600

400

200

0

Time-->

