


Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010378.D
Acq On : 02 Jun 2017 09:38
Operator : SJ/MA
Sample : PB99350BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK50

Manual Integrations
APPROVED

mohammad
6/5/2017 11:37:37 AM

Quant Time: Jun 02 18:02:15 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

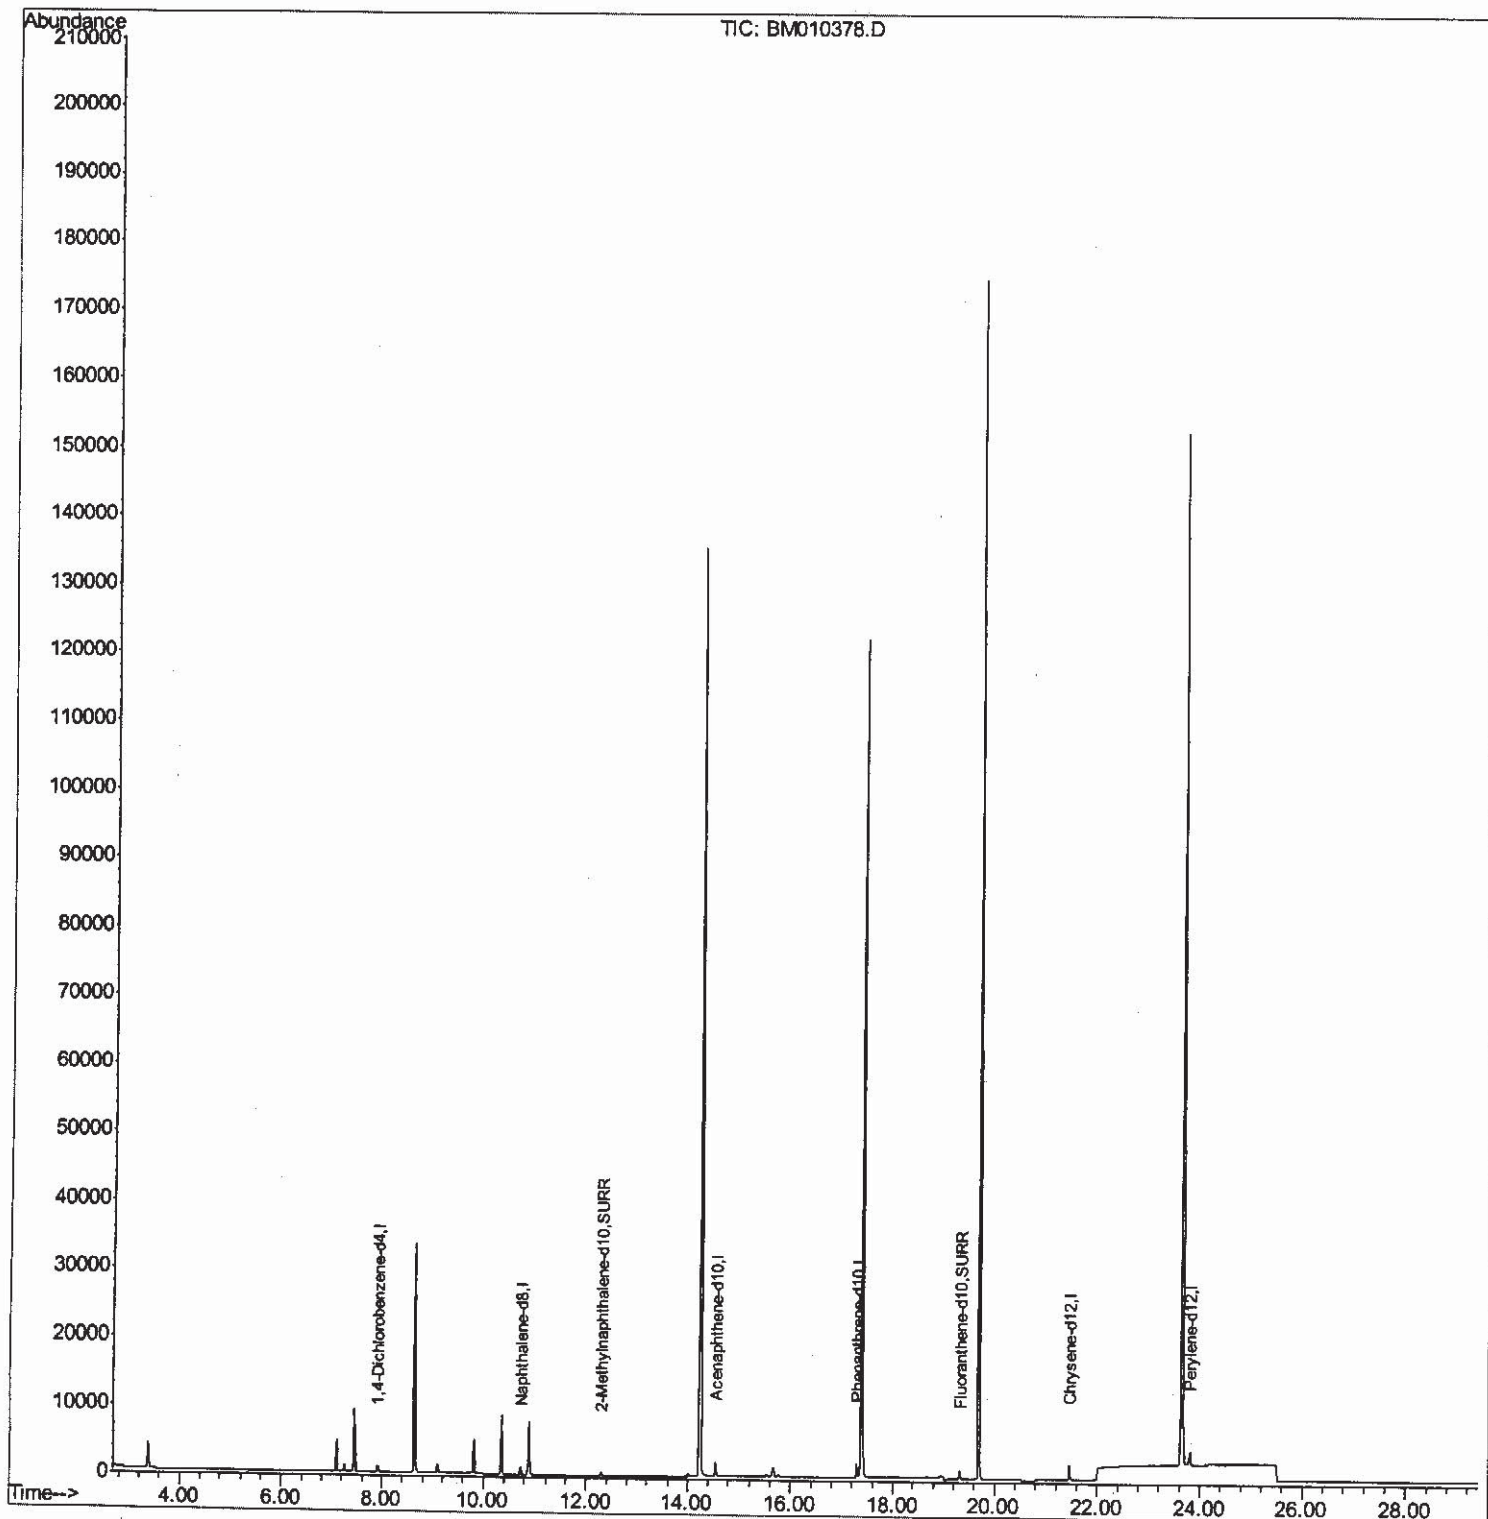




Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010378.D
Acq On : 02 Jun 2017 09:38
Operator : SJ/MA
Sample : PB99350BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK50

Manual Integrations
APPROVED

mohammad
6/5/2017 11:37:37 AM

Quant Time: Jun 02 17:40:54 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

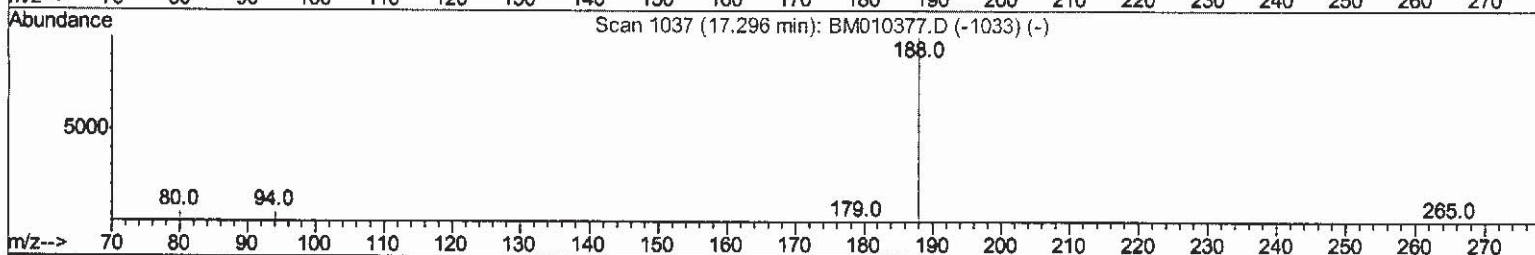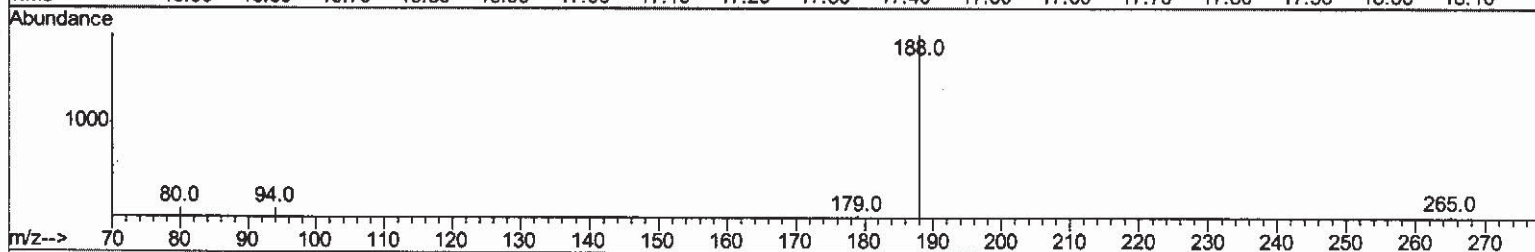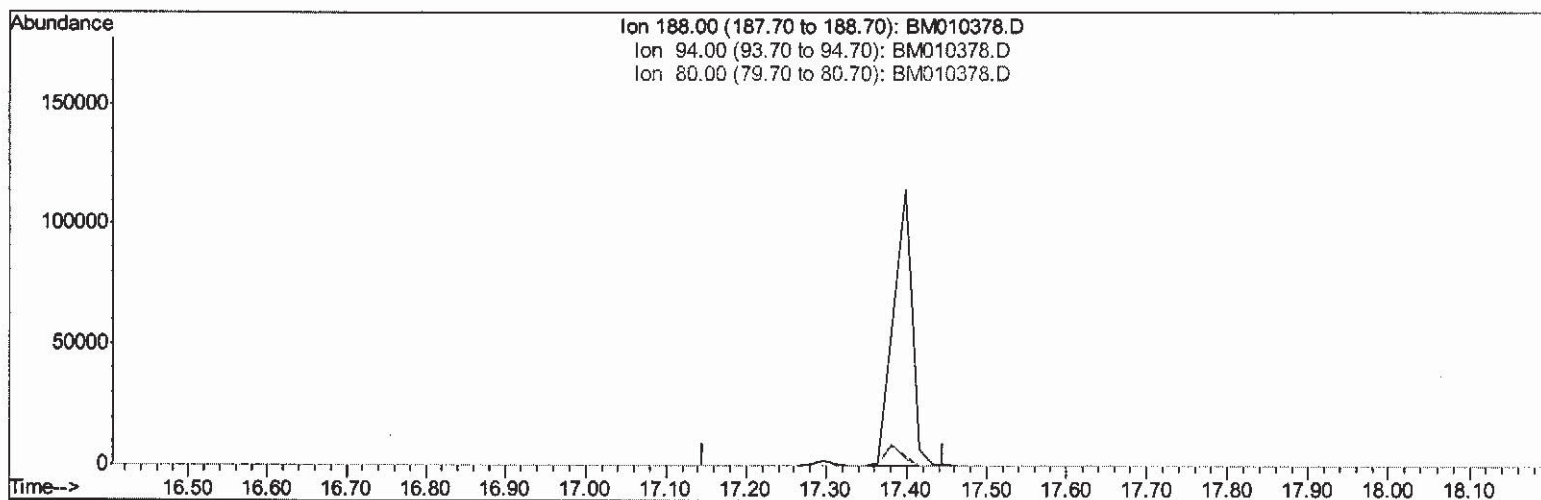

TIC: BM010378.D

(10) Phenanthrene-d10 (I)

17.296min (-17.296) 0.00ng/ui

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010378.D
Acq On : 02 Jun 2017 09:38
Operator : SJ/MA
Sample : PB99350BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK50

Manual Integrations
APPROVED

mohammad
6/5/2017 11:37:37 AM

Quant Time: Jun 02 17:40:54 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

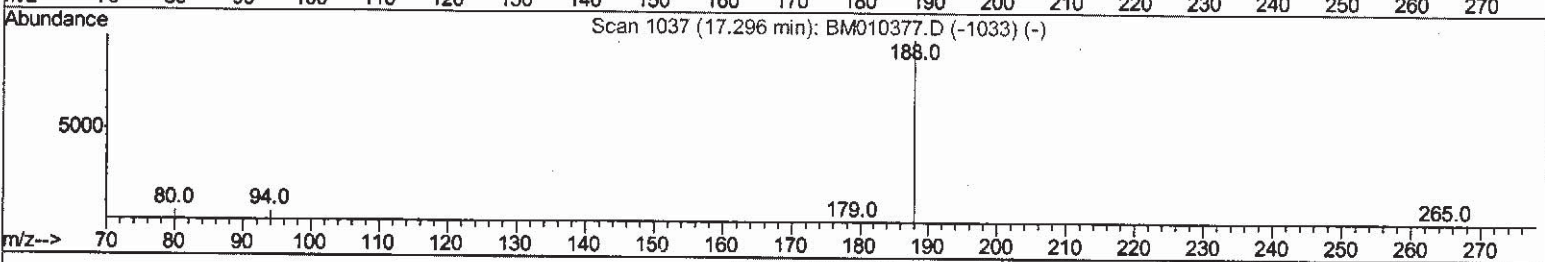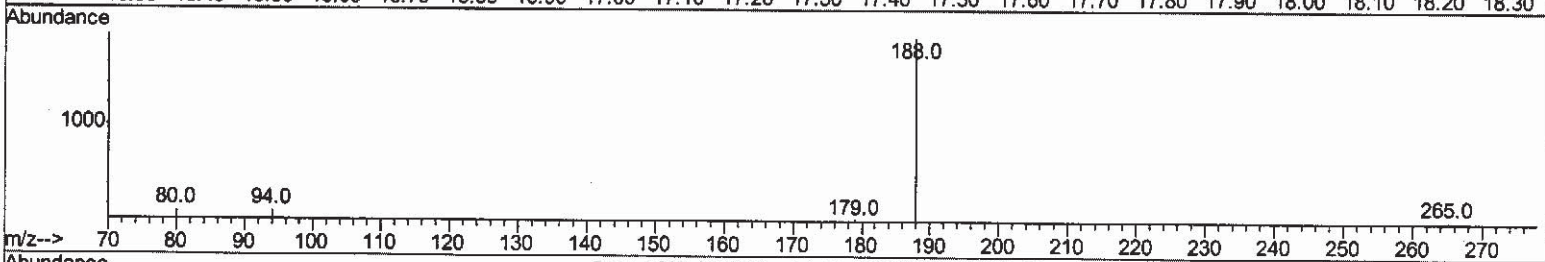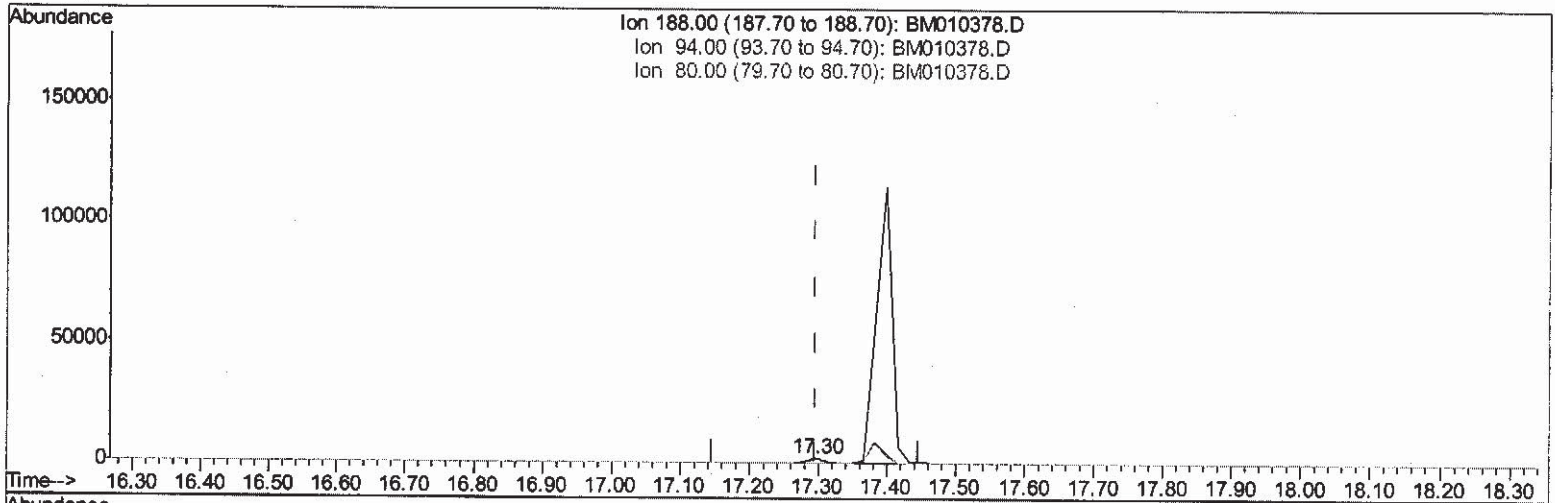

TIC: BM010378.D

(10) Phenanthrene-d10 (I)

17.296min (+0.000) 0.40ng/ul m SJ 6/5/17

response 2789

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.69#
80.00	11.80	7.69#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010378.D
Acq On : 02 Jun 2017 09:38
Operator : SJ/MA
Sample : PB99350BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK50

Manual Integrations
APPROVED

mohammad
6/5/2017 11:37:37 AM

Quant Time: Jun 02 18:01:27 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

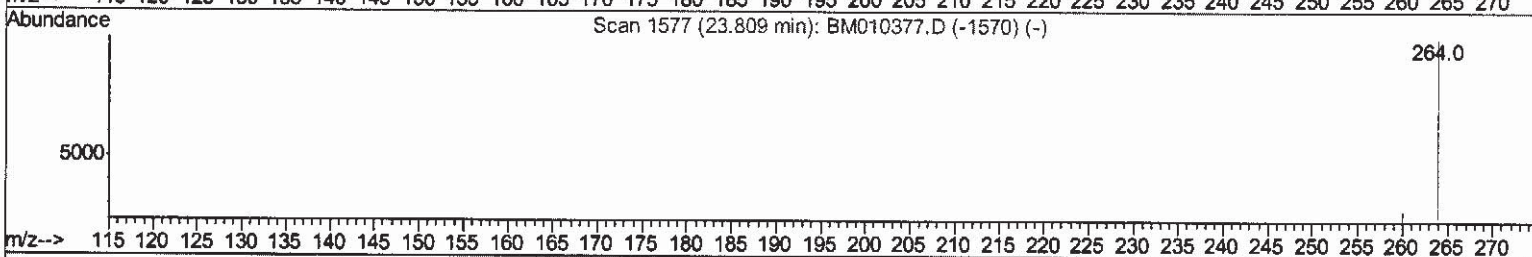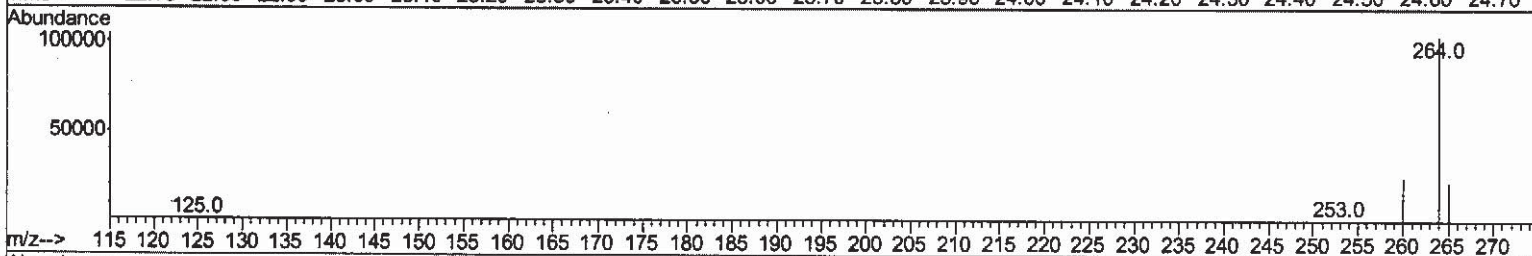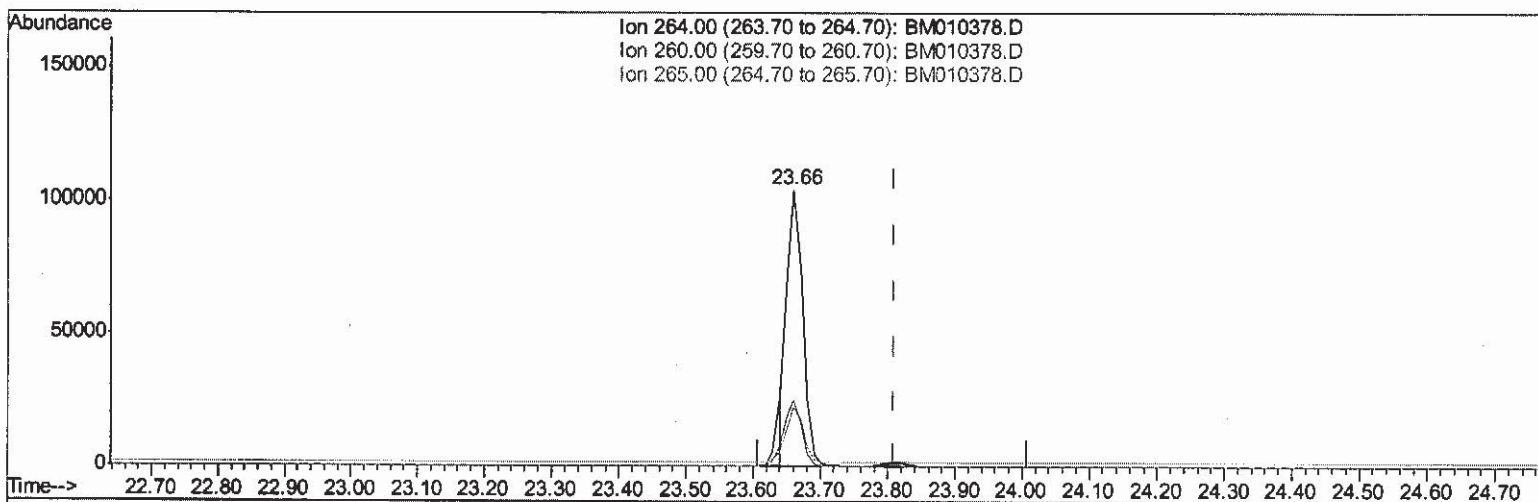

TIC: BM010378.D

(20) Perylene-d12 (I)

23.660min (-0.149) 0.40ng/ul

response 173616

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.10
265.00	103.50	21.54#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010378.D
Acq On : 02 Jun 2017 09:38
Operator : SJ/MA
Sample : PB99350BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK50

Manual Integrations
APPROVED

mohammad
6/5/2017 11:37:37 AM

Quant Time: Jun 02 18:01:27 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

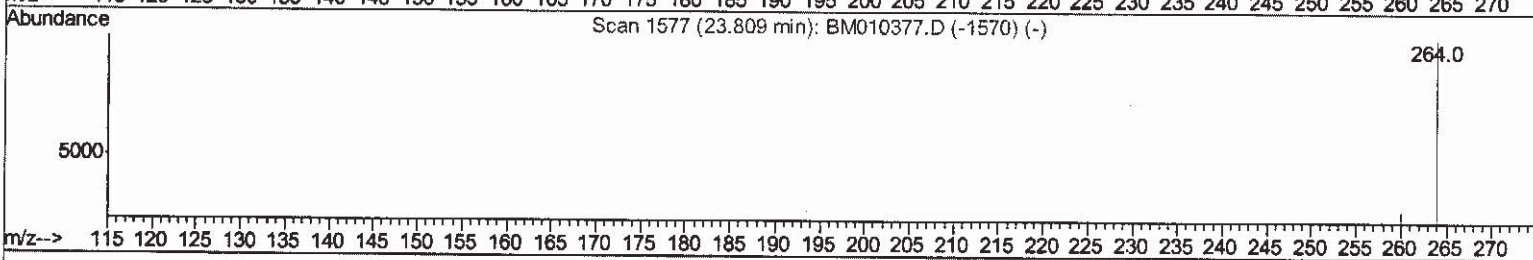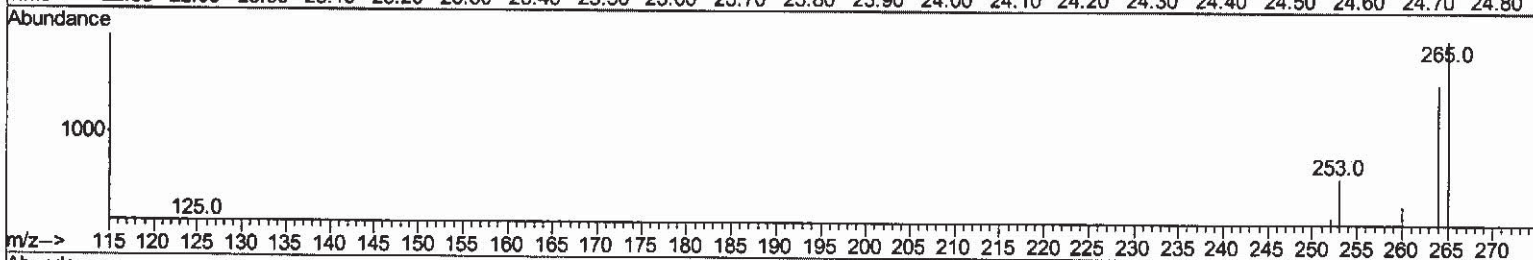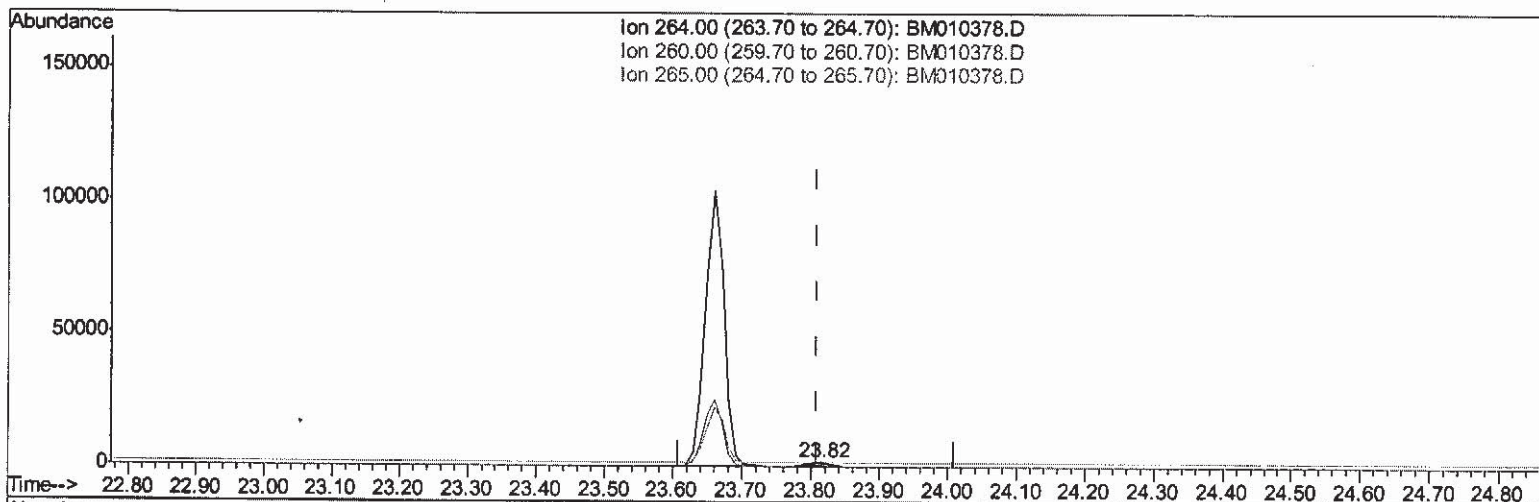

TIC: BM010378.D

(20) Perylene-d12 (I)

23.816min (+0.007) 0.40ng/ul m SJ 6/6/17

response 2578

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	30.19
265.00	103.50	125.09#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010378.D
Acq On : 02 Jun 2017 09:38
Operator : SJ/MA
Sample : PB99350BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK50

Manual Integrations
APPROVED

mohammad
6/5/2017 11:37:37 AM

Quant Time: Jun 02 18:02:15 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	712	0.40	ng/ul	0.00
2) Naphthalene-d8	10.73	136	2079	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.55	164	1223	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	2789m>	0.40	ng/ul	0.00
16) Chrysene-d12	21.47	240	2551	0.40	ng/ul	0.00
20) Perylene-d12	23.82	264	2578m>	0.40	ng/ul	0.00

} SJ 6/6/17

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.31	152	920	0.30	ng/ul	0.01
14) Fluoranthene-d10	19.33	212	2149	0.29	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed