


Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010385.D
Acq On : 02 Jun 2017 13:50
Operator : SJ/MA
Sample : I3164-03MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSGMSD

Manual Integrations
APPROVED

mohammad
6/5/2017 11:38:00 AM

Quant Time: Jun 02 18:23:15 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

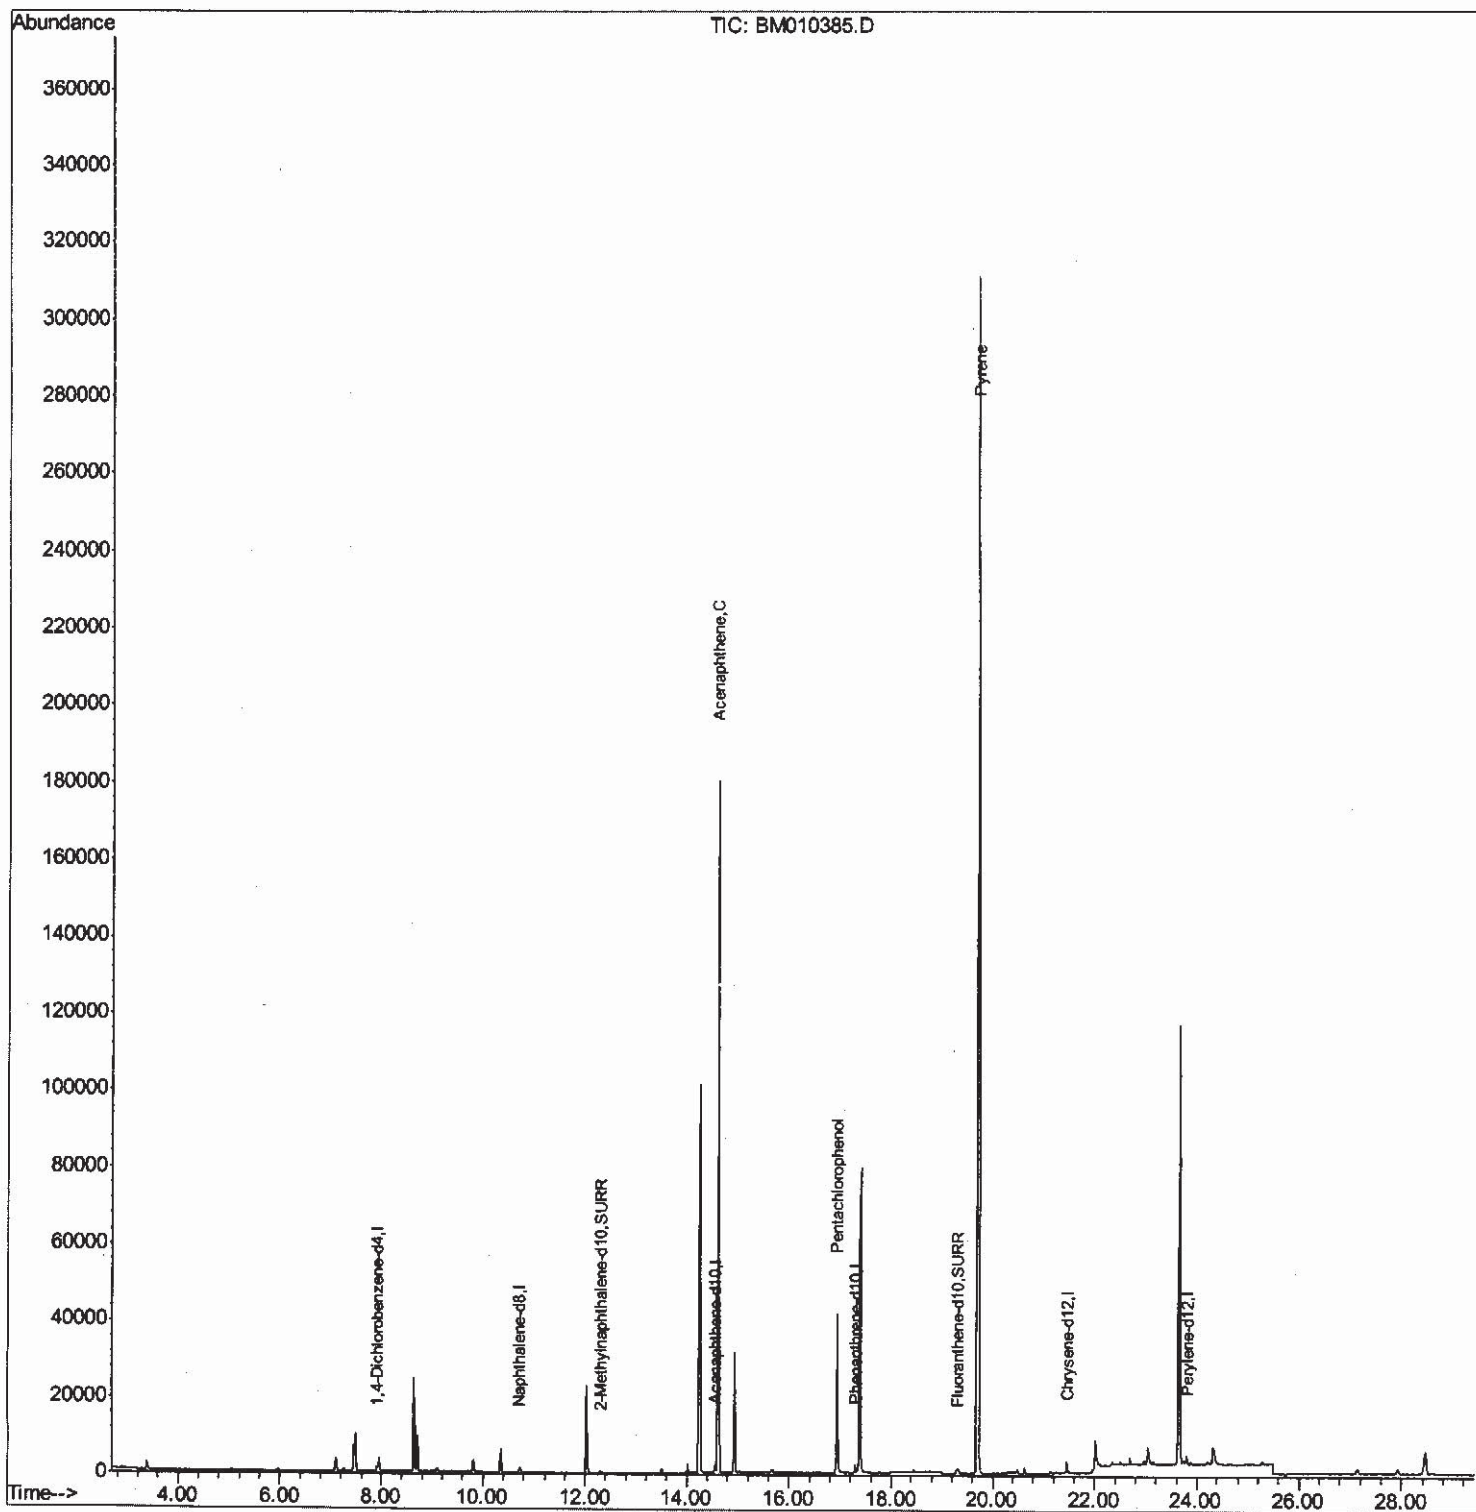




Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010385.D
Acq On : 02 Jun 2017 13:50
Operator : SJ/MA
Sample : I3164-03MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSGMSD

Manual Integrations
APPROVED

mohammad
6/5/2017 11:38:00 AM

Quant Time: Jun 02 18:21:28 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

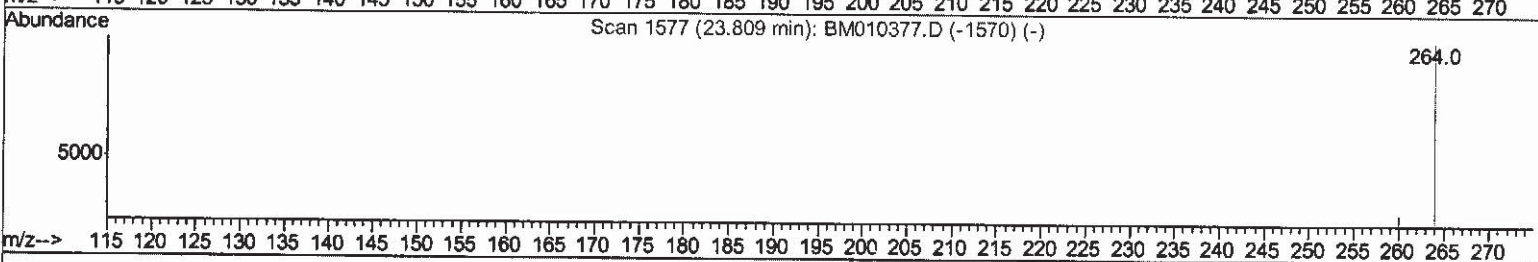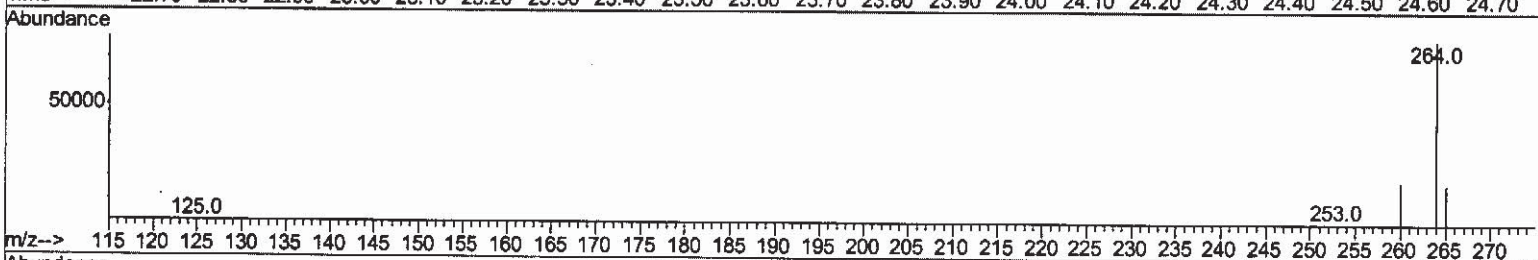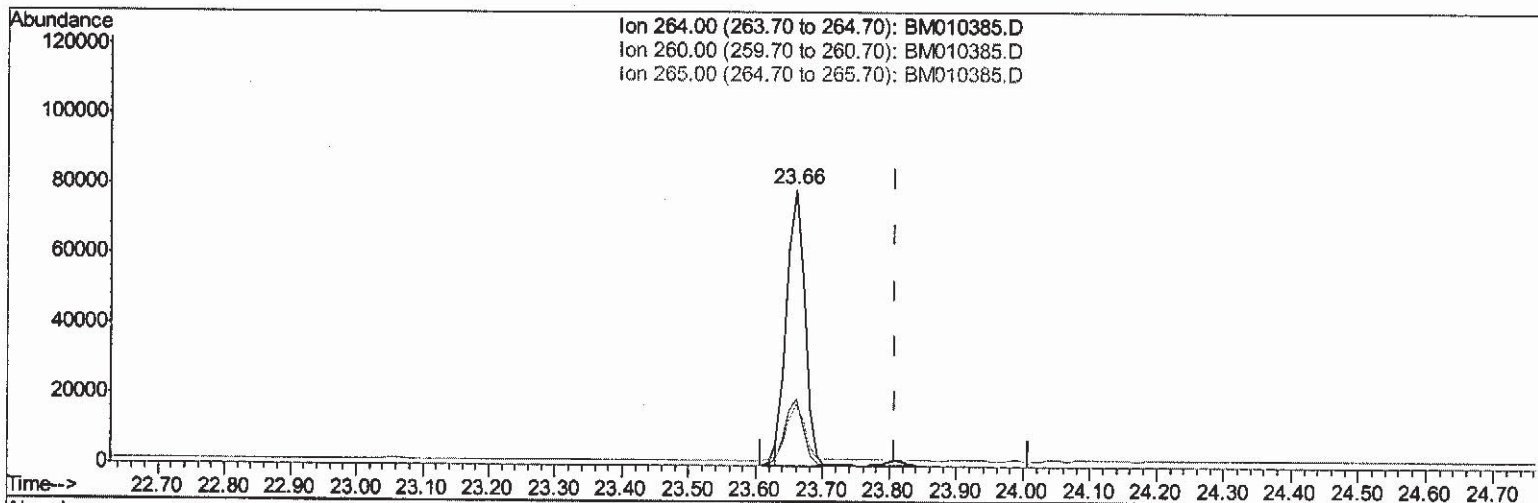

TIC: BM010385.D

(20) Perylene-d12 (I)

23.660min (-0.149) 0.40ng/ul

response 146916

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.99#
265.00	103.50	22.34#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010385.D
Acq On : 02 Jun 2017 13:50
Operator : SJ/MA
Sample : I3164-03MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSGMSD

Manual Integrations
APPROVED

mohammad
6/5/2017 11:38:00 AM

Quant Time: Jun 02 18:21:28 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

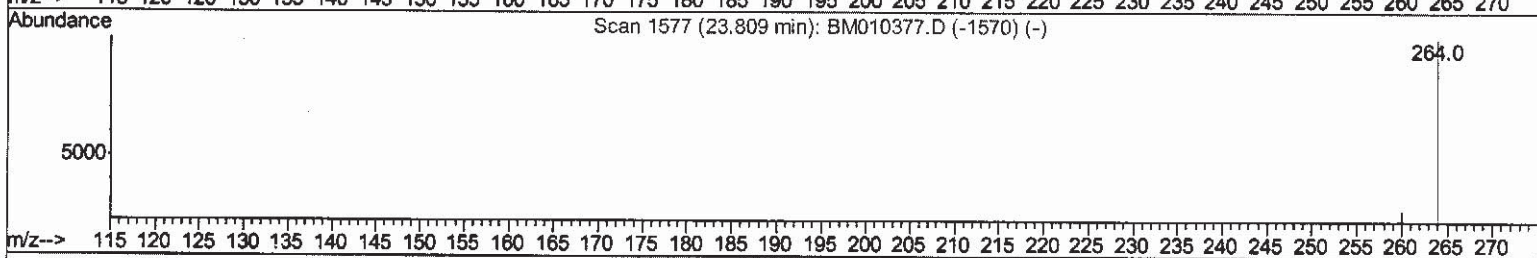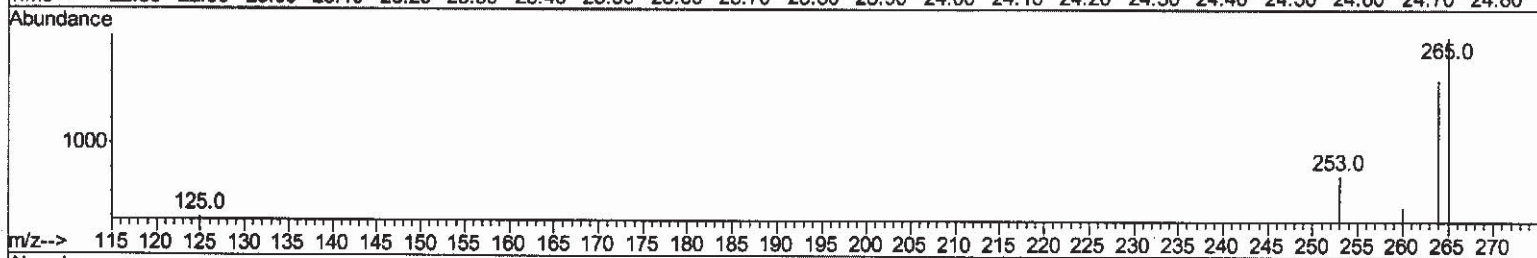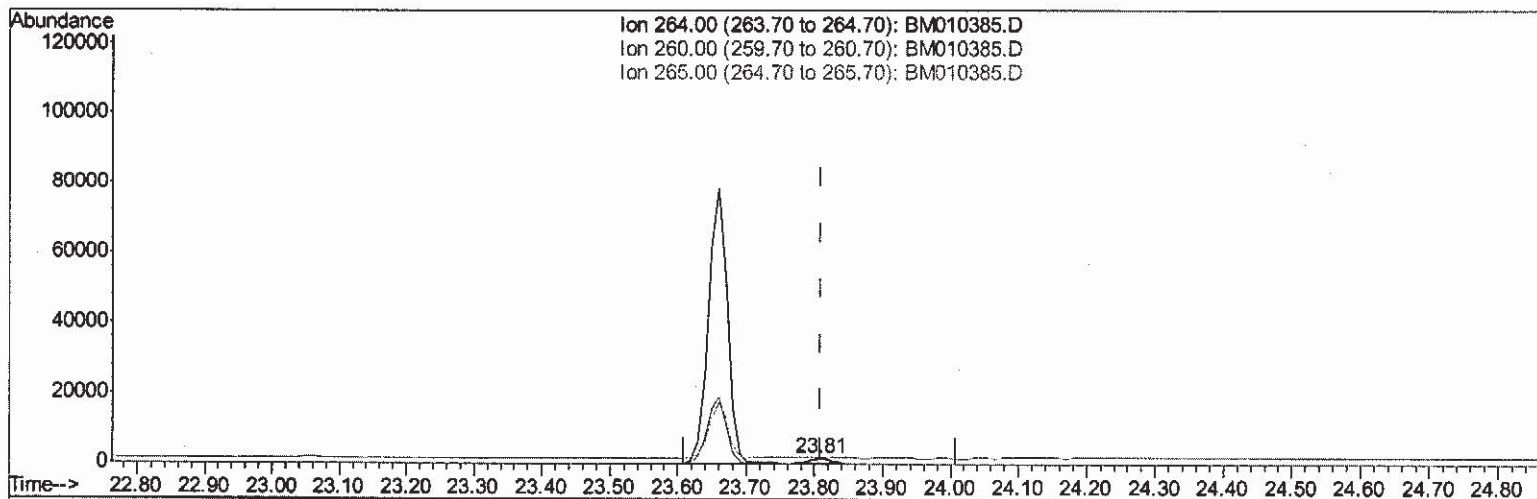

TIC: BM010385.D

(20) Perylene-d12 (I)

23.806min (-0.003) 0.40ng/ul m

SJ 6/6/17

response 2975

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	32.25
265.00	103.50	122.39
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
 Data File : BM010385.D
 Acq On : 02 Jun 2017 13:50
 Operator : SJ/MA
 Sample : I3164-03MSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSGMSD

Manual Integrations
 APPROVED

mohammad
 6/5/2017 11:38:00 AM

Quant Time: Jun 02 18:23:15 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 02 17:41:09 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	782	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.72	136	2397	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.55	164	1280	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	2820	0.40	ng/ul	0.00
16) Chrysene-d12	21.46	240	2980	0.40	ng/ul	0.00
20) Perylene-d12	23.81	264	2975m>	0.40	ng/ul	0.00

SJ 6/6/17

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.30	152	682	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.31	212	1746	0.23	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
8) Acenaphthene	14.61	153	104477	21.62	ng/ul	95
11) Pentachlorophenol	16.94	266	29578	27.43	ng/ul	97
17) Pyrene	19.71	202	274472	21.62	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed