

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
 Data File : BM010389.D
 Acq On : 02 Jun 2017 16:13
 Operator : SJ/MA
 Sample : I3163-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 02 18:32:43 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 02 17:41:09 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 JHSF9

Manual Integrations
 APPROVED

mohammad
 6/5/2017 11:38:17 AM

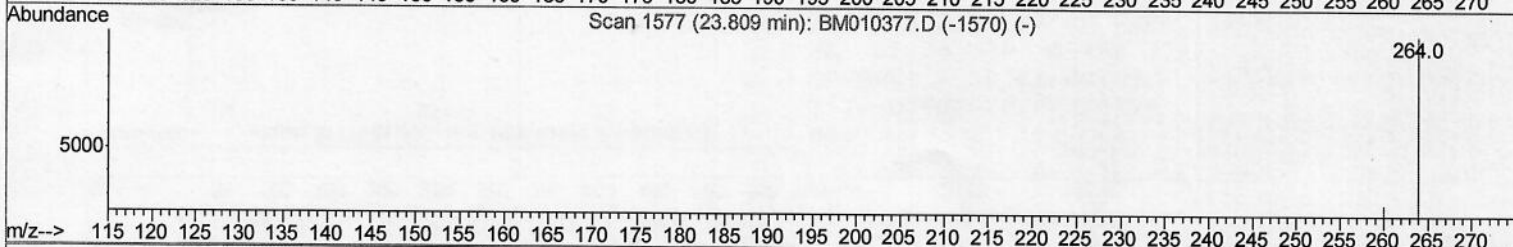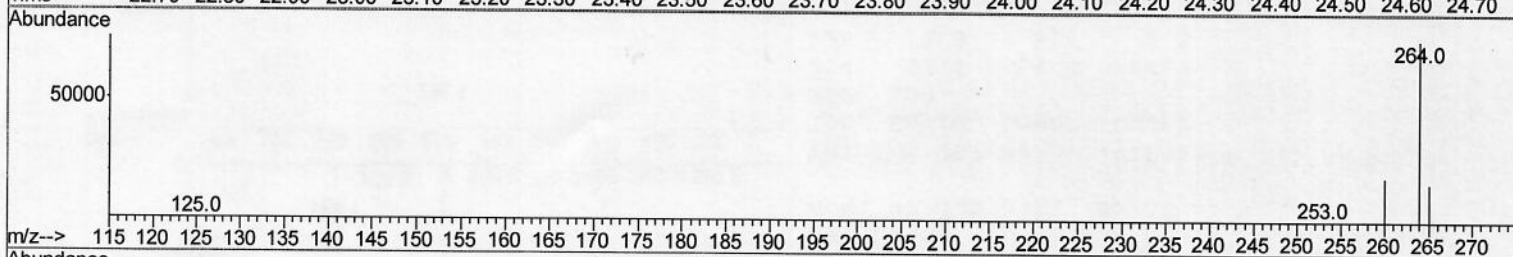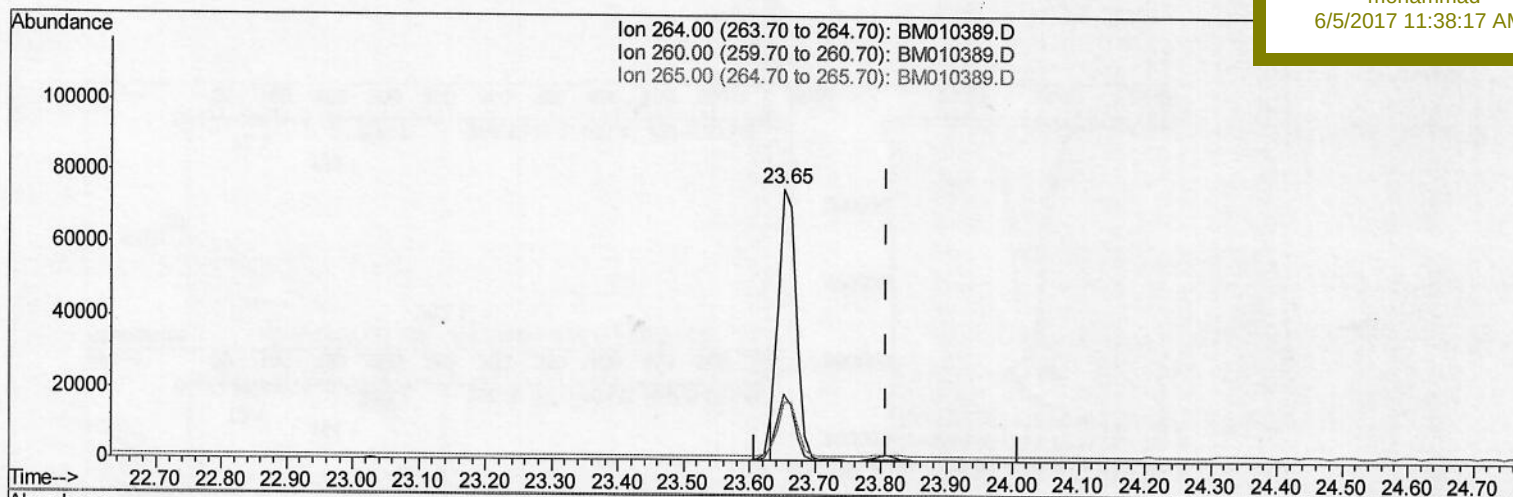

TIC: BM010389.D

(20) Perylene-d12 (I)

23.653min (-0.156) 0.40ng/ul

response 141242

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.00
265.00	103.50	21.77#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
 Data File : BM010389.D
 Acq On : 02 Jun 2017 16:13
 Operator : SJ/MA
 Sample : I3163-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 02 18:32:43 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 02 17:41:09 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 JHSF9

Manual Integrations
 APPROVED

mohammad
 6/5/2017 11:38:17 AM

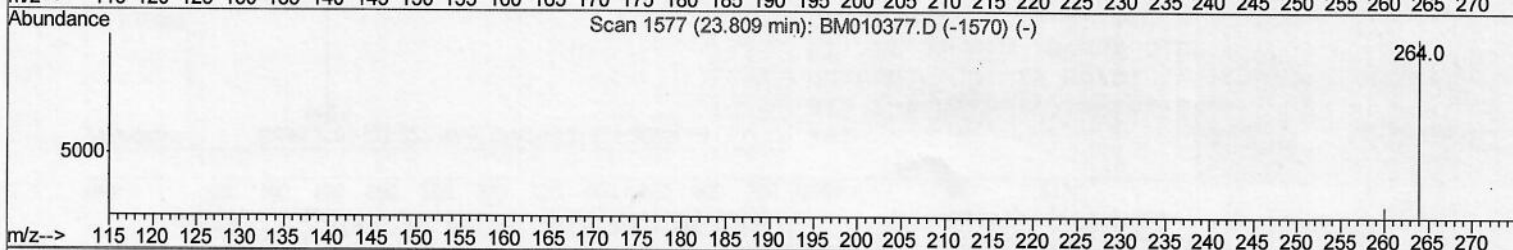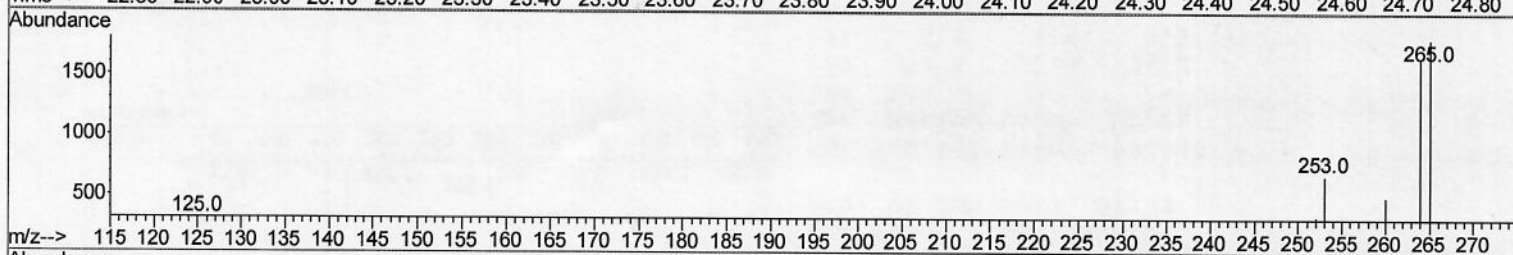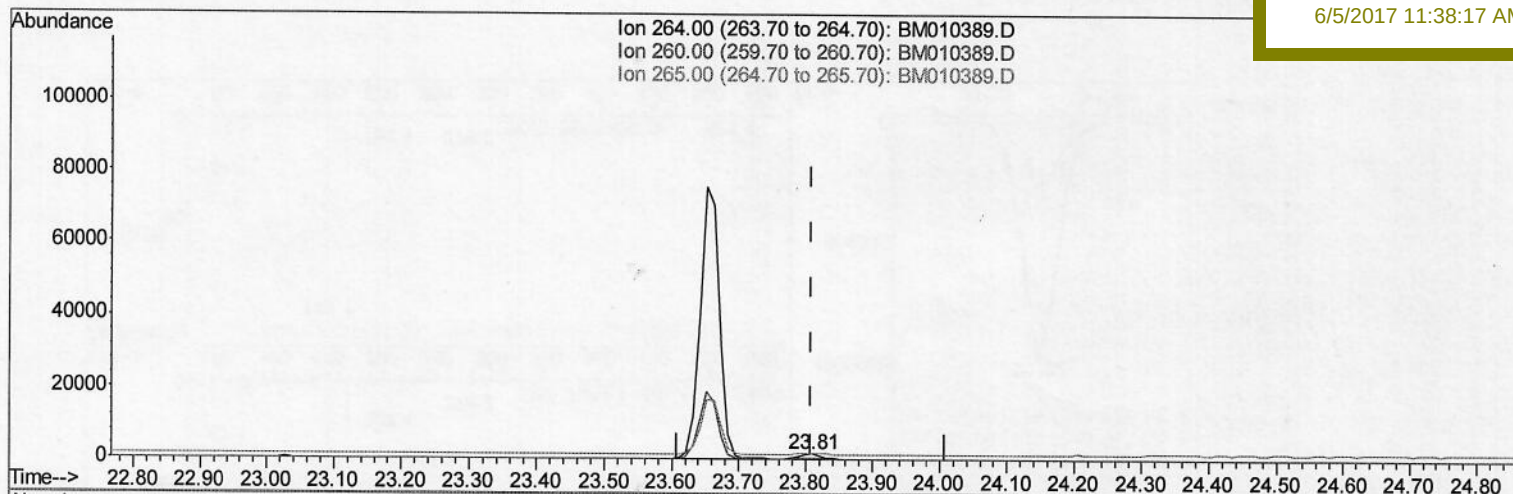

TIC: BM010389.D

(20) Perylene-d12 (I)

23.809min (+0.000) 0.40ng/ul m

SJ 06/06/17

response 2857

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	30.48
265.00	103.50	109.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM060217\
 Data File : BM010389.D
 Acq On : 02 Jun 2017 16:13
 Operator : SJ/MA
 Sample : I3163-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 14 15:52:40 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 02 17:41:09 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 JHSF9

Manual Integrations
 APPROVED

mohammad
 6/5/2017 11:38:17 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	741	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.72	136	2190	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.55	164	1268	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	2802	0.40	ng/ul	0.00
16) Chrysene-d12	21.46	240	2839	0.40	ng/ul	0.00
20) Perylene-d12	23.81	264	2857m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.30	152	659	0.21	ng/ul	0.00
14) Fluoranthene-d10	19.32	212	1765	0.24	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.33	178	303	0.03	ng/ul#	55

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 06/06/17

Data Path : Z:\HPCHEM1\BNA M\DATA\BM060217\
Data File : BM010389.D
Acq On : 02 Jun 2017 16:13
Operator : SJ/MA
Sample : I3163-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Jun 14 15:52:40 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
JHSF9

Manual Integrations
APPROVED

mohammad
6/5/2017 11:38:17 AM

