


Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010392.D
Acq On : 02 Jun 2017 18:01
Operator : SJ/MA
Sample : I3163-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSF5

Manual Integrations
APPROVED

mohammad
6/5/2017 11:38:39 AM

Quant Time: Jun 02 18:54:18 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

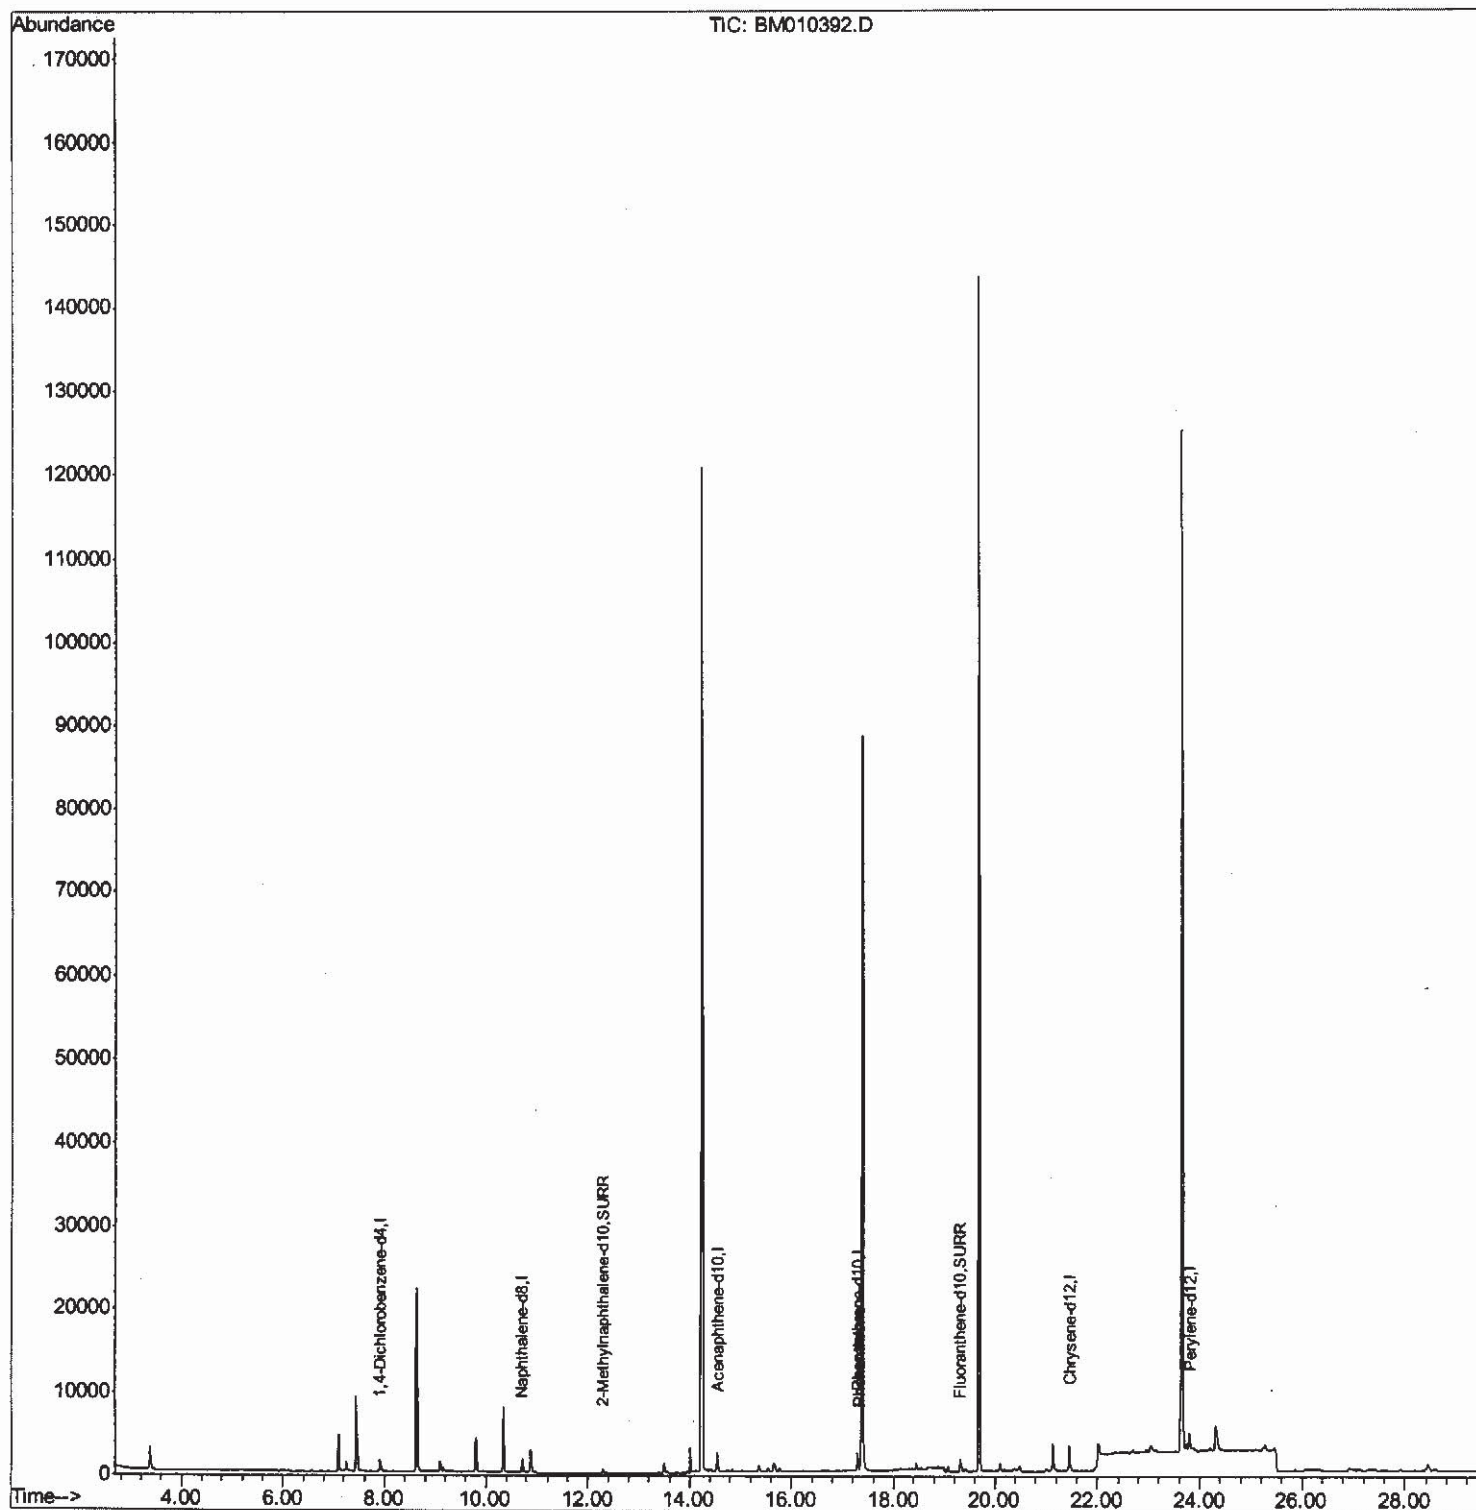




Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010392.D
Acq On : 02 Jun 2017 18:01
Operator : SJ/MA
Sample : I3163-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSF5

Manual Integrations
APPROVED

mohammad
6/5/2017 11:38:39 AM

Quant Time: Jun 02 18:53:18 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

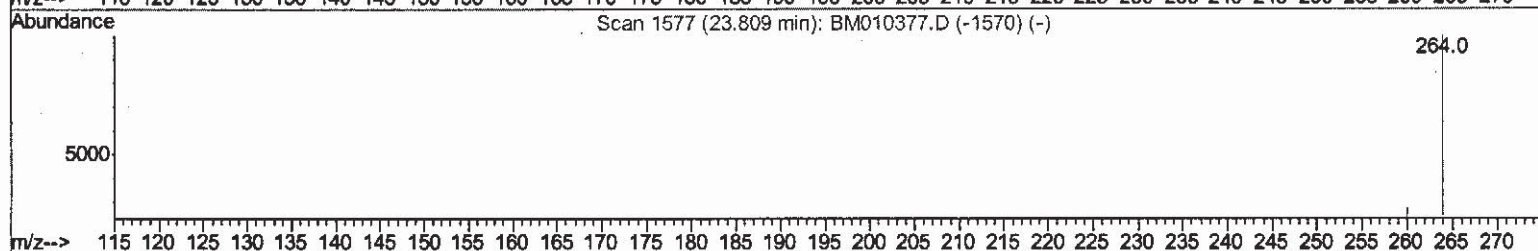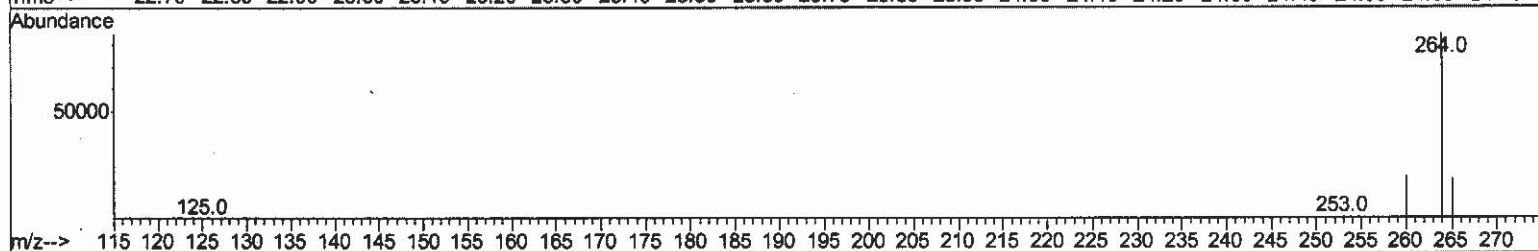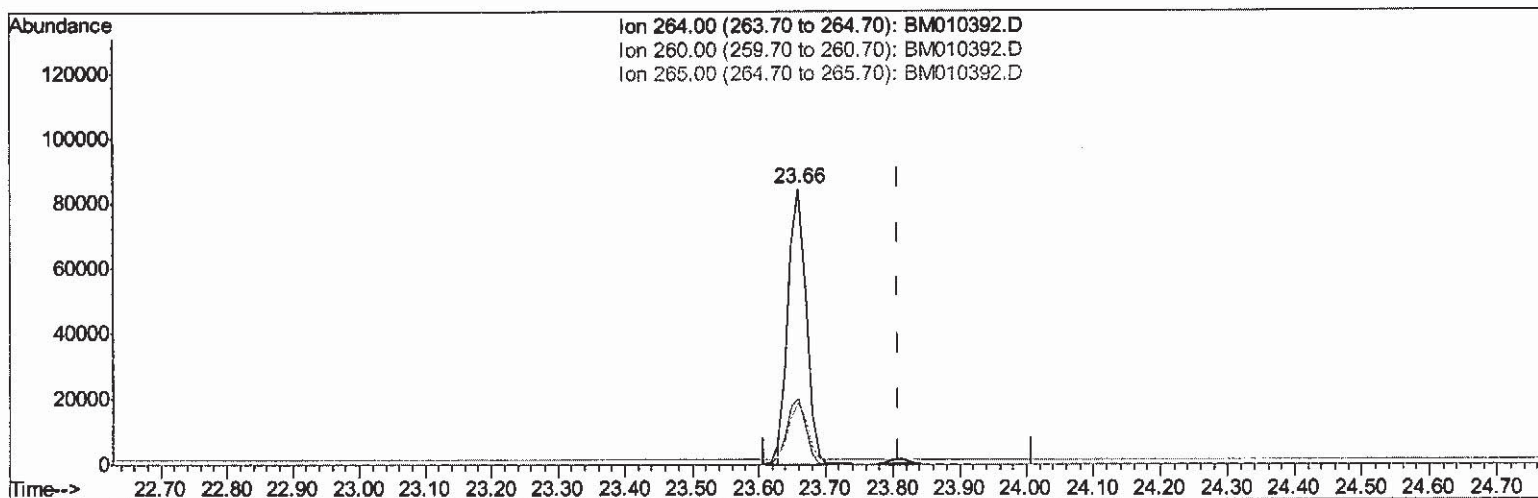

TIC: BM010392.D

(20) Perylene-d12 (I)

23.660min (-0.149) 0.40ng/ui

response 155816

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	23.61#
265.00	103.50	22.29#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010392.D
Acq On : 02 Jun 2017 18:01
Operator : SJ/MA
Sample : I3163-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSF5

Manual Integrations
APPROVED

mohammad
6/5/2017 11:38:39 AM

Quant Time: Jun 02 18:53:18 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

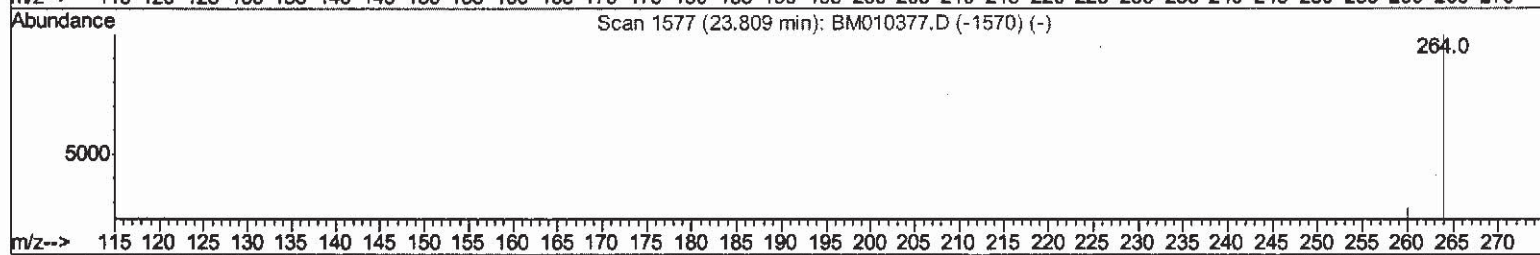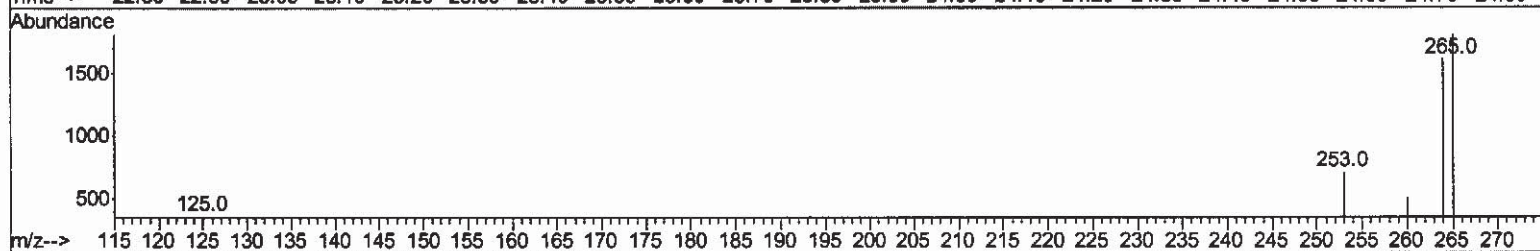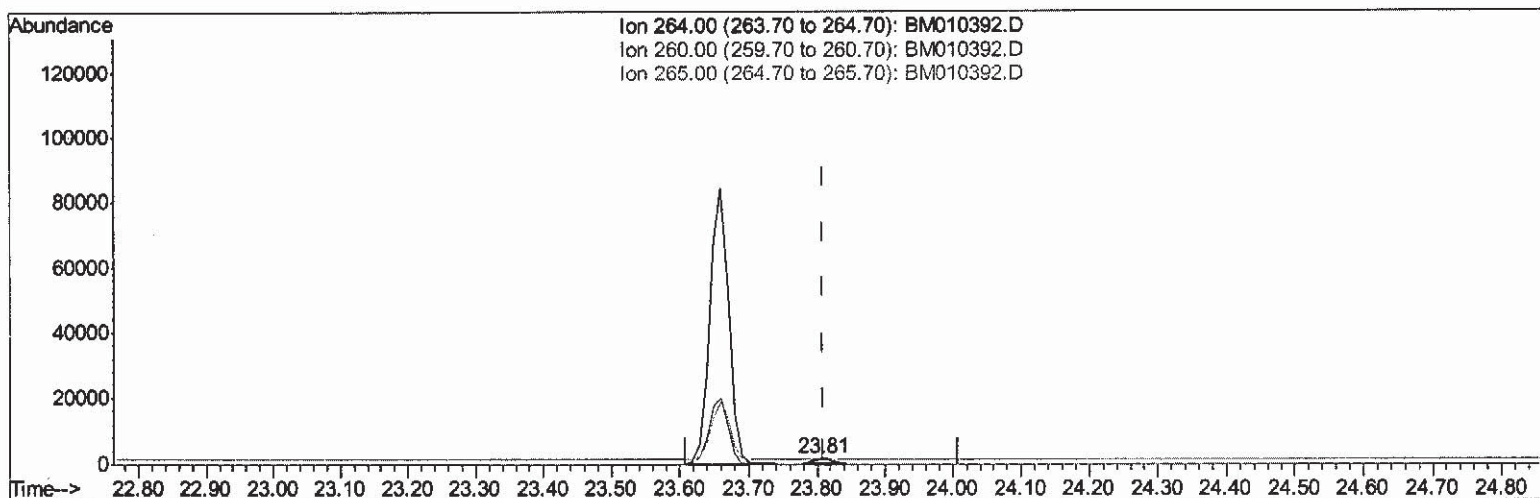

TIC: BM010392.D

(20) Perylene-d12 (I)

23.806min (-0.003) 0.40ng/ul m

SJ 6/6/17

response 3002

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	31.36
265.00	103.50	111.95
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM060217\
Data File : BM010392.D
Acq On : 02 Jun 2017 18:01
Operator : SJ/MA
Sample : I3163-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSF5

Manual Integrations
APPROVED

mohammad
6/5/2017 11:38:39 AM

Quant Time: Jun 02 18:54:18 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 02 17:41:09 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	887	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.72	136	2556	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.55	164	1442	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	3022	0.40	ng/ul	0.00
16) Chrysene-d12	21.46	240	2983	0.40	ng/ul	0.00
20) Perylene-d12	23.81	264	3002m	0.40	ng/ul	0.00

SJ 6/6/17

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.30	152	834	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.31	212	1922	0.24	ng/ul	0.00

Target Compounds

12) Phenanthrene	17.33	178	280	0.03	ng/ul#	50
------------------	-------	-----	-----	------	--------	----

(#) = qualifier out of range (m) = manual integration (+) = signals summed