

Data Path : Z:\HPCHEM1\BNA M\DATA\BM060217\
 Data File : BM010396.D
 Acq On : 02 Jun 2017 20:24
 Operator : SJ/MA
 Sample : I3164-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSL1

Quant Time: Jun 13 12:50:53 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 03 05:17:32 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	849	0.40	ng/ul	0.00
2) Naphthalene-d8	10.72	136	2512	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.55	164	1408	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.30	188	3121	0.40	ng/ul	0.00
16) Chrysene-d12	21.46	240	3186	0.40	ng/ul	0.00
20) Perylene-d12	23.81	264	3544	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.30	152	581	0.16	ng/ul	0.00
14) Fluoranthene-d10	19.32	212	1472	0.18	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.33	178	379	0.04	ng/ul#	Ovalue 66




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM060217\
Data File : BM010396.D
Acq On : 02 Jun 2017 20:24
Operator : SJ/MA
Sample : I3164-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSL1

Quant Time: Jun 13 12:50:53 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM053017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 03 05:17:32 2017
Response via : Initial Calibration

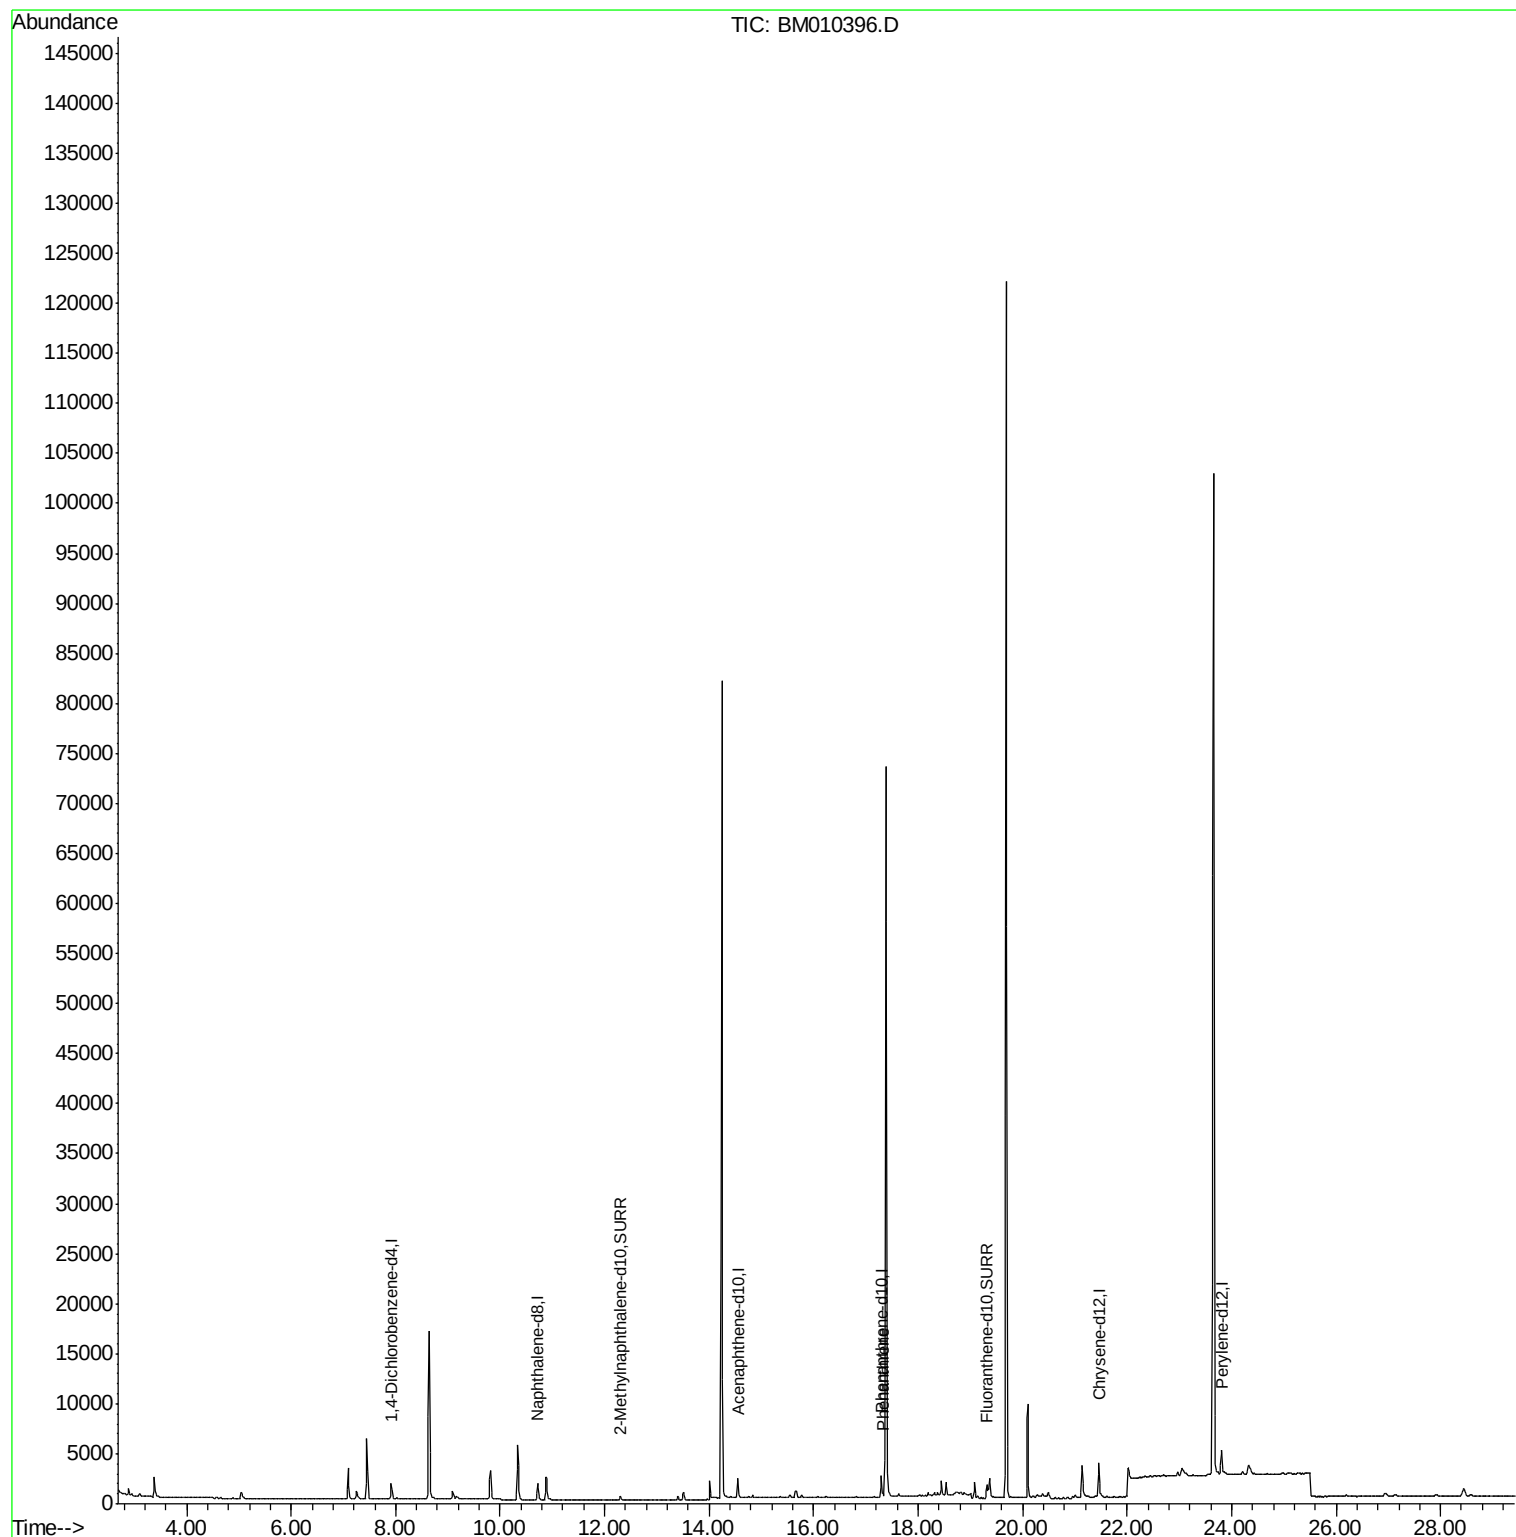

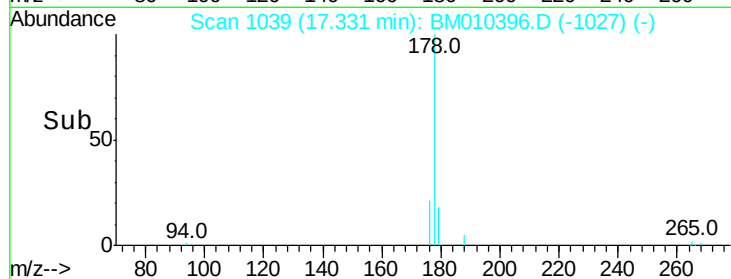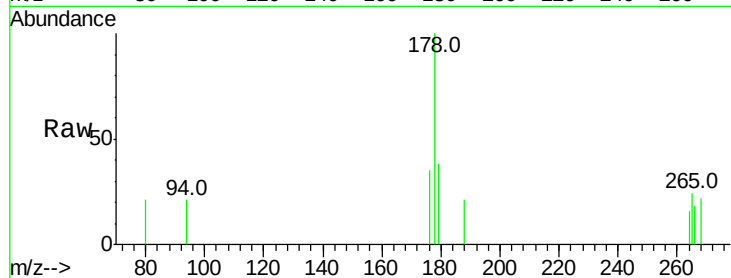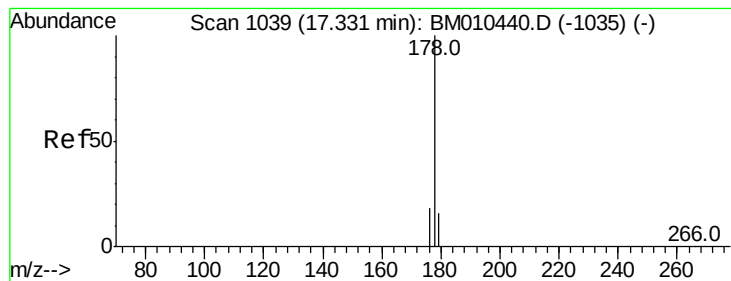

#12

Phenanthrene

Concen: 0.04 ng/ul

RT: 17.33 min Scan# 1039

Delta R.T. 0.00 min

Lab File: BM010396.D

Acq: 02 Jun 2017 20:24

Instrument :
BNA_M
ClientSampleId :
JHSL1

Tot Ion	Ratio	Lower	Upper
178	100		
176	34.8	18.4	27.6#
179	37.8	13.6	20.4#

