


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060221\
Data File : BM030266.D
Acq On : 02 Jun 2021 19:16
Operator : CG/JU
Sample : M2568-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GN0

Quant Time: Jun 03 01:31:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 02 17:27:46 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/3/2021 11:06:15 AM

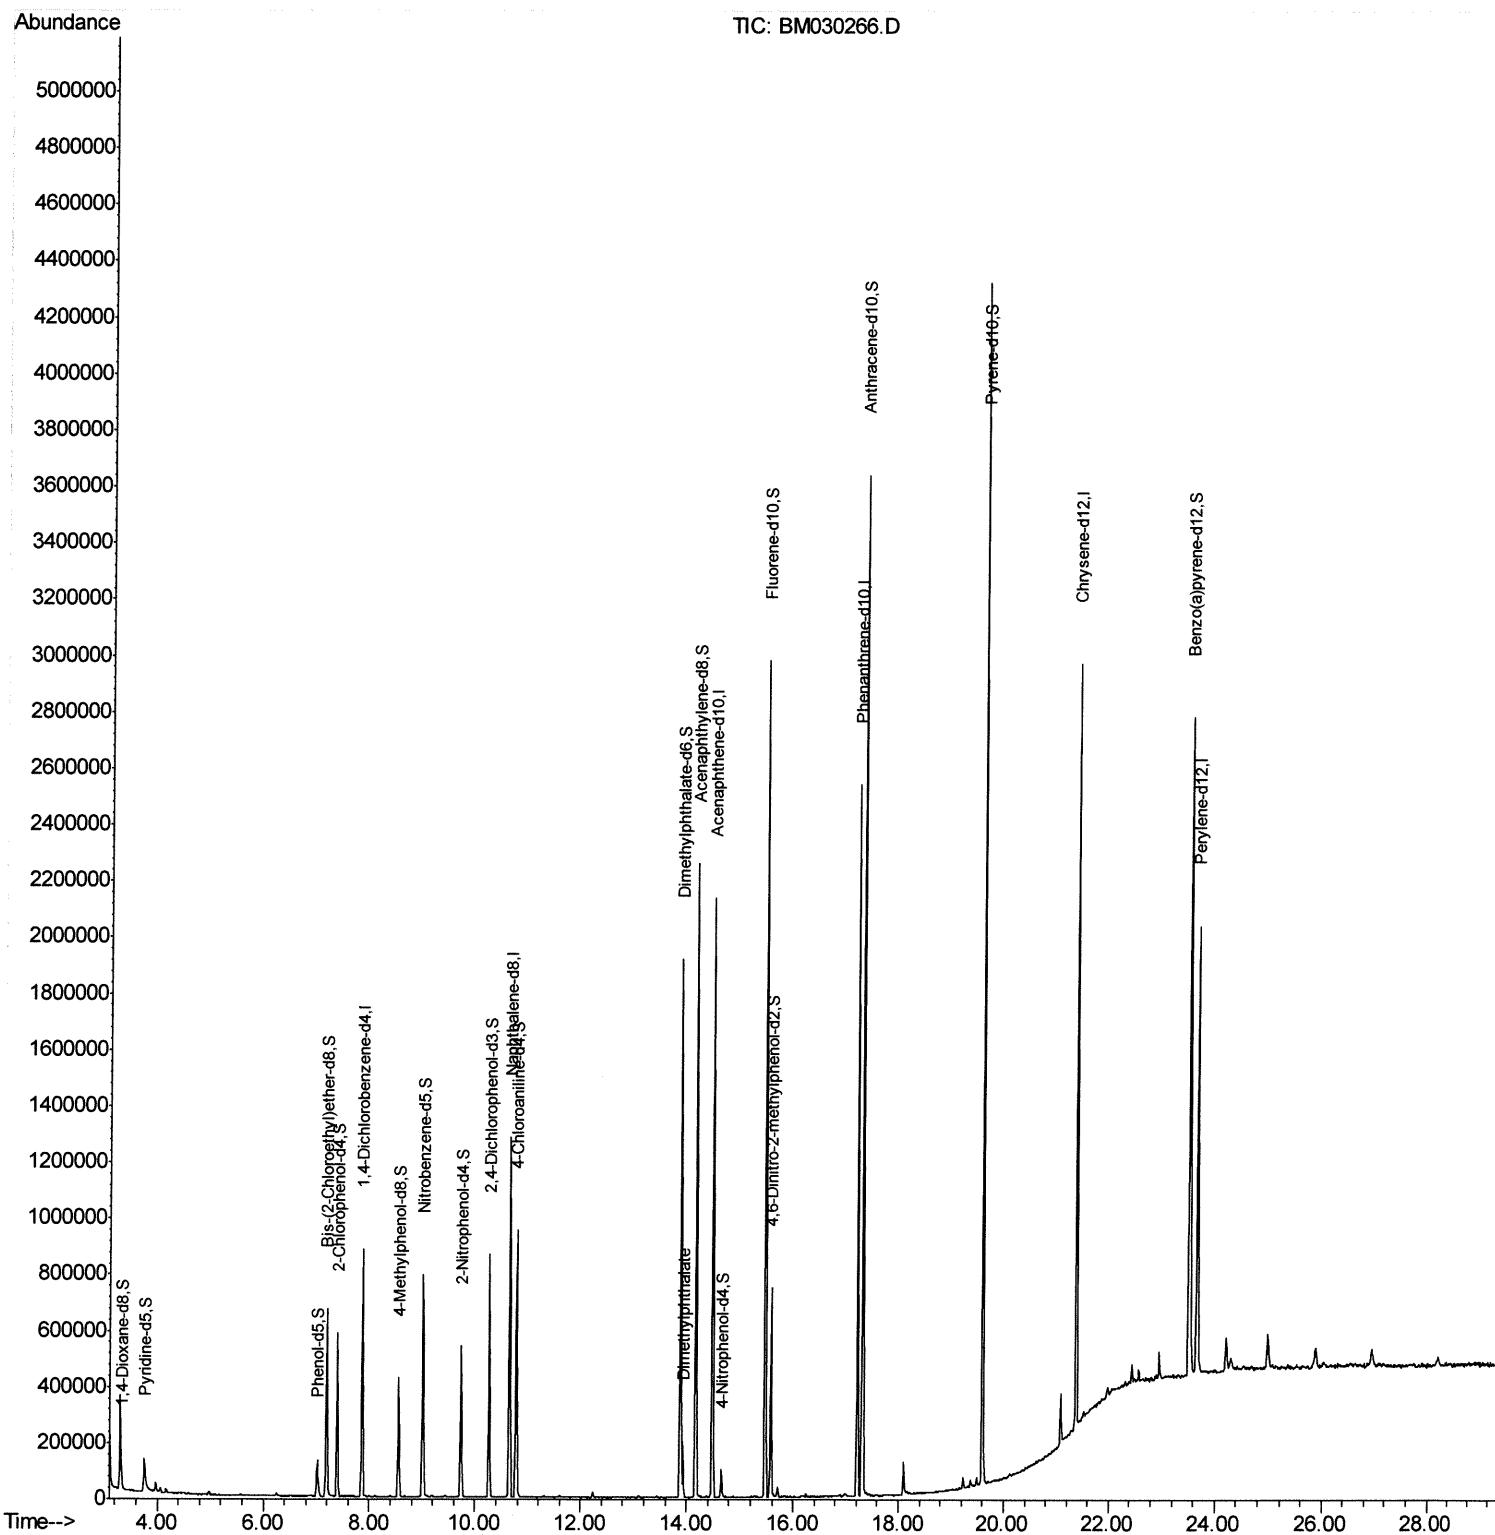




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060221\
 Data File : BM030266.D
 Acq On : 02 Jun 2021 19:16
 Operator : CG/JU
 Sample : M2568-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GN0

Manual Integrations
 APPROVED

mohammad
 6/3/2021 11:06:15 AM

Quant Time: Jun 03 01:06:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration

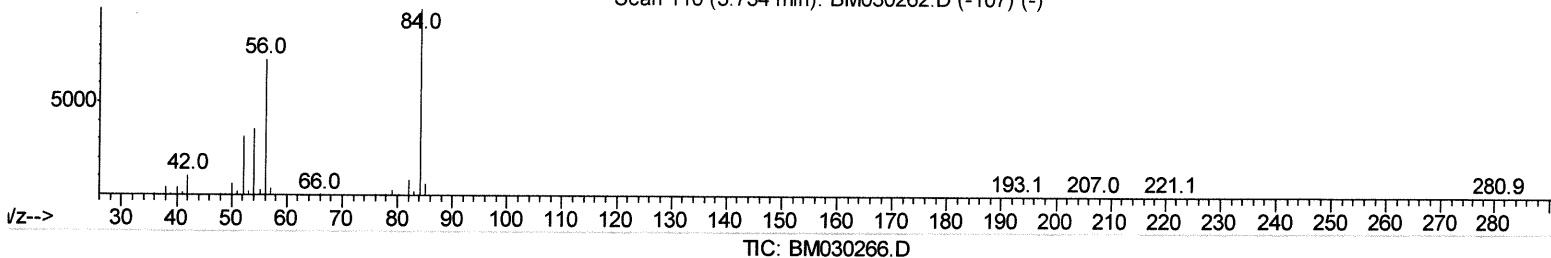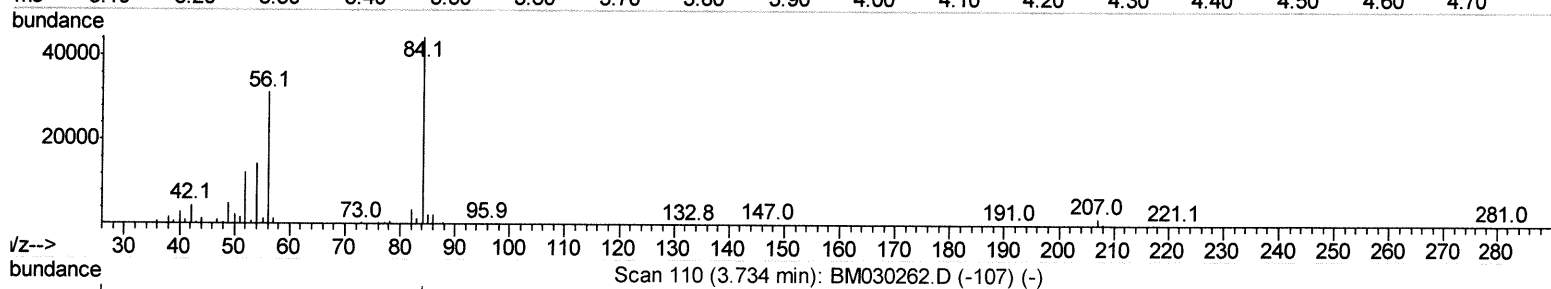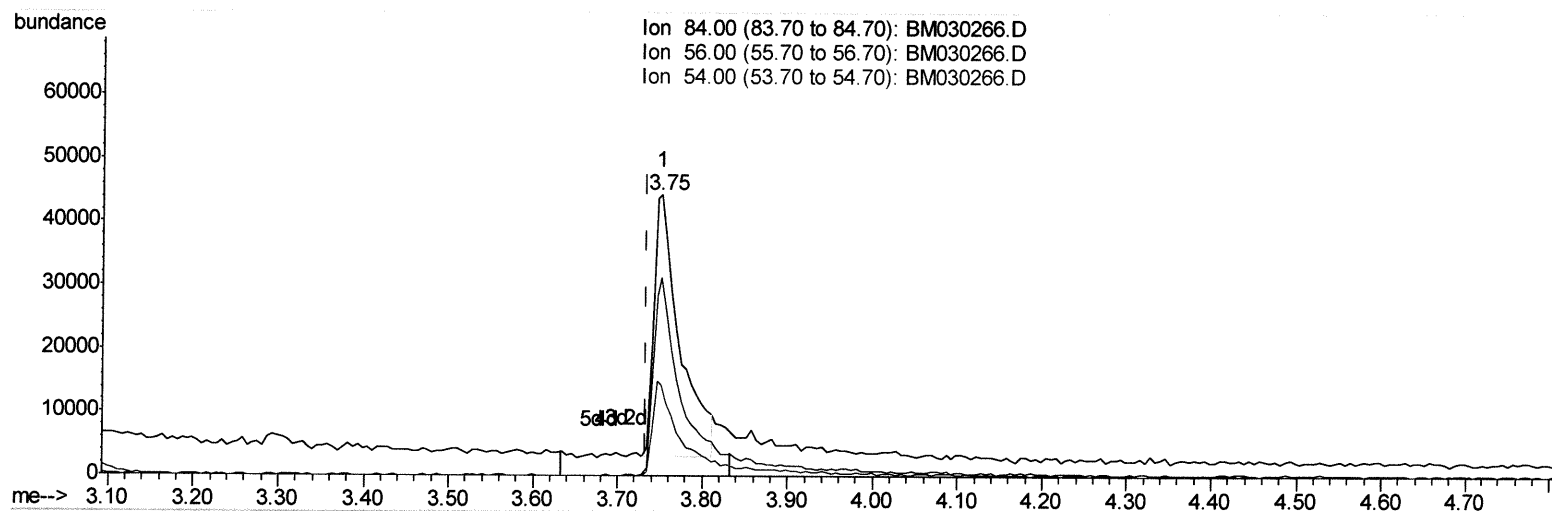

(4) Pyridine-d5 (S)

3.751min (+0.018) 5.42ng/ul

response 88748

Ion	Exp%	Act%
84.00	100	100
56.00	72.30	70.65
54.00	35.20	32.49
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060221\
 Data File : BM030266.D
 Acq On : 02 Jun 2021 19:16
 Operator : CG/JU
 Sample : M2568-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GN0

Manual Integrations
 APPROVED

mohammad
 6/3/2021 11:06:15 AM

Quant Time: Jun 03 01:06:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration

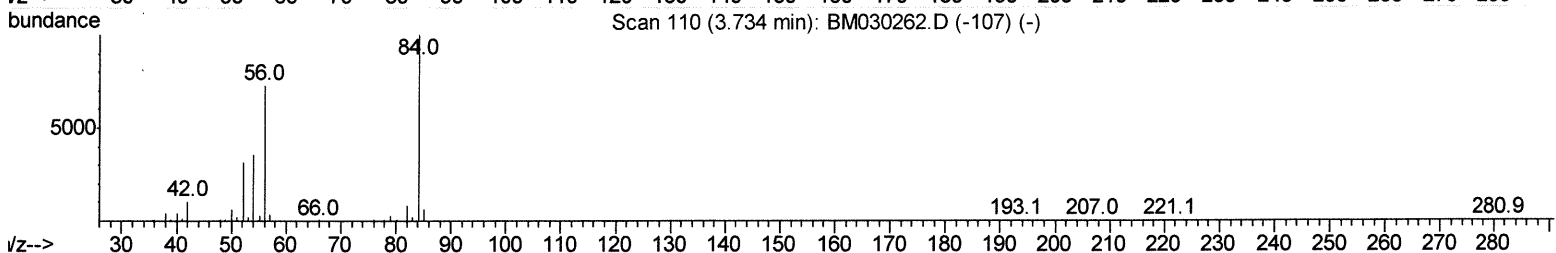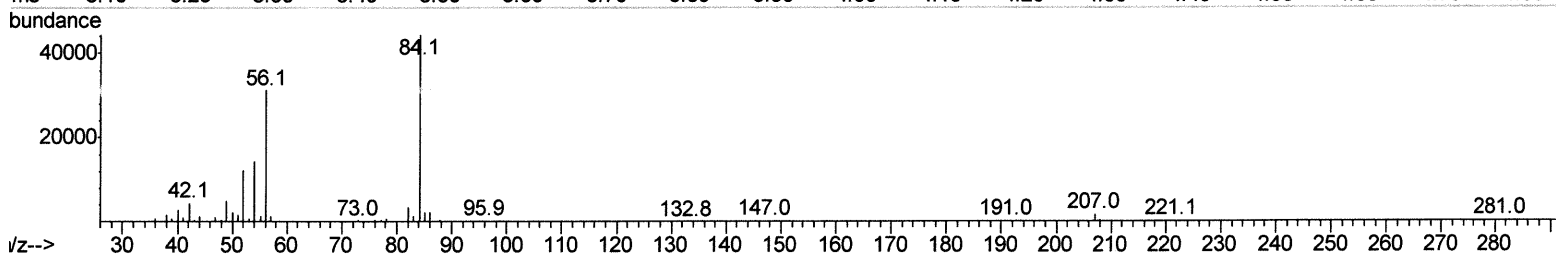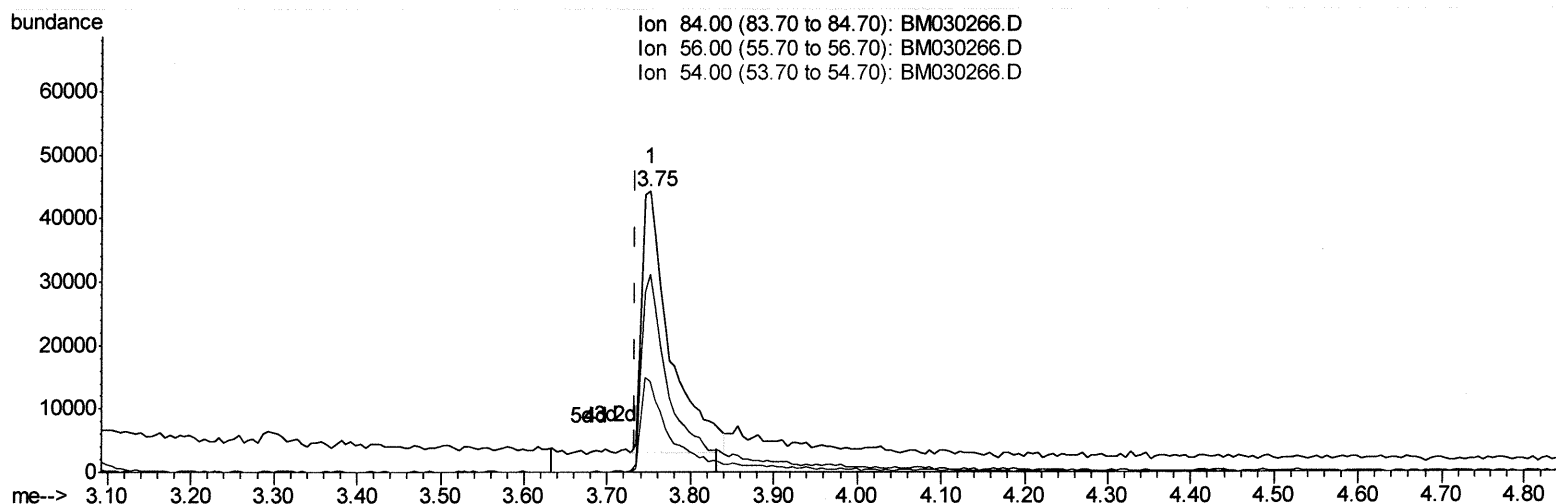

TIC: BM030266.D

(4) Pyridine-d5 (S)

3.751min (+0.018) 5.94ng/ul m

response 97203

Ju 6/03/21

Ion	Exp%	Act%
84.00	100	100
56.00	72.30	70.65
54.00	35.20	32.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060221\
 Data File : BM030266.D
 Acq On : 02 Jun 2021 19:16
 Operator : CG/JU
 Sample : M2568-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COGN0

Manual Integrations
 APPROVED

mohammad
 6/3/2021 11:06:15 AM

Quant Time: Jun 03 01:31:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	238952	20.00	ng/ul	0.00
20) Naphthalene-d8	10.65	136	1038737	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.48	164	696063	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.22	188	1429956	20.00	ng/ul	0.00
79) Chrysene-d12	21.37	240	1178284	20.00	ng/ul	0.00
88) Perylene-d12	23.66	264	1050242	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.32	96	23950	4.10	ng/uL	0.00
4) Pyridine-d5	3.75	84	97203m	5.94	ng/ul	0.02
7) Phenol-d5	7.02	99	69000	3.28	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.19	67	312874	23.59	ng/ul	0.00
11) 2-Chlorophenol-d4	7.39	132	253466	16.11	ng/ul	0.00
15) 4-Methylphenol-d8	8.55	113	147960	8.87	ng/ul	0.00
21) Nitrobenzene-d5	9.02	128	174056	25.67	ng/ul	0.00
24) 2-Nitrophenol-d4	9.73	143	157656	24.41	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.26	165	307439	18.45	ng/ul	0.00
31) 4-Chloroaniline-d4	10.78	131	478492	19.34	ng/ul	0.00
46) Dimethylphthalate-d6	13.89	166	1237716	23.26	ng/ul	0.00
49) Acenaphthylene-d8	14.17	160	1503301	21.92	ng/ul	0.00
54) 4-Nitrophenol-d4	14.66	143	22096	2.57	ng/ul	0.00
60) Fluorene-d10	15.47	176	1132008	24.37	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.58	200	150231	21.67	ng/ul	0.00
73) Anthracene-d10	17.32	188	1906883	26.94	ng/ul	0.00
81) Pyrene-d10	19.60	212	1999505	31.66	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.51	264	1558796	26.18	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.93	163	117032	2.226	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

74 6/3/21