


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060221\
Data File : BM030267.D
Acq On : 02 Jun 2021 19:53
Operator : CG/JU
Sample : M2568-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GM9

Quant Time: Jun 03 01:38:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 02 17:27:46 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/3/2021 11:06:21 AM

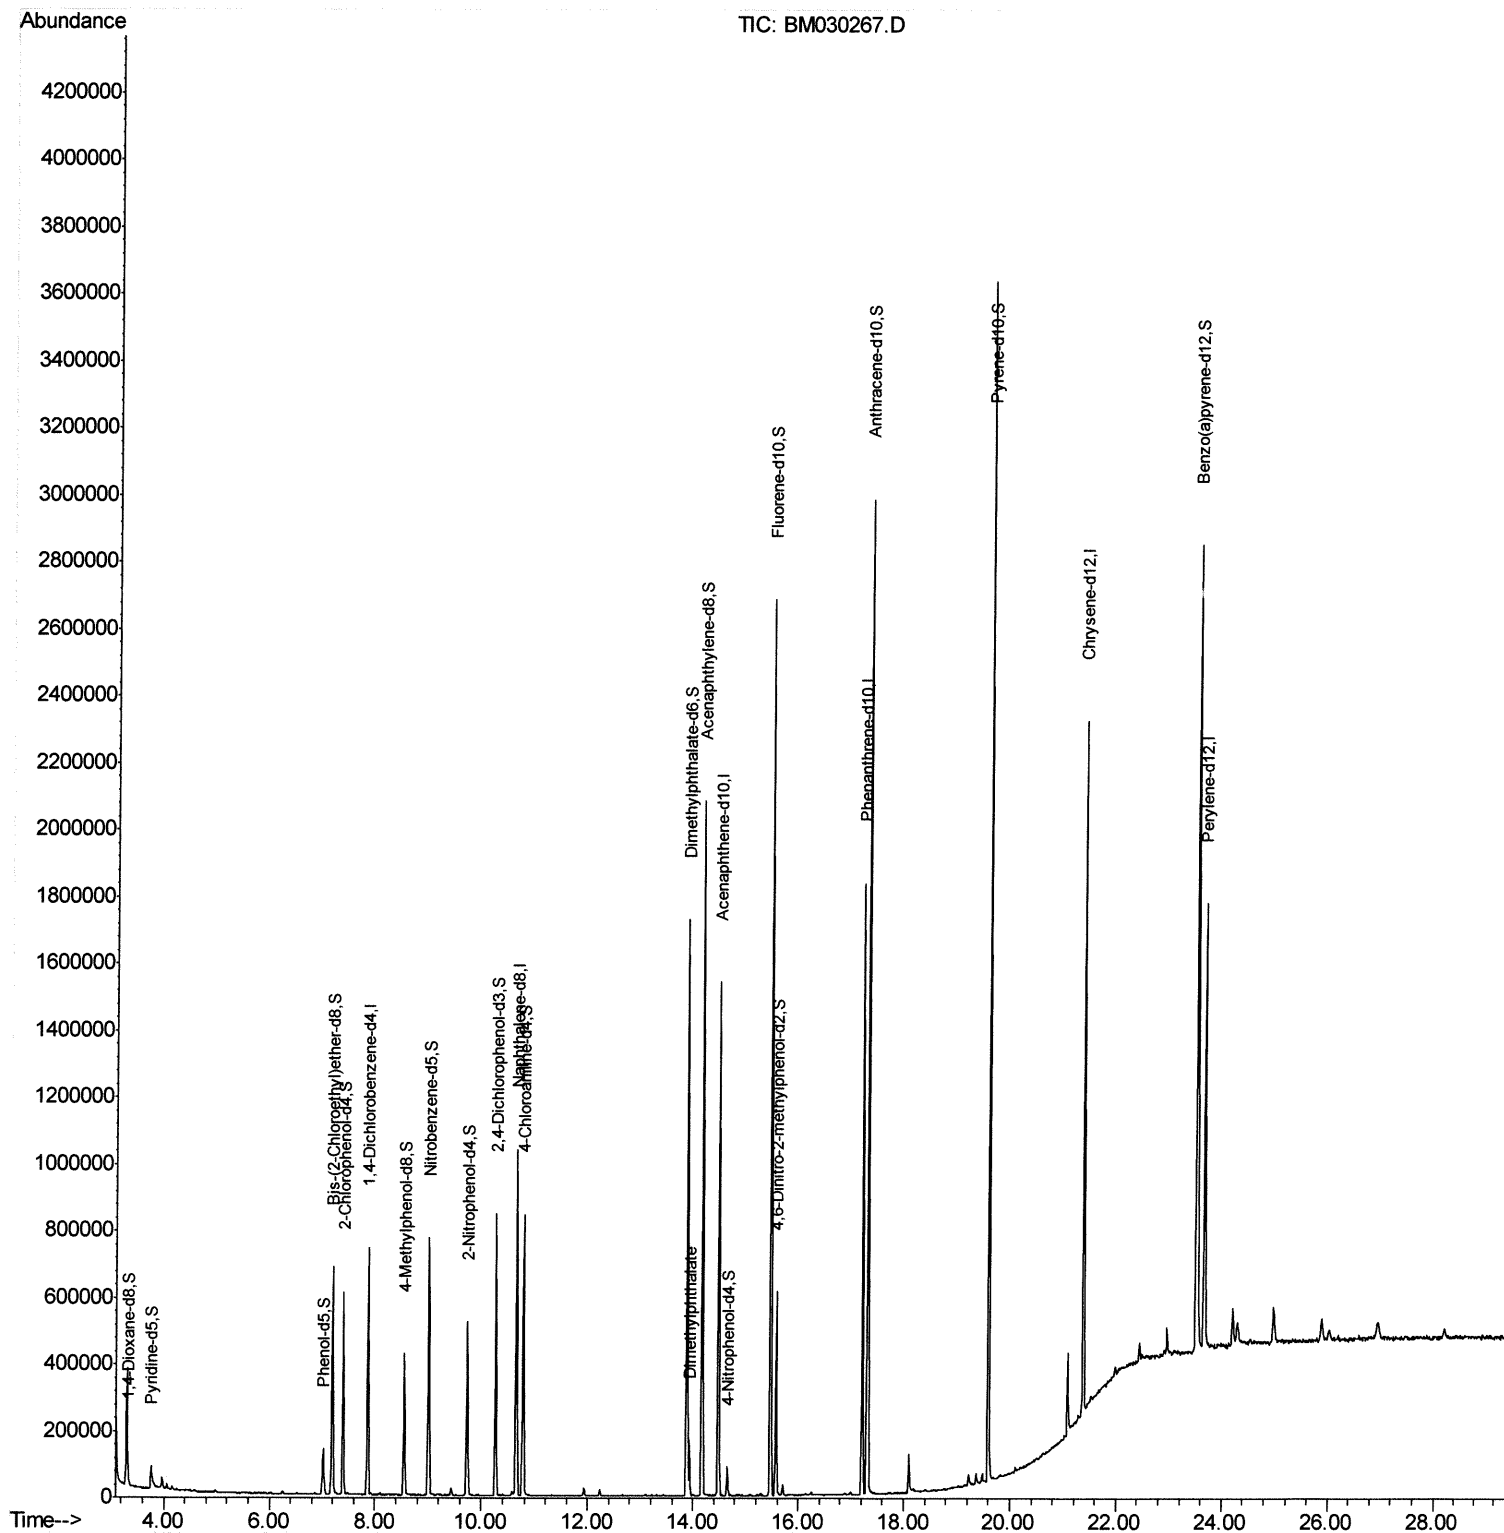




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060221\
 Data File : BM030267.D
 Acq On : 02 Jun 2021 19:53
 Operator : CG/JU
 Sample : M2568-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GM9

Manual Integrations
 APPROVED

mohammad
 6/3/2021 11:06:21 AM

Quant Time: Jun 03 01:37:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration

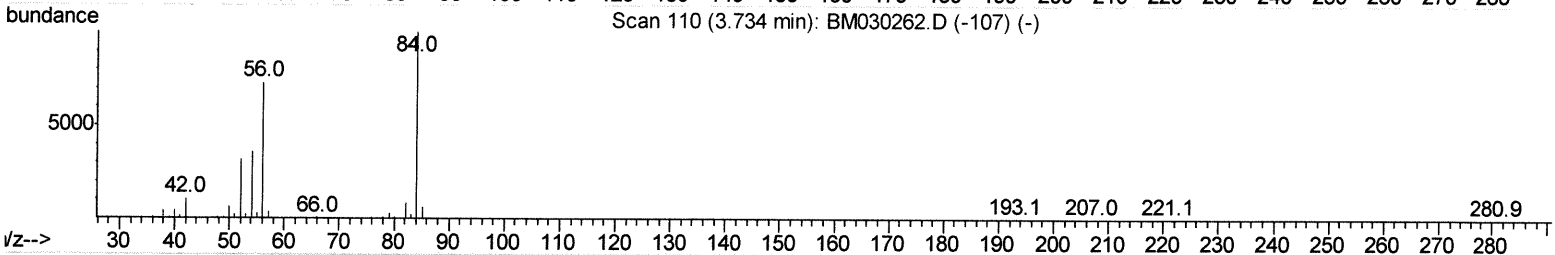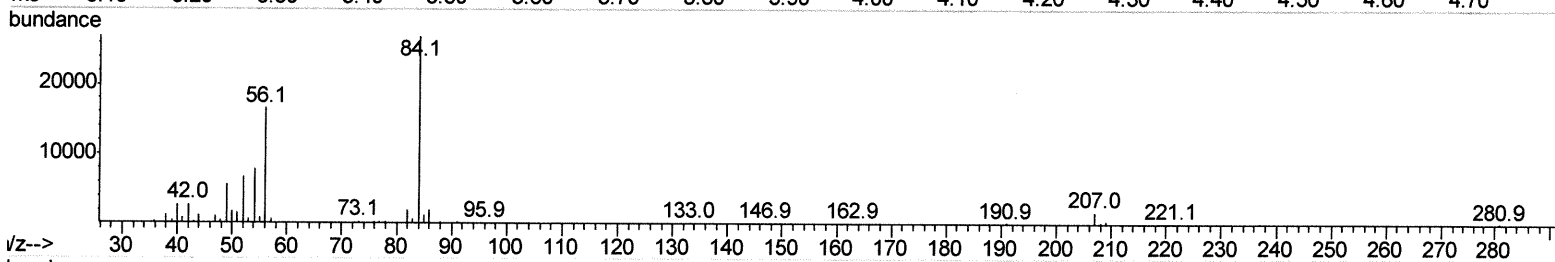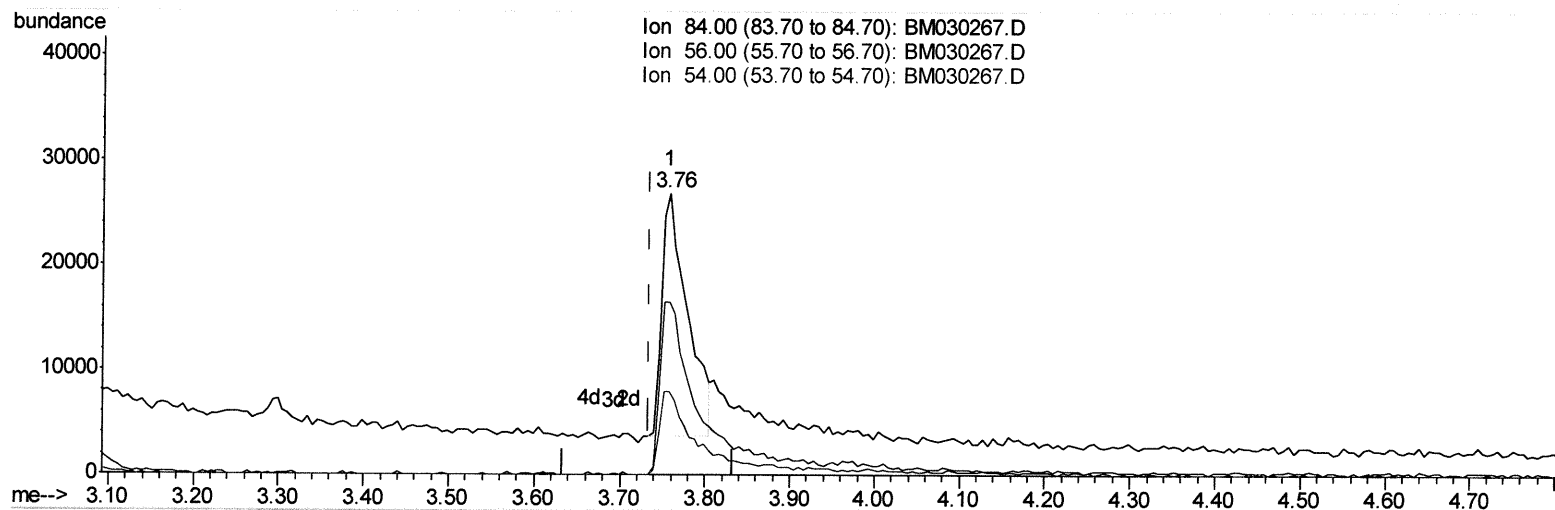

TIC: BM030267.D

(4) Pyridine-d5 (S)

3.757min (+0.024) 3.52ng/ul

response 48366

Ion	Exp%	Act%
84.00	100	100
56.00	72.30	61.57
54.00	35.20	29.49
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060221\
 Data File : BM030267.D
 Acq On : 02 Jun 2021 19:53
 Operator : CG/JU
 Sample : M2568-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GM9

Manual Integrations
 APPROVED

mohammad
 6/3/2021 11:06:21 AM

Quant Time: Jun 03 01:37:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration

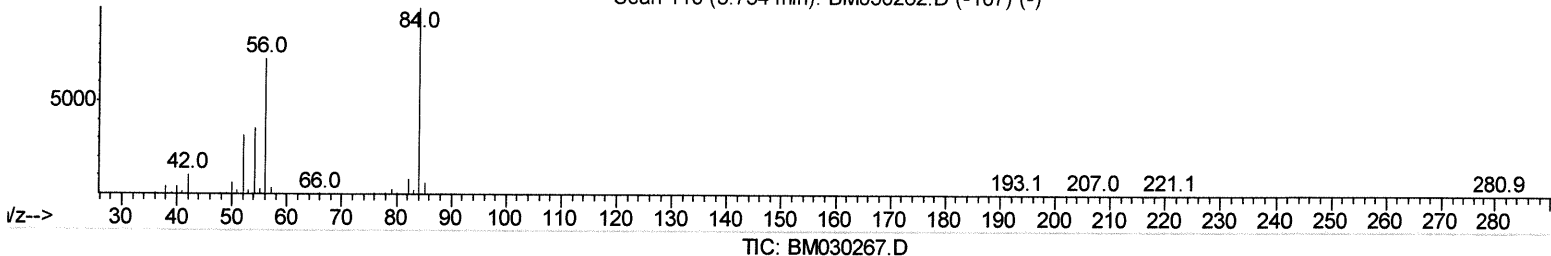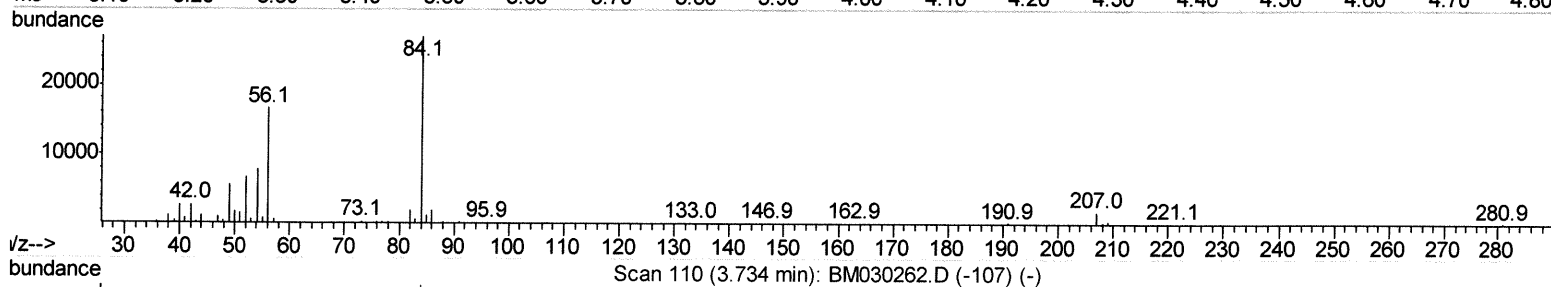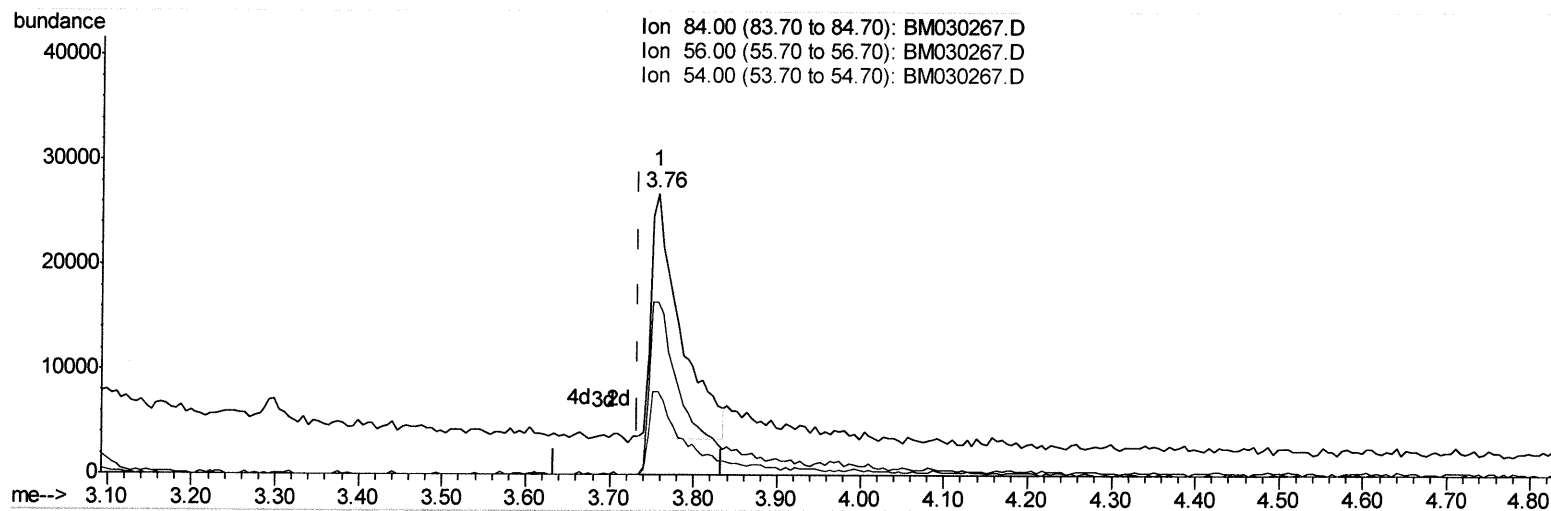

(4) Pyridine-d5 (S)

3.757min (+0.024) 4.12ng/ul m

JU 6/3/21

response 56540

Ion	Exp%	Act%
84.00	100	100
56.00	72.30	61.57
54.00	35.20	29.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060221\
 Data File : BM030267.D
 Acq On : 02 Jun 2021 19:53
 Operator : CG/JU
 Sample : M2568-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GM9

Manual Integrations
 APPROVED

mohammad
 6/3/2021 11:06:21 AM

Quant Time: Jun 03 01:38:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	200512	20.00	ng/ul	0.00
20) Naphthalene-d8	10.65	136	842143	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.48	164	519800	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.22	188	1006934	20.00	ng/ul	0.00
79) Chrysene-d12	21.37	240	893422	20.00	ng/ul	0.00
88) Perylene-d12	23.66	264	903442	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	20773	4.24	ng/uL	0.00
4) Pvrindine-d5	3.76	84	56540m	4.12	ng/ul	0.02
7) Phenol-d5	7.02	99	71564	4.06	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.19	67	316279	28.42	ng/ul	0.00
11) 2-Chlorophenol-d4	7.39	132	261284	19.79	ng/ul	0.00
15) 4-Methylphenol-d8	8.55	113	148999	10.64	ng/ul	0.00
21) Nitrobenzene-d5	9.02	128	171659	31.23	ng/ul	0.00
24) 2-Nitrophenol-d4	9.73	143	156369	29.87	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.26	165	304290	22.53	ng/ul	0.00
31) 4-Chloroaniline-d4	10.78	131	431771	21.52	ng/ul	0.00
46) Dimethylphthalate-d6	13.89	166	1125286	28.32	ng/ul	0.00
49) Acenaphthylene-d8	14.17	160	1385445	27.05	ng/ul	0.00
54) 4-Nitrophenol-d4	14.66	143	18691	2.91	ng/ul	0.00
60) Fluorene-d10	15.47	176	1018859	29.37	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.58	200	123879	25.38	ng/ul	0.00
73) Anthracene-d10	17.32	188	1607840	32.26	ng/ul	0.00
81) Pyrene-d10	19.60	212	1694957	35.39	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.51	264	1636082	31.95	ng/ul	0.00

JY 6/03/21

Target Compounds					Ovalue	
47) Dimethylphthalate	13.93	163	100541	2.561	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed