

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030265.D
 Acq On : 02 Jun 2021 18:40
 Operator : CG/JU
 Sample : M2568-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GN4

Quant Time: Jun 03 01:06:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	204317	20.00	ng/ul	0.00
20) Naphthalene-d8	10.651	136	849066	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.480	164	526718	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.215	188	1007691	20.00	ng/ul	0.00
79) Chrysene-d12	21.374	240	874166	20.00	ng/ul	0.00
88) Perylene-d12	23.662	264	864232	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	1288916	258.19	ng/uL	-0.03
4) Pyridine-d5	3.752	84	64577	4.61	ng/ul	0.02
7) Phenol-d5	7.016	99	75944	4.23	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	340602	30.04	ng/ul	0.00
11) 2-Chlorophenol-d4	7.393	132	278836	20.72	ng/ul	0.00
15) 4-Methylphenol-d8	8.551	113	157674	11.05	ng/ul	0.00
21) Nitrobenzene-d5	9.016	128	186199	33.60	ng/ul	0.00
24) 2-Nitrophenol-d4	9.734	143	171358	32.46	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.263	165	326387	23.96	ng/ul	0.00
31) 4-Chloroaniline-d4	10.781	131	468571	23.17	ng/ul	0.00
46) Dimethylphthalate-d6	13.886	166	1228904	30.52	ng/ul	0.00
49) Acenaphthylene-d8	14.174	160	1509812	29.09	ng/ul	0.00
54) 4-Nitrophenol-d4	14.657	143	19256	2.96	ng/ul	0.00
60) Fluorene-d10	15.468	176	1088245	30.96	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.580	200	136563	27.95	ng/ul	0.00
73) Anthracene-d10	17.315	188	1732367	34.73	ng/ul	0.00
81) Pyrene-d10	19.598	212	1833492	39.13	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	1717297	35.05	ng/ul	0.00
Target Compounds						
						Qvalue
8) Phenol	7.040	94	19422	1.06	ng/ul	98
47) Dimethylphthalate	13.933	163	197345	4.96	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030265.D
Acq On : 02 Jun 2021 18:40
Operator : CG/JU
Sample : M2568-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GN4

Quant Time: Jun 03 01:06:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 02 17:27:46 2021
Response via : Initial Calibration

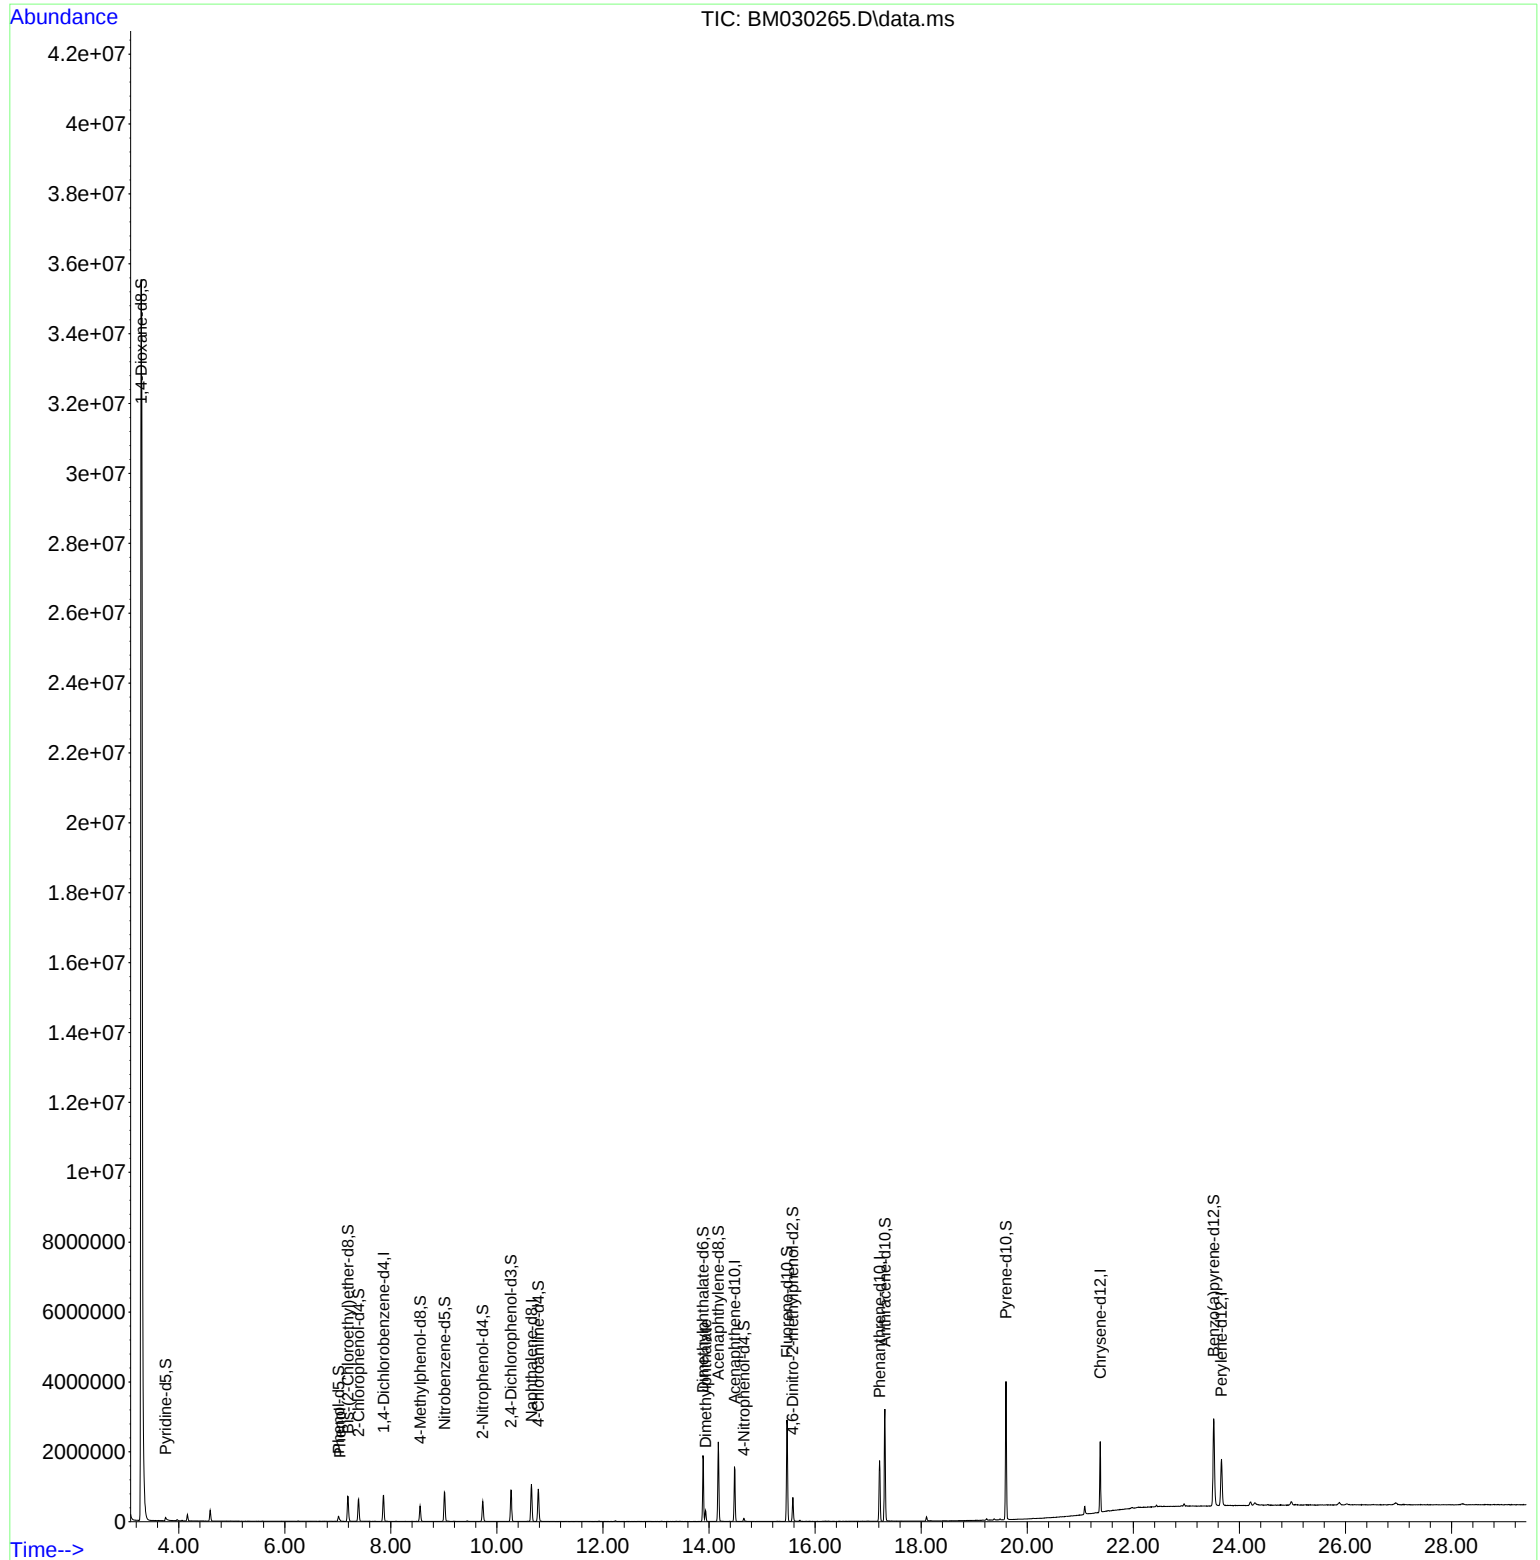




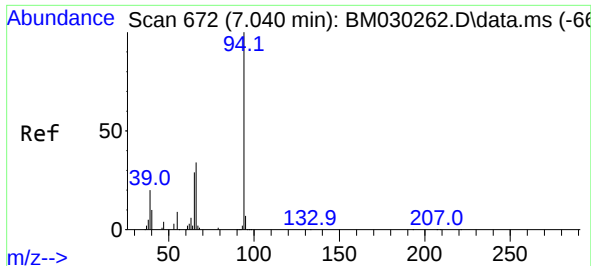


#8
Phenol
Concen: 1.06 ng/ul
RT: 7.040 min Scan# 672
Delta R.T. 0.000 min
Lab File: BM030265.D
Acq: 02 Jun 2021 18:40

Instrument :
BNA_M
ClientSampleId :
C0GN4

Tgt Ion: 94 Resp: 19422

Ion	Ratio	Lower	Upper
94	100		
65	31.1	23.3	34.9
66	36.4	29.8	44.6

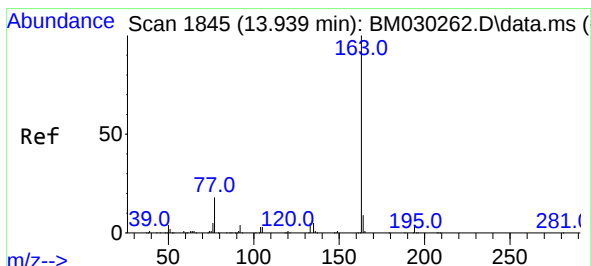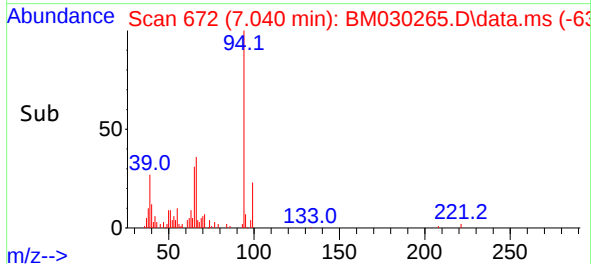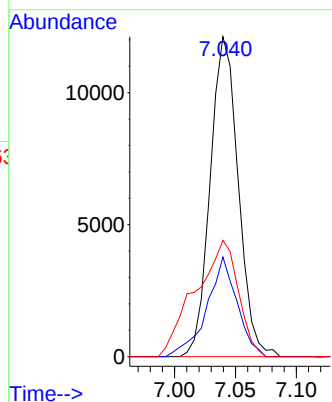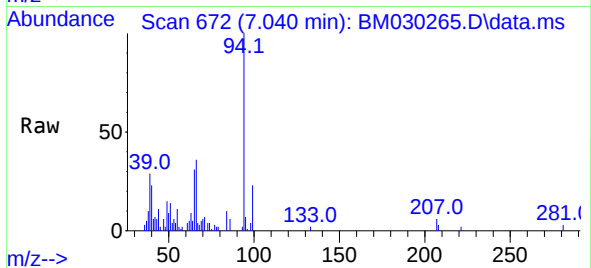

#47
Dimethylphthalate
Concen: 4.96 ng/ul
RT: 13.933 min Scan# 1844
Delta R.T. -0.006 min
Lab File: BM030265.D
Acq: 02 Jun 2021 18:40

Tgt Ion: 163 Resp: 197345

Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.0
164	10.1	8.2	12.2

