

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030266.D
 Acq On : 02 Jun 2021 19:16
 Operator : CG/JU
 Sample : M2568-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GN0

Manual Integrations
 APPROVED

mohammad
 6/3/2021 11:06:15 AM

Quant Time: Jun 03 01:06:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	238952	20.00	ng/ul	0.00
20) Naphthalene-d8	10.651	136	1038737	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.480	164	696063	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.215	188	1429956	20.00	ng/ul	0.00
79) Chrysene-d12	21.374	240	1178284	20.00	ng/ul	0.00
88) Perylene-d12	23.662	264	1050242	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	23950	4.10	ng/uL	0.00
4) Pyridine-d5	3.751	84	97203m	5.94	ng/ul	0.02
7) Phenol-d5	7.016	99	69000	3.28	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	312874	23.59	ng/ul	0.00
11) 2-Chlorophenol-d4	7.392	132	253466	16.11	ng/ul	0.00
15) 4-Methylphenol-d8	8.551	113	147960	8.87	ng/ul	0.00
21) Nitrobenzene-d5	9.016	128	174056	25.67	ng/ul	0.00
24) 2-Nitrophenol-d4	9.733	143	157656	24.41	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.263	165	307439	18.45	ng/ul	0.00
31) 4-Chloroaniline-d4	10.780	131	478492	19.34	ng/ul	0.00
46) Dimethylphthalate-d6	13.886	166	1237716	23.26	ng/ul	0.00
49) Acenaphthylene-d8	14.174	160	1503301	21.92	ng/ul	0.00
54) 4-Nitrophenol-d4	14.657	143	22096	2.57	ng/ul	0.00
60) Fluorene-d10	15.468	176	1132008	24.37	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.580	200	150231	21.67	ng/ul	0.00
73) Anthracene-d10	17.315	188	1906883	26.94	ng/ul	0.00
81) Pyrene-d10	19.598	212	1999505	31.66	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	1558796	26.18	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.933	163	117032	2.23	ng/ul	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030266.D
Acq On : 02 Jun 2021 19:16
Operator : CG/JU
Sample : M2568-01
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0GN0

Manual Integrations
APPROVED


mohammad
6/3/2021 11:06:15 AM

Quant Time: Jun 03 01:06:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 02 17:27:46 2021
Response via : Initial Calibration


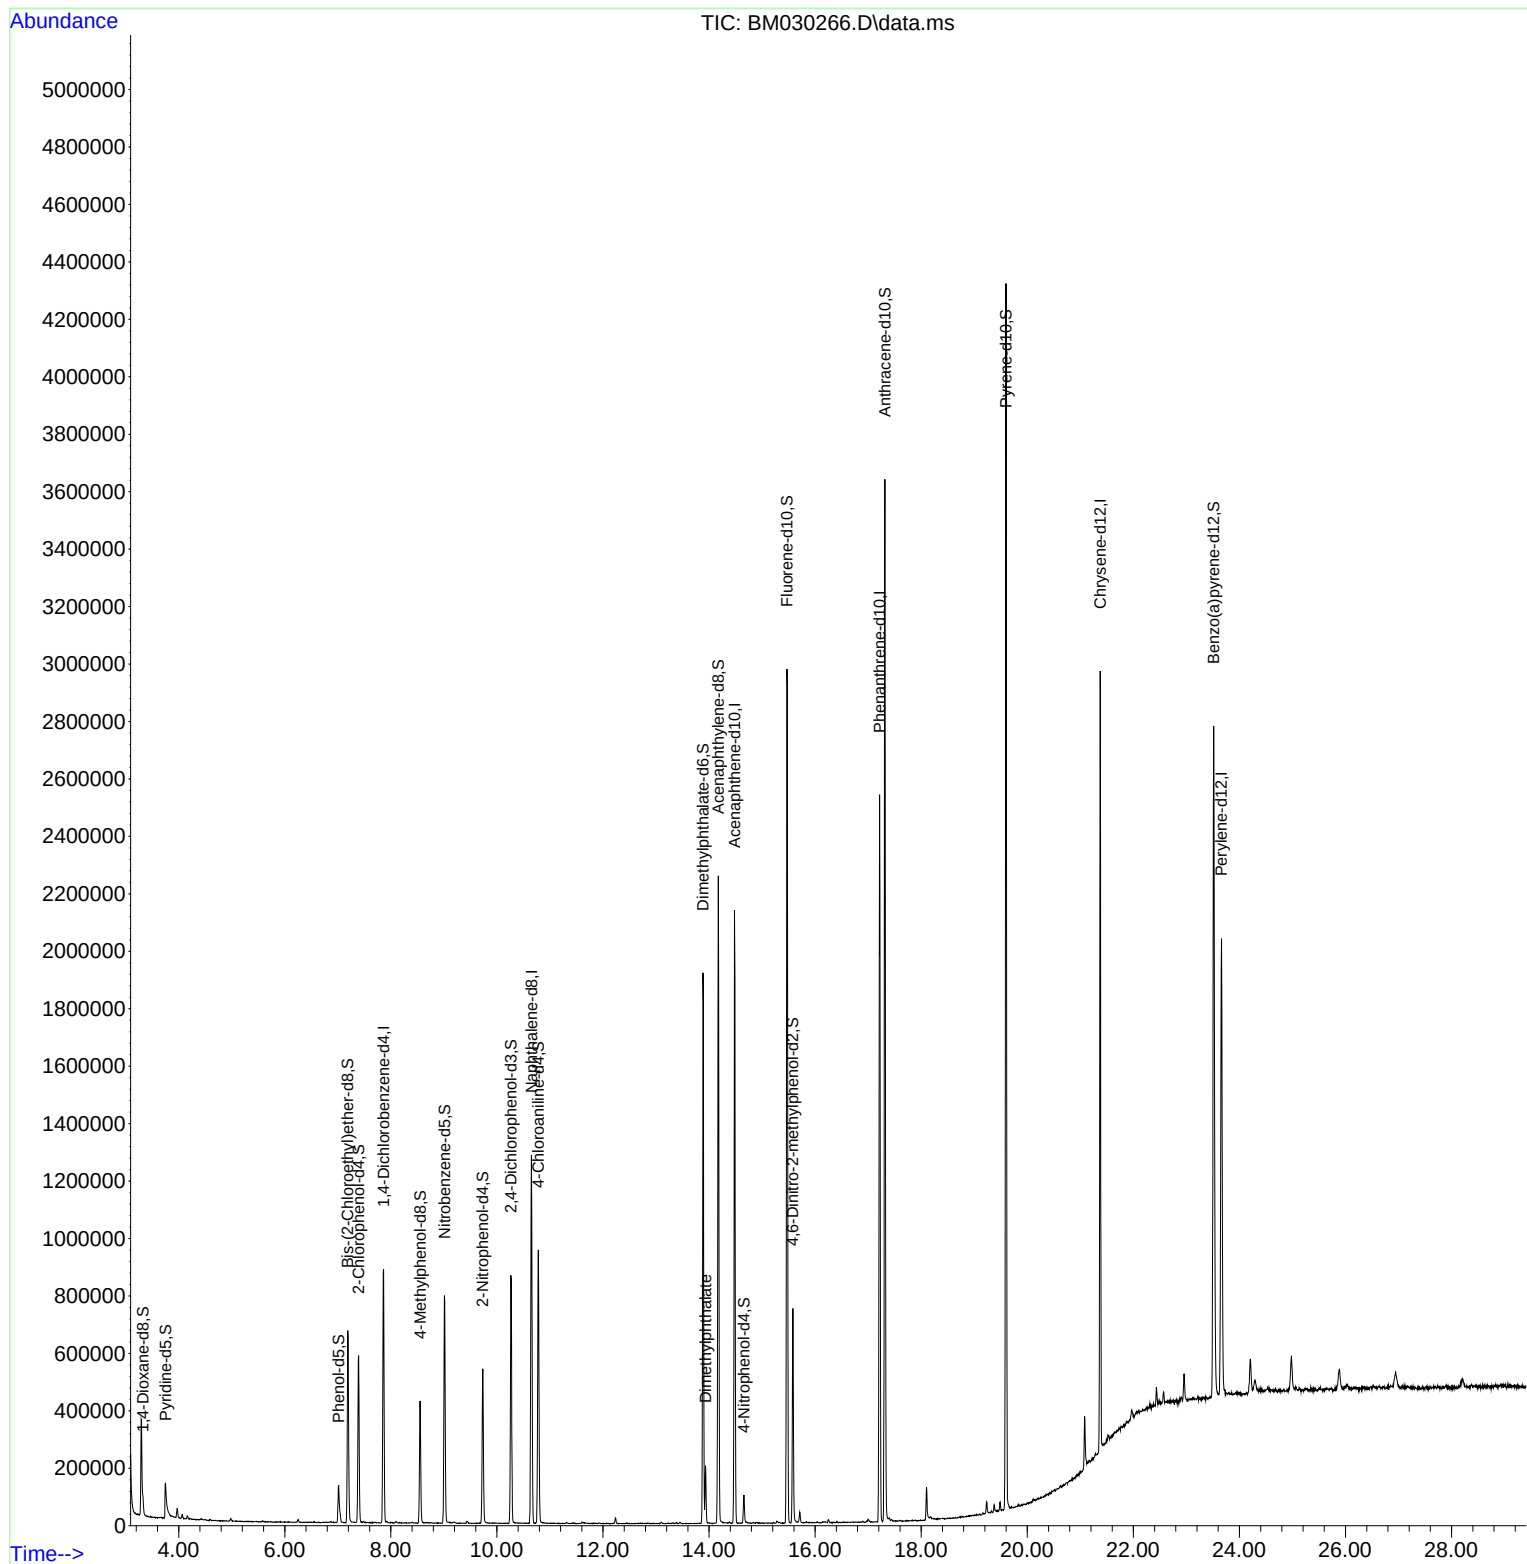


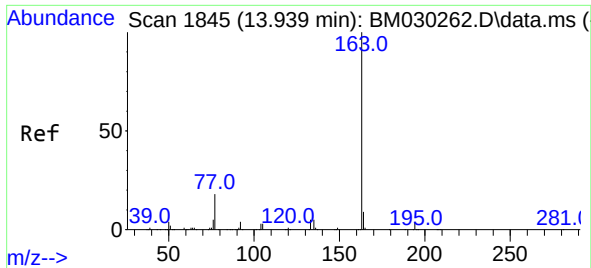

#47
 Dimethylphthalate
 Concen: 2.23 ng/ul
 RT: 13.933 min Scan# 1844
 Delta R.T. -0.006 min
 Lab File: BM030266.D
 Acq: 02 Jun 2021 19:16

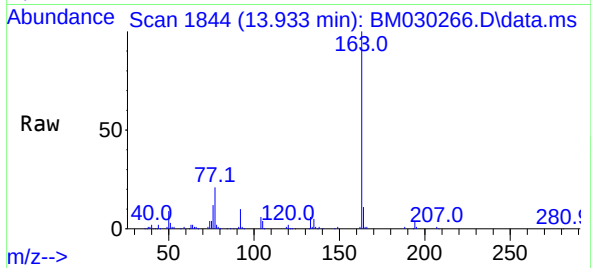

Tgt Ion:163 Resp: 117032
 Ion Ratio Lower Upper
 163 100
 194 3.7 3.4 5.0
 164 10.9 8.2 12.2

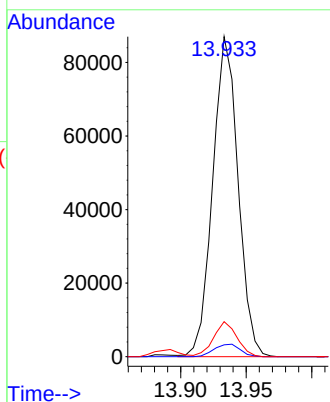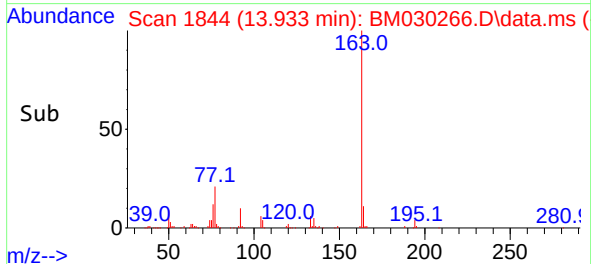

Instrument :
 BNA_M
 ClientSampleId :
 C0GN0

Manual Integrations
 APPROVED

mohammad
 6/3/2021 11:06:15 AM