

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030267.D
 Acq On : 02 Jun 2021 19:53
 Operator : CG/JU
 Sample : M2568-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GM9

Manual Integrations
 APPROVED

mohammad
 6/3/2021 11:06:21 AM

Quant Time: Jun 03 01:06:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	200512	20.00	ng/ul	0.00
20) Naphthalene-d8	10.651	136	842143	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.480	164	519800	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.215	188	1006934	20.00	ng/ul	0.00
79) Chrysene-d12	21.374	240	893422	20.00	ng/ul	0.00
88) Perylene-d12	23.662	264	903442	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	20773	4.24	ng/uL	0.00
4) Pyridine-d5	3.757	84	56540m	4.12	ng/ul	0.02
7) Phenol-d5	7.016	99	71564	4.06	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	316279	28.42	ng/ul	0.00
11) 2-Chlorophenol-d4	7.393	132	261284	19.79	ng/ul	0.00
15) 4-Methylphenol-d8	8.551	113	148999	10.64	ng/ul	0.00
21) Nitrobenzene-d5	9.016	128	171659	31.23	ng/ul	0.00
24) 2-Nitrophenol-d4	9.734	143	156369	29.87	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.263	165	304290	22.53	ng/ul	0.00
31) 4-Chloroaniline-d4	10.781	131	431771	21.52	ng/ul	0.00
46) Dimethylphthalate-d6	13.886	166	1125286	28.32	ng/ul	0.00
49) Acenaphthylene-d8	14.174	160	1385445	27.05	ng/ul	0.00
54) 4-Nitrophenol-d4	14.657	143	18691	2.91	ng/ul	0.00
60) Fluorene-d10	15.468	176	1018859	29.37	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.580	200	123879	25.38	ng/ul	0.00
73) Anthracene-d10	17.315	188	1607840	32.26	ng/ul	0.00
81) Pyrene-d10	19.598	212	1694957	35.39	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	1636082	31.95	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.933	163	100541	2.56	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030267.D
Acq On : 02 Jun 2021 19:53
Operator : CG/JU
Sample : M2568-04
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0GM9

Manual Integrations
APPROVED

mohammad
6/3/2021 11:06:21 AM

Quant Time: Jun 03 01:06:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 02 17:27:46 2021
Response via : Initial Calibration

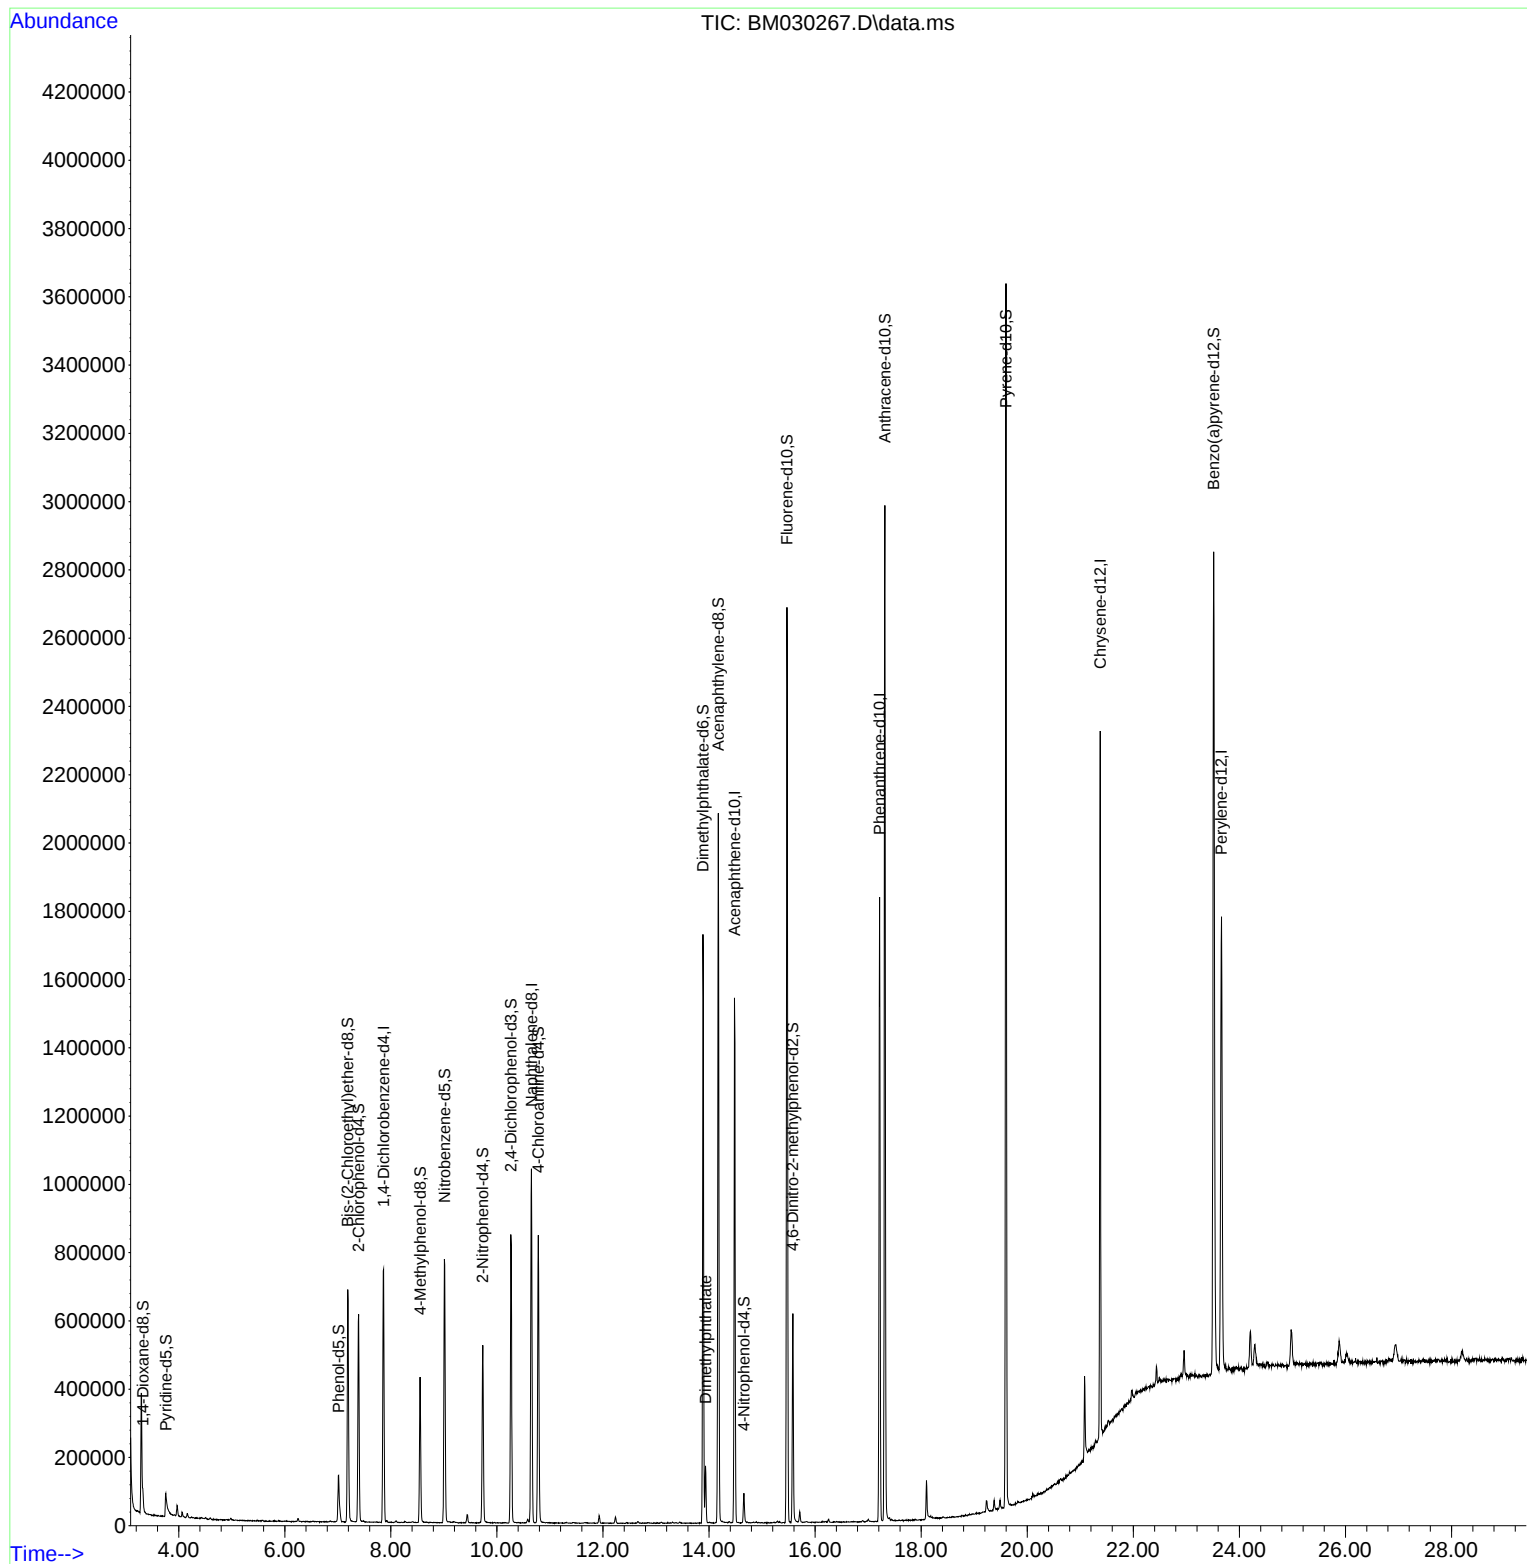

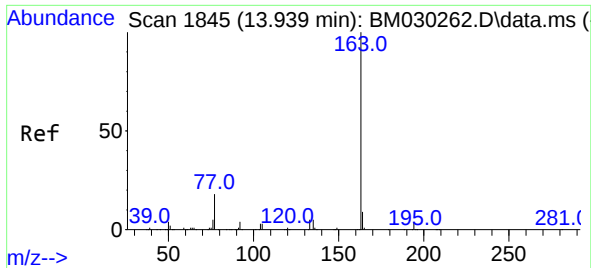

#47
 Dimethylphthalate
 Concen: 2.56 ng/ul
 RT: 13.933 min Scan# 1844
 Delta R.T. -0.006 min
 Lab File: BM030267.D
 Acq: 02 Jun 2021 19:53

Tgt Ion:163 Resp: 100541
 Ion Ratio Lower Upper
 163 100
 194 4.6 3.4 5.0
 164 10.1 8.2 12.2

Instrument :
 BNA_M
 ClientSampleId :
 C0GM9

Manual Integrations
 APPROVED

mohammad
 6/3/2021 11:06:21 AM

