

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030268.D
 Acq On : 02 Jun 2021 20:30
 Operator : CG/JU
 Sample : M2568-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GN3


Quant Time: Jun 03 01:06:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	219872	20.00	ng/ul	0.00
20) Naphthalene-d8	10.651	136	955462	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.480	164	651370	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.215	188	1335598	20.00	ng/ul	0.00
79) Chrysene-d12	21.374	240	1123316	20.00	ng/ul	0.00
88) Perylene-d12	23.662	264	997317	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	1291190	240.34	ng/uL	-0.03
4) Pyridine-d5	3.746	84	97251	6.46	ng/ul	0.01
7) Phenol-d5	7.016	99	94220	4.87	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	382822	31.37	ng/ul	0.00
11) 2-Chlorophenol-d4	7.392	132	319459	22.06	ng/ul	0.00
15) 4-Methylphenol-d8	8.551	113	196446	12.80	ng/ul	0.00
21) Nitrobenzene-d5	9.010	128	217079	34.81	ng/ul	0.00
24) 2-Nitrophenol-d4	9.733	143	199542	33.59	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.263	165	391415	25.54	ng/ul	0.00
31) 4-Chloroaniline-d4	10.780	131	578829	25.43	ng/ul	0.00
46) Dimethylphthalate-d6	13.886	166	1583244	31.79	ng/ul	0.00
49) Acenaphthylene-d8	14.174	160	1917474	29.87	ng/ul	0.00
54) 4-Nitrophenol-d4	14.657	143	30662	3.81	ng/ul	0.00
60) Fluorene-d10	15.468	176	1428916	32.87	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.580	200	196498	30.35	ng/ul	0.00
73) Anthracene-d10	17.315	188	2371559	35.88	ng/ul	0.00
81) Pyrene-d10	19.598	212	2536822	42.13	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	2013993	35.62	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.040	94	19864	1.01	ng/ul	99
47) Dimethylphthalate	13.933	163	126776	2.58	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 03 01:06:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 02 17:27:46 2021
Response via : Initial Calibration






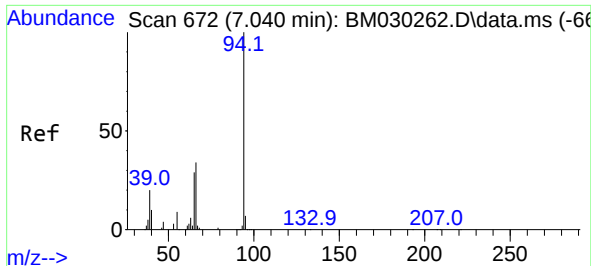


#8
Phenol
Concen: 1.01 ng/ul
RT: 7.040 min Scan# 672
Delta R.T. -0.000 min
Lab File: BM030268.D
Acq: 02 Jun 2021 20:30

Instrument :
BNA_M
ClientSampleId :
C0GN3

Tgt Ion: 94 Resp: 19864

Ion	Ratio	Lower	Upper
94	100		
65	29.9	23.3	34.9
66	36.7	29.8	44.6

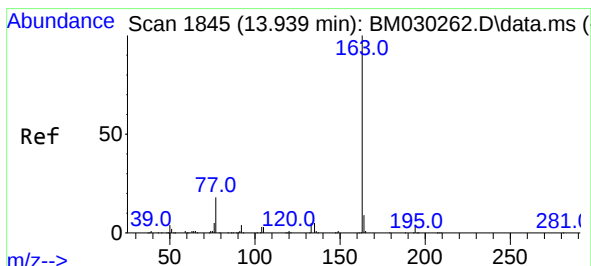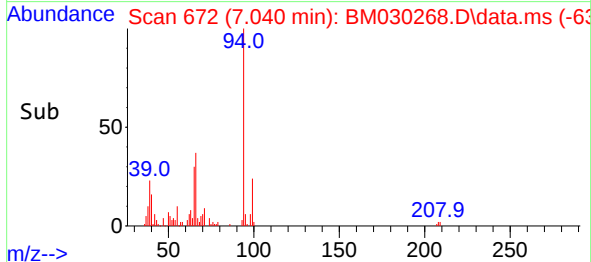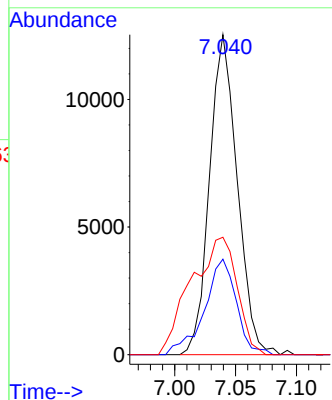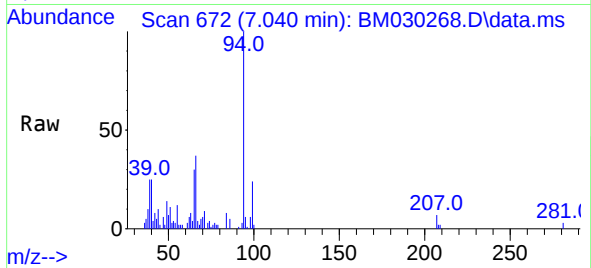

#47
Dimethylphthalate
Concen: 2.58 ng/ul
RT: 13.933 min Scan# 1844
Delta R.T. -0.006 min
Lab File: BM030268.D
Acq: 02 Jun 2021 20:30

Tgt Ion: 163 Resp: 126776

Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.4	5.0
164	10.6	8.2	12.2

