

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030269.D
 Acq On : 02 Jun 2021 21:06
 Operator : CG/JU
 Sample : M2568-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GN2

Manual Integrations
 APPROVED

mohammad
 6/3/2021 11:06:25 AM

Quant Time: Jun 03 01:07:08 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	221651	20.00	ng/ul	0.00
20) Naphthalene-d8	10.651	136	958273	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.480	164	610202	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.216	188	1168824	20.00	ng/ul	0.00
79) Chrysene-d12	21.374	240	976286	20.00	ng/ul	0.00
88) Perylene-d12	23.662	264	955619	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	21423	3.96	ng/uL	0.00
4) Pyridine-d5	3.752	84	73734m	4.86	ng/ul	0.02
7) Phenol-d5	7.010	99	80224	4.12	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	399343	32.46	ng/ul	0.00
11) 2-Chlorophenol-d4	7.393	132	305804	20.95	ng/ul	0.00
15) 4-Methylphenol-d8	8.551	113	172557	11.15	ng/ul	0.00
21) Nitrobenzene-d5	9.010	128	223114	35.67	ng/ul	0.00
24) 2-Nitrophenol-d4	9.734	143	197650	33.18	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.263	165	381358	24.81	ng/ul	0.00
31) 4-Chloroaniline-d4	10.781	131	554587	24.29	ng/ul	0.00
46) Dimethylphthalate-d6	13.886	166	1536078	32.93	ng/ul	0.00
49) Acenaphthylene-d8	14.175	160	1876266	31.20	ng/ul	0.00
54) 4-Nitrophenol-d4	14.657	143	22398	2.97	ng/ul	0.00
60) Fluorene-d10	15.469	176	1373665	33.73	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.580	200	169043	29.83	ng/ul	0.00
73) Anthracene-d10	17.316	188	2116927	36.59	ng/ul	0.00
81) Pyrene-d10	19.598	212	2159074	41.26	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	1980284	36.56	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.040	94	25519	1.29	ng/ul	95
47) Dimethylphthalate	13.933	163	216193	4.69	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030269.D
Acq On : 02 Jun 2021 21:06
Operator : CG/JU
Sample : M2568-02
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0GN2

Manual Integrations
APPROVED

mohammad
6/3/2021 11:06:25 AM

Quant Time: Jun 03 01:07:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 02 17:27:46 2021
Response via : Initial Calibration

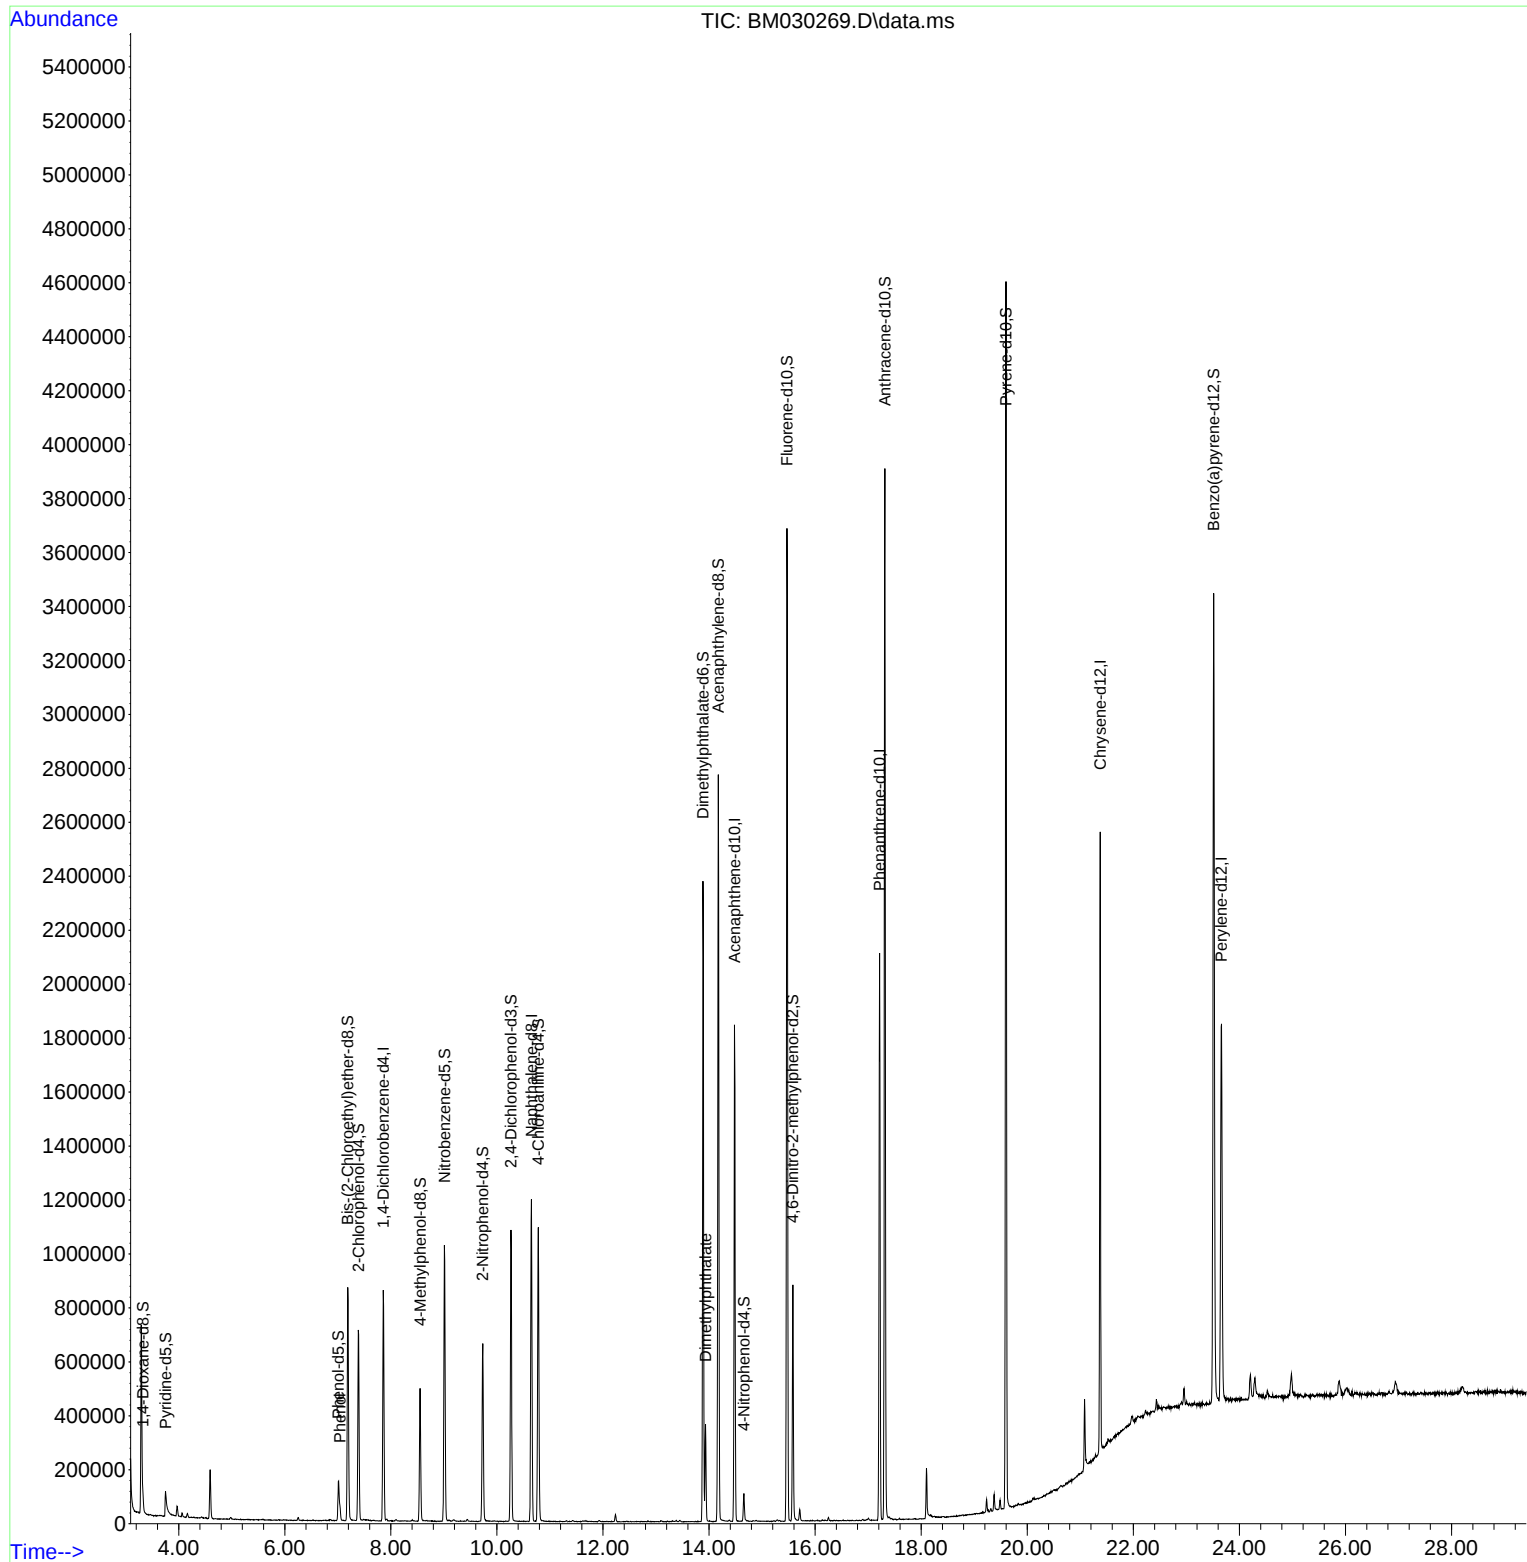

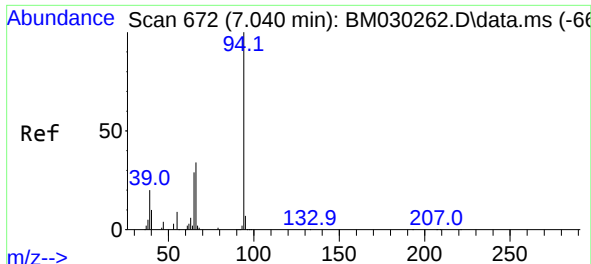





#8
Phenol
Concen: 1.29 ng/ul
RT: 7.040 min Scan# 672
Delta R.T. 0.000 min
Lab File: BM030269.D
Acq: 02 Jun 2021 21:06

Tgt Ion:	94	Resp:	25519
Ion	Ratio	Lower	Upper
94	100		
65	32.8	23.3	34.9
66	39.6	29.8	44.6

Instrument :
BNA_M
ClientSampleId :
C0GN2

Manual Integrations
APPROVED

mohammad
6/3/2021 11:06:25 AM

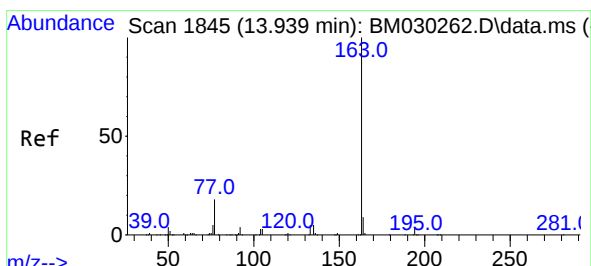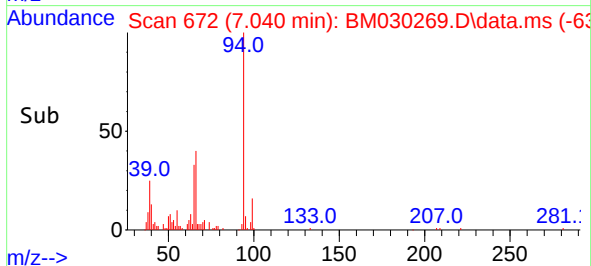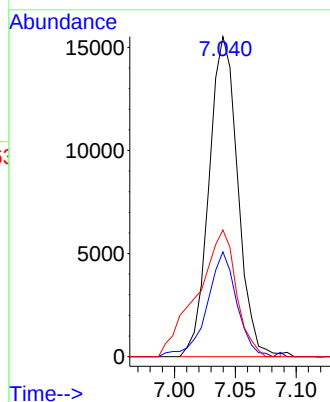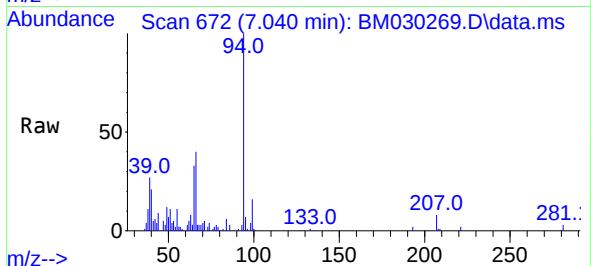

#47
Dimethylphthalate
Concen: 4.69 ng/ul
RT: 13.933 min Scan# 1844
Delta R.T. -0.006 min
Lab File: BM030269.D
Acq: 02 Jun 2021 21:06

Tgt Ion:	163	Resp:	216193
Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.0
164	10.5	8.2	12.2

