

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030270.D
 Acq On : 02 Jun 2021 21:43
 Operator : CG/JU
 Sample : M2568-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GN1

Quant Time: Jun 03 01:07:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 02 17:27:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	198760	20.00	ng/ul	0.00
20) Naphthalene-d8	10.651	136	812980	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.480	164	505869	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.215	188	974324	20.00	ng/ul	0.00
79) Chrysene-d12	21.374	240	862067	20.00	ng/ul	0.00
88) Perylene-d12	23.656	264	851343	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	18928	3.90	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	7.016	99	67139	3.84	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	301005	27.29	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	247493	18.91	ng/ul	0.00
15) 4-Methylphenol-d8	8.551	113	140219	10.10	ng/ul	0.00
21) Nitrobenzene-d5	9.010	128	164724	31.04	ng/ul	0.00
24) 2-Nitrophenol-d4	9.734	143	142855	28.27	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.263	165	284001	21.78	ng/ul	0.00
31) 4-Chloroaniline-d4	10.781	131	130659	6.75	ng/ul	0.00
46) Dimethylphthalate-d6	13.886	166	1028322	26.59	ng/ul	0.00
49) Acenaphthylene-d8	14.174	160	1267325	25.42	ng/ul	0.00
54) 4-Nitrophenol-d4	14.657	143	18751	3.00	ng/ul	0.00
60) Fluorene-d10	15.468	176	929256	27.53	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.580	200	117222	24.82	ng/ul	0.00
73) Anthracene-d10	17.315	188	1515015	31.42	ng/ul	0.00
81) Pyrene-d10	19.598	212	1605886	34.75	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	1499632	31.07	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.040	94	25174	1.42	ng/ul	95
47) Dimethylphthalate	13.933	163	132097	3.46	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030270.D
Acq On : 02 Jun 2021 21:43
Operator : CG/JU
Sample : M2568-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GN1

Quant Time: Jun 03 01:07:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 02 17:27:46 2021
Response via : Initial Calibration




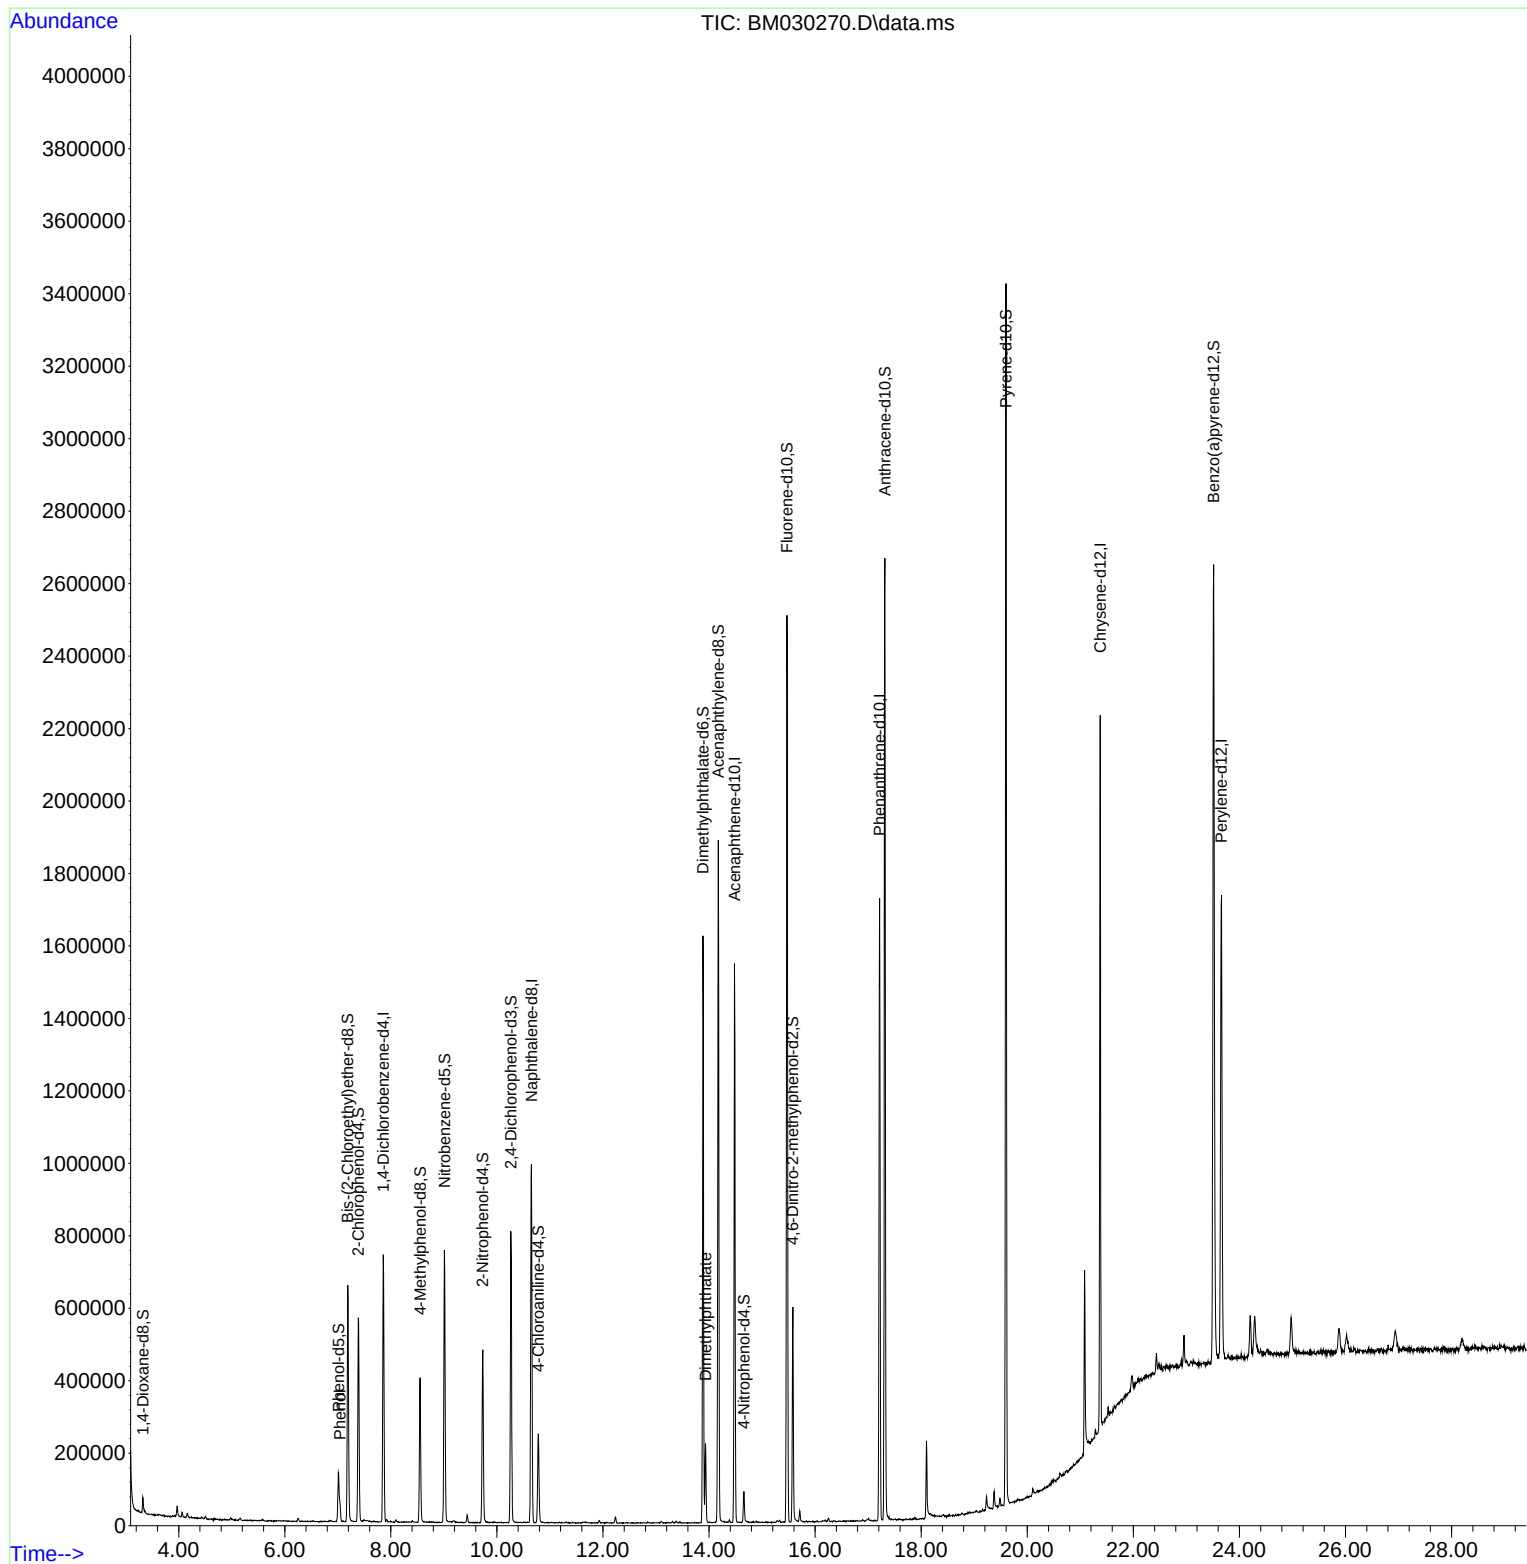


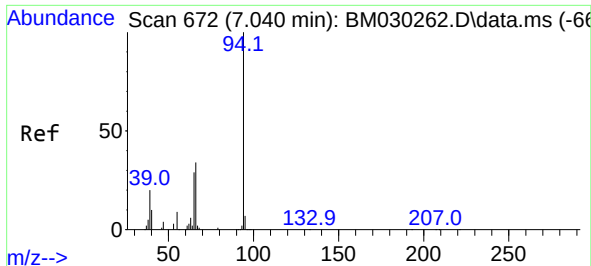

#8
Phenol
Concen: 1.42 ng/ul
RT: 7.040 min Scan# 672
Delta R.T. 0.000 min
Lab File: BM030270.D
Acq: 02 Jun 2021 21:43

Instrument :
BNA_M
ClientSampleId :
C0GN1

Tgt Ion: 94	Resp: 25174
Ion Ratio	Lower Upper
94 100	
65 31.6	23.3 34.9
66 34.0	29.8 44.6

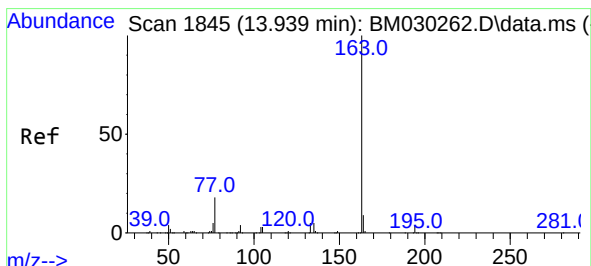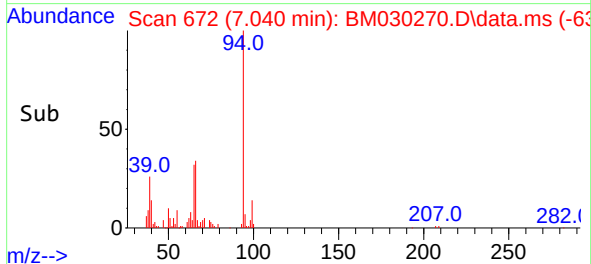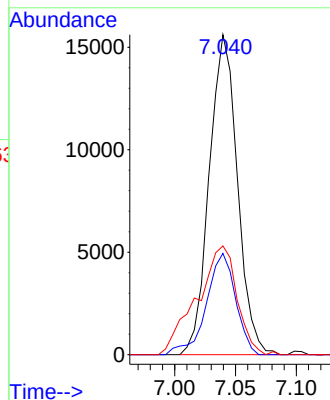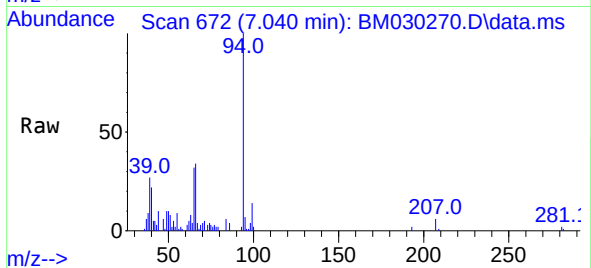

#47
Dimethylphthalate
Concen: 3.46 ng/ul
RT: 13.933 min Scan# 1844
Delta R.T. -0.006 min
Lab File: BM030270.D
Acq: 02 Jun 2021 21:43

Tgt Ion:163	Resp:	132097	
Ion	Ratio	Lower	Upper
163	100		
194	3.5	3.4	5.0
164	10.0	8.2	12.2

