

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030263.D
 Acq On : 02 Jun 2021 17:26
 Operator : CG/JU
 Sample : PB136743BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK743

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030263.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	37	40	47	rVB	87928	111157	1.74%	0.159%
2	3.734	106	110	137	rBV	867248	1491501	23.32%	2.128%
3	4.063	163	166	172	rVB	15352	23706	0.37%	0.034%
4	5.069	333	337	341	rVB6	4062	6885	0.11%	0.010%
5	7.016	660	668	680	rBV	1249062	1940106	30.33%	2.768%
6	7.192	691	698	714	rBV	958708	1569441	24.54%	2.239%
7	7.392	724	732	741	rBV	1230322	1951596	30.51%	2.784%
8	7.857	804	811	821	rBV	992326	1618142	25.30%	2.309%
9	8.551	922	929	939	rBV	1499868	2355180	36.82%	3.360%
10	9.016	999	1008	1020	rBV	1129866	1875315	29.32%	2.676%
11	9.733	1123	1130	1140	rBV	835718	1333081	20.84%	1.902%
12	10.269	1213	1221	1234	rBV	1398746	2364884	36.97%	3.374%
13	10.651	1278	1286	1296	rVB	1461564	2430521	38.00%	3.468%
14	10.780	1300	1308	1320	rBV	1422006	2462398	38.50%	3.513%
15	12.233	1548	1555	1562	rBV3	25394	45439	0.71%	0.065%
16	12.445	1588	1591	1597	rBV6	3988	6776	0.11%	0.010%
17	13.457	1758	1763	1768	rVB5	4949	7517	0.12%	0.011%
18	13.892	1829	1837	1848	rBV	2583471	3633800	56.81%	5.184%
19	14.174	1876	1885	1896	rBV	3023193	4426204	69.20%	6.315%
20	14.480	1930	1937	1946	rBV	2232297	3361801	52.56%	4.796%
21	14.662	1961	1968	1985	rBV	1153272	1667936	26.08%	2.380%
22	15.468	2098	2105	2113	rBV	3828554	5573416	87.14%	7.952%
23	15.580	2118	2124	2135	rBV	1016730	1364328	21.33%	1.946%
24	15.709	2140	2146	2152	rVB	43934	65969	1.03%	0.094%
25	16.251	2234	2238	2242	rVB4	13306	17510	0.27%	0.025%
26	17.004	2362	2366	2373	rBV	9955	15651	0.24%	0.022%
27	17.215	2395	2402	2411	rBV	2749956	3834125	59.94%	5.470%
28	17.315	2412	2419	2435	rVV	4233127	5818767	90.97%	8.302%
29	17.592	2460	2466	2470	rBV7	3986	7288	0.11%	0.010%
30	18.103	2549	2553	2560	rBV6	13874	21994	0.34%	0.031%
31	19.233	2740	2745	2749	rBV	45259	65136	1.02%	0.093%
32	19.380	2766	2770	2775	rBV6	15045	21921	0.34%	0.031%
33	19.486	2784	2788	2794	rBV2	34407	50051	0.78%	0.071%
34	19.597	2801	2807	2817	rBV	4895275	6396207	100.00%	9.125%
35	21.374	3104	3109	3115	rBV	2811154	3547422	55.46%	5.061%
36	23.515	3467	3473	3486	rVB2	2756789	5320258	83.18%	7.590%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030263.D
Acq On : 02 Jun 2021 17:26
Operator : CG/JU
Sample : PB136743BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK743

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Title : SVOA CALIBRATION

37	23.662	3492	3498	3510	rVB2	1774036	3288386	51.41%	4.692%
----	--------	------	------	------	------	---------	---------	--------	--------


Sum of corrected areas: 70091815

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030263.D
Acq On : 02 Jun 2021 17:26
Operator : CG/JU
Sample : PB136743BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK743

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

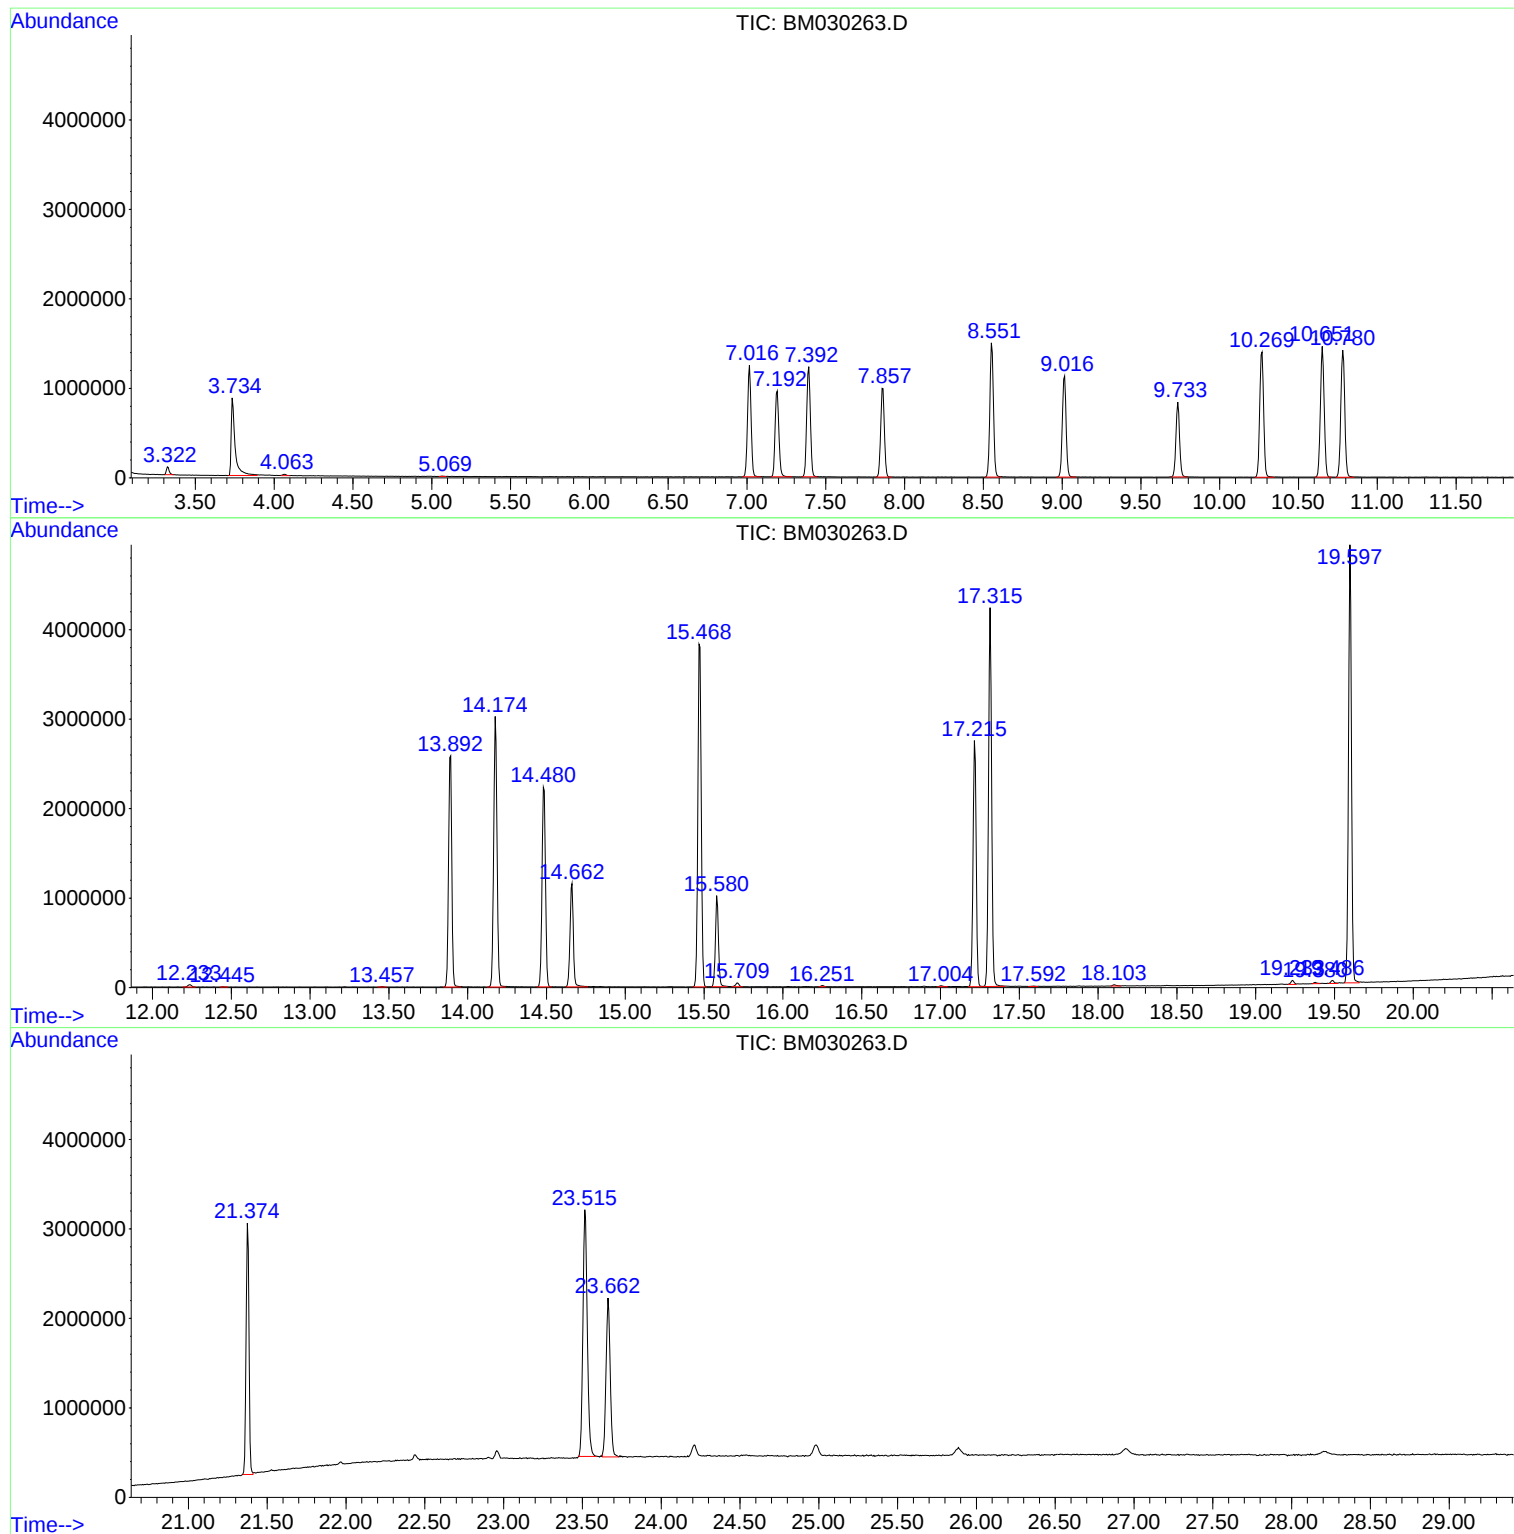

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030263.D
Acq On : 02 Jun 2021 17:26
Operator : CG/JU
Sample : PB136743BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK743

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030263.D
Acq On : 02 Jun 2021 17:26
Operator : CG/JU
Sample : PB136743BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK743

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------