

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030267.D
 Acq On : 02 Jun 2021 19:53
 Operator : CG/JU
 Sample : M2568-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GM9

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030267.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	31	36	47	rBV2	350133	558892	11.89%	1.195%
2	3.757	110	114	132	rBV	66722	182160	3.88%	0.389%
3	3.969	146	150	156	rVB	31928	47872	1.02%	0.102%
4	4.063	163	166	176	rVB	17004	28729	0.61%	0.061%
5	4.157	179	182	188	rVB6	12125	18834	0.40%	0.040%
6	4.593	253	256	261	rVB6	4907	7590	0.16%	0.016%
7	4.981	319	322	325	rVB3	5253	6332	0.13%	0.014%
8	6.251	534	538	541	rBV4	8495	12151	0.26%	0.026%
9	7.016	661	668	678	rVB2	136613	274642	5.84%	0.587%
10	7.187	690	697	708	rBV	681364	1118793	23.81%	2.392%
11	7.393	724	732	741	rBV	607718	977079	20.79%	2.089%
12	7.863	804	812	819	rBV	742621	1218243	25.92%	2.604%
13	8.098	844	852	857	rBV10	5591	11967	0.25%	0.026%
14	8.551	922	929	941	rVB	425718	660126	14.05%	1.411%
15	9.010	999	1007	1018	rBV	772821	1311346	27.90%	2.803%
16	9.439	1075	1080	1087	rBV	23759	39581	0.84%	0.085%
17	9.734	1122	1130	1144	rVB	519658	856652	18.23%	1.831%
18	10.263	1213	1220	1233	rBV	844728	1407872	29.96%	3.010%
19	10.581	1269	1274	1278	rBV	11016	18058	0.38%	0.039%
20	10.651	1278	1286	1294	rVB	1036123	1747803	37.19%	3.736%
21	10.781	1300	1308	1318	rBV	842092	1435274	30.54%	3.068%
22	11.928	1497	1503	1509	rBV2	22482	34697	0.74%	0.074%
23	12.233	1550	1555	1562	rVB2	19213	30727	0.65%	0.066%
24	12.657	1624	1627	1633	rVB6	4770	7722	0.16%	0.017%
25	13.104	1698	1703	1706	rVB6	3387	5453	0.12%	0.012%
26	13.451	1755	1762	1765	rBV6	3807	6361	0.14%	0.014%
27	13.886	1830	1836	1841	rVV	1725440	2419274	51.48%	5.172%
28	13.933	1841	1844	1850	rVB	166654	228250	4.86%	0.488%
29	14.174	1878	1885	1899	rBV	2077562	2936948	62.49%	6.278%
30	14.380	1915	1920	1925	rBV8	4166	7086	0.15%	0.015%
31	14.480	1930	1937	1947	rVV	1537409	2292139	48.77%	4.900%
32	14.657	1961	1967	1975	rBV	86003	130079	2.77%	0.278%
33	15.227	2056	2064	2067	rBV7	3193	5503	0.12%	0.012%
34	15.292	2069	2075	2077	rVV4	5768	9636	0.21%	0.021%
35	15.333	2079	2082	2087	rVB5	3960	4983	0.11%	0.011%
36	15.468	2098	2105	2113	rBV	2682900	3865441	82.25%	8.263%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030267.D
 Acq On : 02 Jun 2021 19:53
 Operator : CG/JU
 Sample : M2568-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GM9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

37	15.580	2118	2124	2136	rVV	613146	859090	18.28%	1.837%
38	15.710	2140	2146	2155	rVB2	31415	49267	1.05%	0.105%
39	16.257	2234	2239	2243	rVV4	9218	13237	0.28%	0.028%
40	16.898	2344	2348	2352	rBV7	3962	6664	0.14%	0.014%
41	17.004	2363	2366	2372	rVB3	6832	8710	0.19%	0.019%
42	17.215	2396	2402	2409	rBV	1828925	2496264	53.12%	5.336%
43	17.315	2412	2419	2431	rVV	2974206	4190390	89.16%	8.958%
44	17.398	2431	2433	2438	rVB6	7353	10386	0.22%	0.022%
45	18.098	2547	2552	2562	rBV	113166	171198	3.64%	0.366%
46	18.180	2564	2566	2570	rVB5	5381	4986	0.11%	0.011%
47	18.768	2663	2666	2670	rBV6	5221	9010	0.19%	0.019%
48	19.233	2741	2745	2749	rBV2	32464	55223	1.18%	0.118%
49	19.374	2765	2769	2775	rBV3	30485	45731	0.97%	0.098%
50	19.486	2785	2788	2793	rVB2	23557	27552	0.59%	0.059%
51	19.598	2801	2807	2818	rBV	3585149	4699660	100.00%	10.047%
52	21.080	3055	3059	3068	rBV2	252913	397217	8.45%	0.849%
53	21.374	3104	3109	3115	rBV	2069367	2535893	53.96%	5.421%
54	23.515	3466	3473	3485	rBV	2396771	4687551	99.74%	10.021%
55	23.662	3491	3498	3508	rVB2	1319662	2585850	55.02%	5.528%


Sum of corrected areas: 46778174

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030267.D
Acq On : 02 Jun 2021 19:53
Operator : CG/JU
Sample : M2568-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GM9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

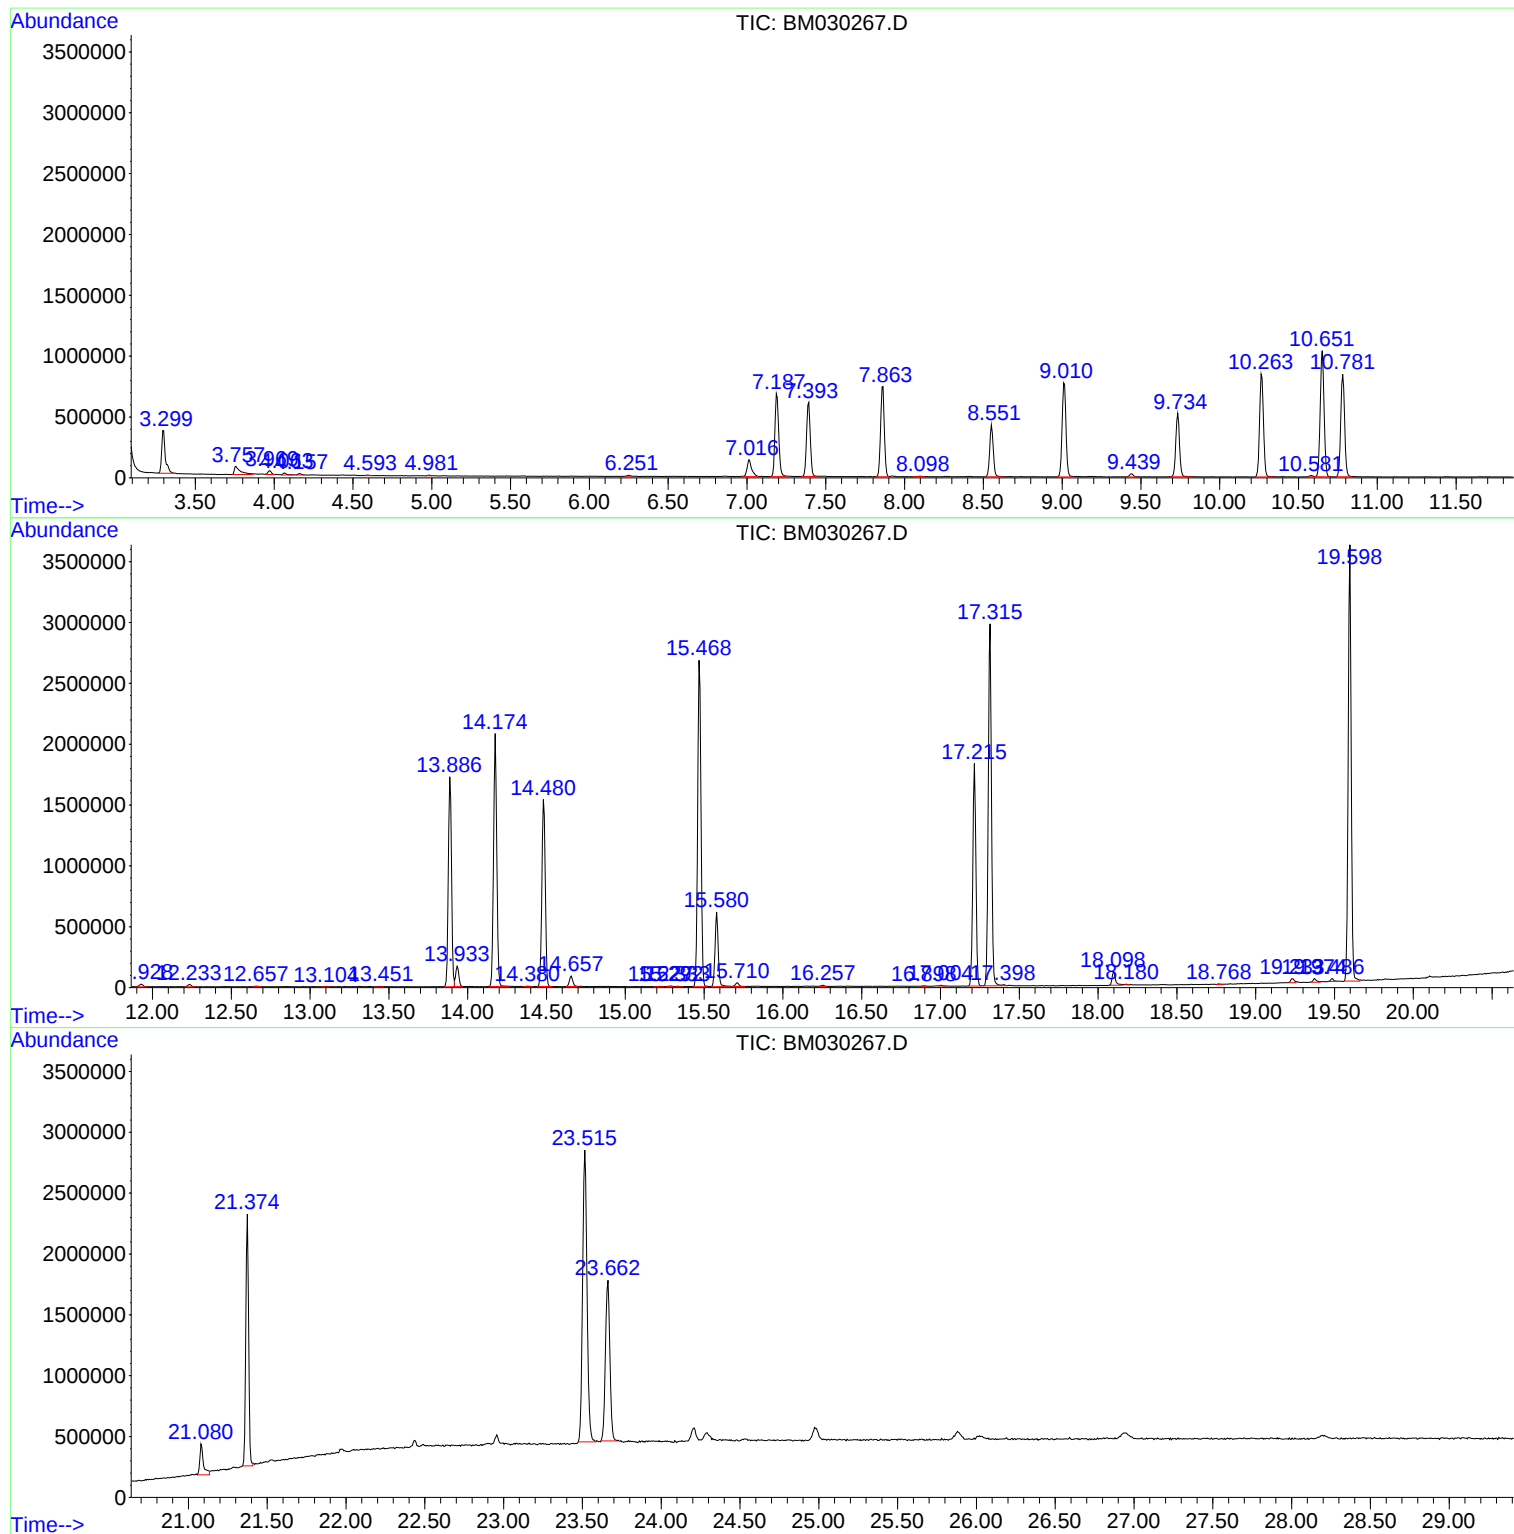

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030267.D
Acq On : 02 Jun 2021 19:53
Operator : CG/JU
Sample : M2568-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GM9










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trichloroacetic acid, hexad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.080	3.13 ng/ul	397217	Chrysene-d12	21.374

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
2			Behenic alcohol	326	C22H46O	000661-19-8	94
3			n-Nonadecanol-1	284	C19H40O	001454-84-8	93
4			1-Docosene	308	C22H44	001599-67-3	93
5			1-Heneicosyl formate	340	C22H44O2	077899-03-7	91

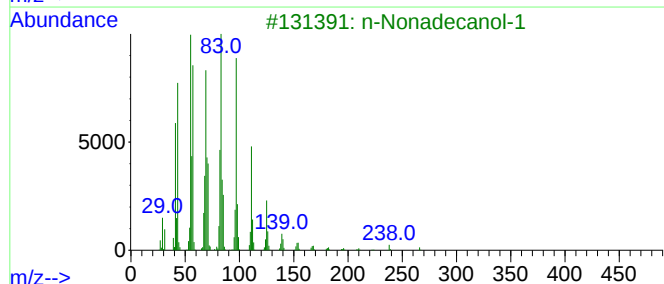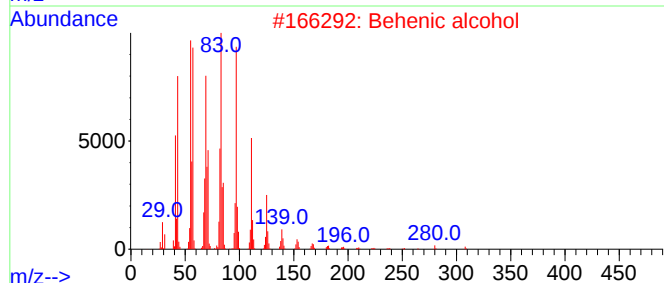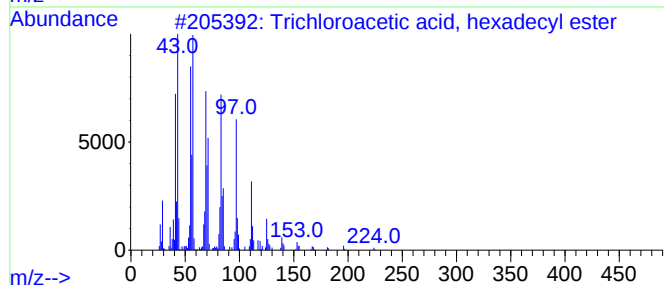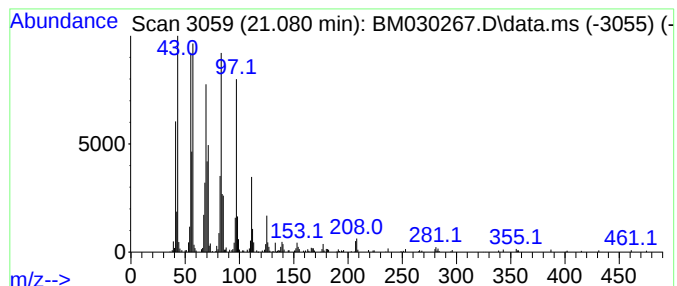

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030267.D
Acq On : 02 Jun 2021 19:53
Operator : CG/JU
Sample : M2568-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GM9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trichloroacetic...	21.080	3.1	ng/ul	397217	5	21.374	2535890	20.0