

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030269.D
 Acq On : 02 Jun 2021 21:06
 Operator : CG/JU
 Sample : M2568-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GN2

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030269.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	30	35	52	rVB2	701892	1065712	17.72%	1.816%
2	3.752	109	113	128	rBV	92626	218598	3.64%	0.372%
3	3.969	146	150	156	rVB	36702	56693	0.94%	0.097%
4	4.063	163	166	173	rVB2	16051	23262	0.39%	0.040%
5	4.163	179	183	189	rVB5	15535	23766	0.40%	0.040%
6	4.593	251	256	267	rVB	183464	273779	4.55%	0.466%
7	4.975	318	321	325	rBV2	6145	9732	0.16%	0.017%
8	6.252	534	538	544	rVB3	11188	16471	0.27%	0.028%
9	7.016	661	668	678	rBV2	146490	314689	5.23%	0.536%
10	7.187	690	697	710	rBV	865406	1406884	23.40%	2.397%
11	7.387	724	731	740	rBV	706441	1137793	18.92%	1.938%
12	7.857	804	811	818	rBV	855738	1336833	22.23%	2.277%
13	7.922	820	822	826	rVB3	7114	9339	0.16%	0.016%
14	8.098	848	852	858	rBV6	5332	10094	0.17%	0.017%
15	8.551	922	929	941	rBV	492938	775531	12.90%	1.321%
16	9.010	999	1007	1016	rBV	1023755	1676567	27.88%	2.856%
17	9.181	1031	1036	1037	rBV5	4473	6364	0.11%	0.011%
18	9.440	1076	1080	1084	rVB5	6960	10295	0.17%	0.018%
19	9.734	1122	1130	1139	rBV	658014	1086197	18.06%	1.850%
20	10.263	1213	1220	1229	rBV	1079606	1765367	29.36%	3.007%
21	10.651	1277	1286	1294	rBV	1193910	2006128	33.36%	3.418%
22	10.781	1300	1308	1318	rBV	1090108	1849643	30.76%	3.151%
23	11.310	1392	1398	1402	rVB7	3968	6567	0.11%	0.011%
24	11.422	1413	1417	1425	rVB6	4294	8874	0.15%	0.015%
25	11.928	1497	1503	1510	rBV5	5293	12240	0.20%	0.021%
26	12.233	1550	1555	1563	rVB	26350	41746	0.69%	0.071%
27	13.098	1695	1702	1707	rBV10	4288	9250	0.15%	0.016%
28	13.316	1733	1739	1743	rBV6	4308	8019	0.13%	0.014%
29	13.380	1746	1750	1755	rVV5	5565	8780	0.15%	0.015%
30	13.451	1756	1762	1769	rVB6	5590	11284	0.19%	0.019%
31	13.886	1829	1836	1841	rBV	2373803	3301267	54.90%	5.624%
32	13.933	1841	1844	1854	rVB	360714	477250	7.94%	0.813%
33	14.175	1874	1885	1899	rBV	2768452	4004426	66.59%	6.822%
34	14.380	1914	1920	1925	rVB7	5088	8781	0.15%	0.015%
35	14.480	1930	1937	1946	rBV	1841151	2706383	45.01%	4.611%
36	14.657	1960	1967	1978	rBV	103254	160117	2.66%	0.273%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030269.D
 Acq On : 02 Jun 2021 21:06
 Operator : CG/JU
 Sample : M2568-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GN2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

37	14.886	2001	2006	2012	rVB8	3875	7034	0.12%	0.012%
38	15.280	2068	2073	2079	rBV4	6125	13297	0.22%	0.023%
39	15.469	2098	2105	2113	rBV	3680357	5206669	86.59%	8.870%
40	15.580	2117	2124	2140	rBV	876175	1165153	19.38%	1.985%
41	15.710	2140	2146	2151	rVB	40249	59191	0.98%	0.101%
42	16.139	2214	2219	2225	rBV9	4282	8768	0.15%	0.015%
43	16.251	2234	2238	2245	rVB3	12832	19411	0.32%	0.033%
44	16.904	2344	2349	2352	rBV6	4363	6915	0.11%	0.012%
45	17.004	2363	2366	2372	rVB2	8112	11502	0.19%	0.020%
46	17.216	2395	2402	2409	rBV	2103117	2901400	48.25%	4.943%
47	17.316	2412	2419	2429	rVV	3895641	5519882	91.80%	9.404%
48	17.398	2429	2433	2437	rVB6	7198	14080	0.23%	0.024%
49	18.098	2547	2552	2562	rBV	188034	286590	4.77%	0.488%
50	19.233	2741	2745	2749	rBV	46530	59270	0.99%	0.101%
51	19.315	2756	2759	2762	rVB3	10615	12574	0.21%	0.021%
52	19.374	2765	2769	2776	rBV3	60210	88503	1.47%	0.151%
53	19.486	2784	2788	2792	rBV	34029	42623	0.71%	0.073%
54	19.598	2801	2807	2820	rBV	4546046	6013252	100.00%	10.244%
55	21.080	3055	3059	3070	rBV2	261417	403122	6.70%	0.687%
56	21.374	3104	3109	3116	rBV	2294074	2745575	45.66%	4.677%
57	23.515	3466	3473	3486	rVB2	2985356	5539133	92.12%	9.436%
58	23.662	3491	3498	3506	rVB2	1383689	2731158	45.42%	4.653%




Sum of corrected areas: 58699823

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030269.D
Acq On : 02 Jun 2021 21:06
Operator : CG/JU
Sample : M2568-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GN2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

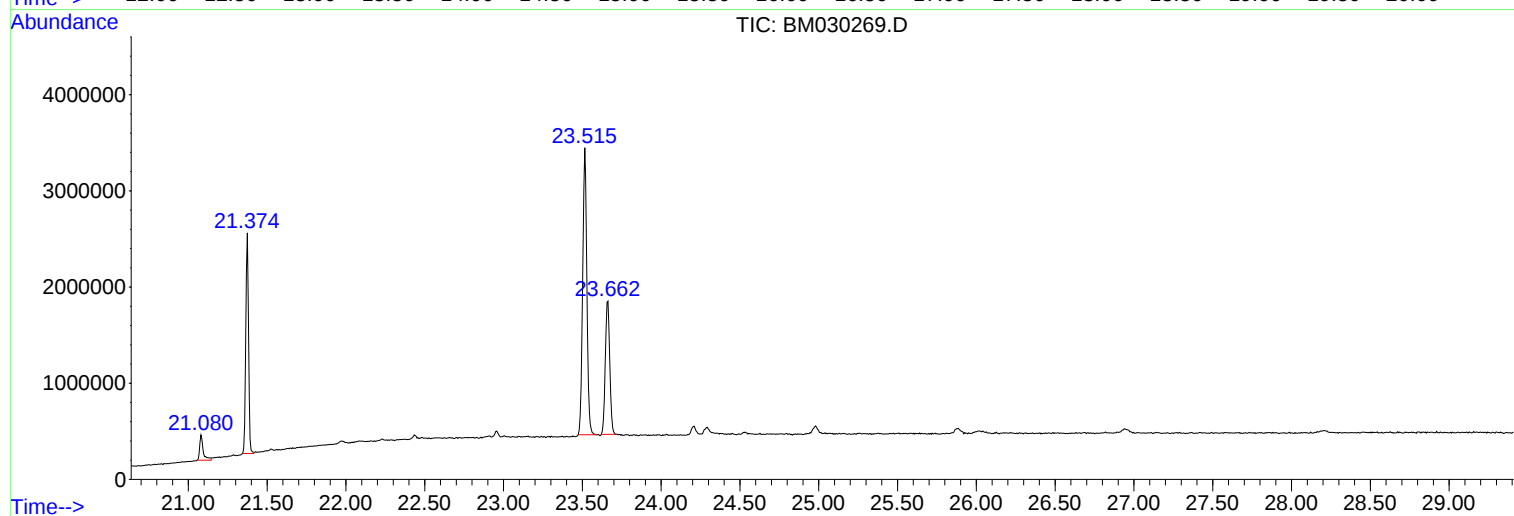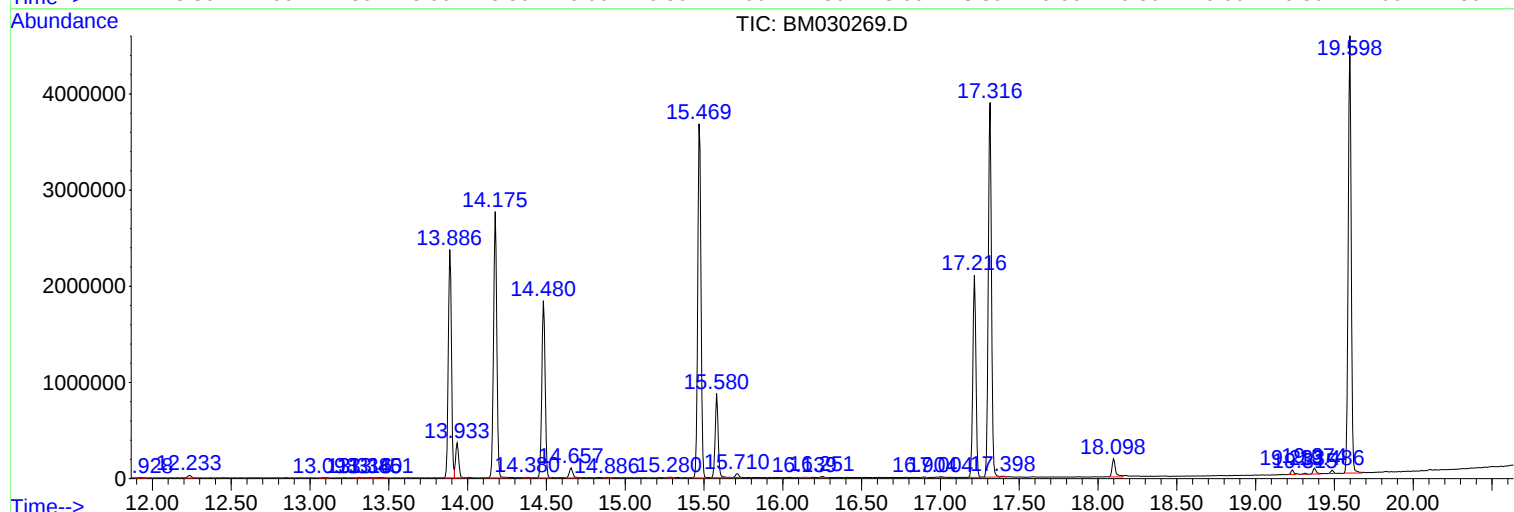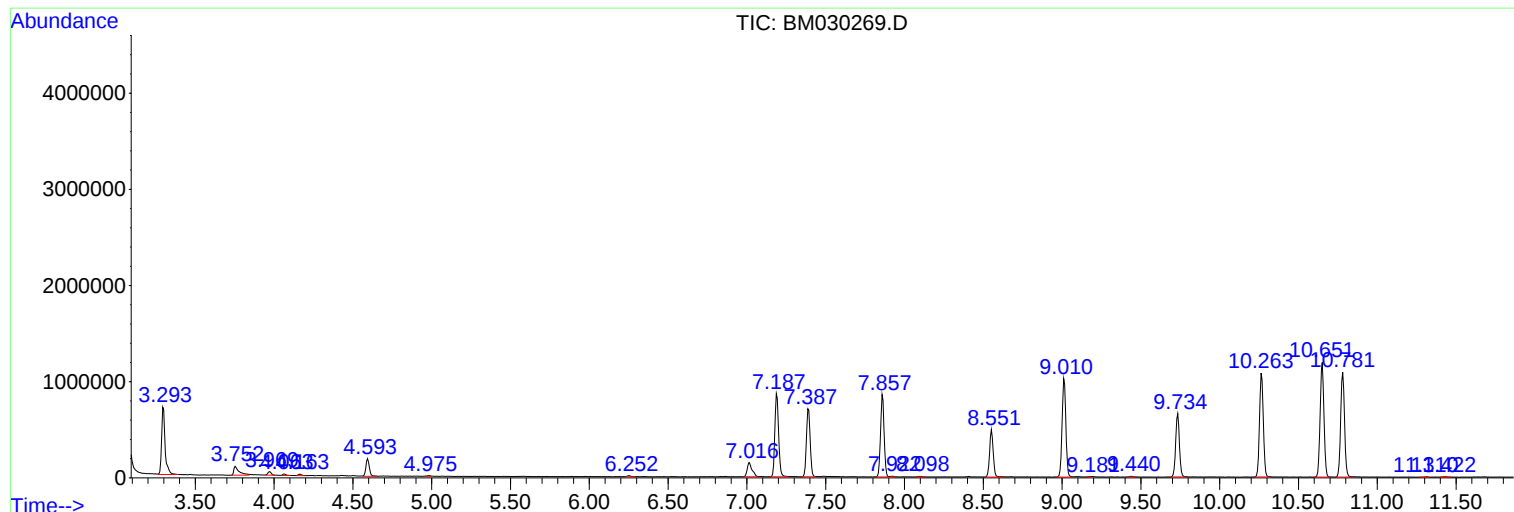

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030269.D
Acq On : 02 Jun 2021 21:06
Operator : CG/JU
Sample : M2568-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GN2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Trichloroacetic acid, penta... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.080	2.94 ng/ul	403122	Chrysene-d12	21.374

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	94
2			Cyclotetracosane	336	C24H48	000297-03-0	93
3			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	91
4			3-Eicosene, (E)-	280	C20H40	074685-33-9	91
5			1-Nonadecene	266	C19H38	018435-45-5	91

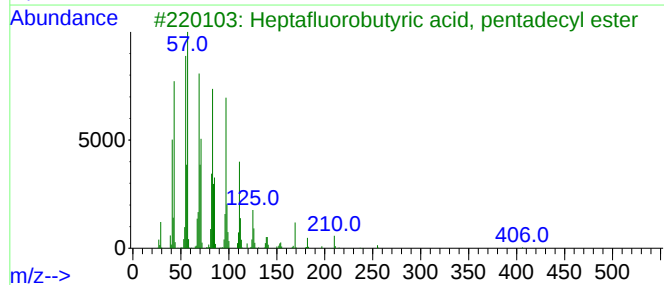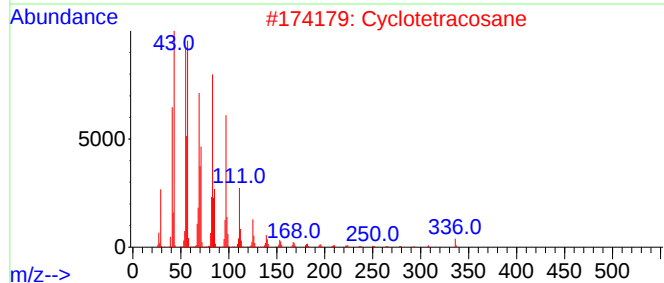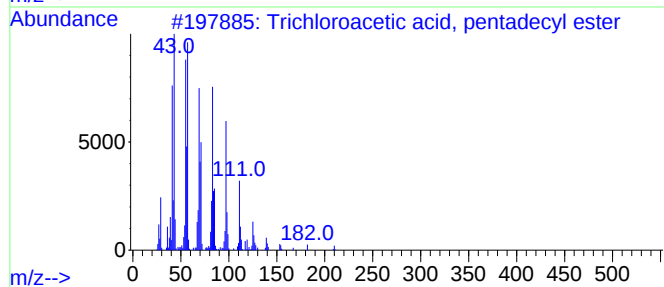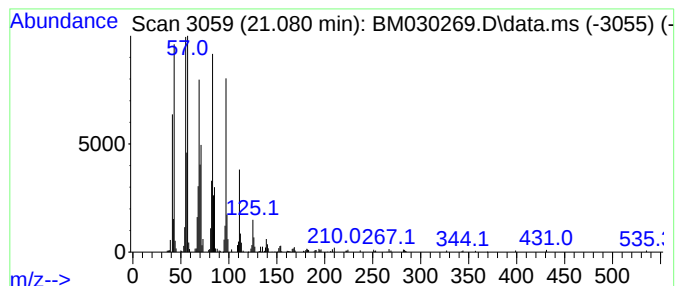

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030269.D
Acq On : 02 Jun 2021 21:06
Operator : CG/JU
Sample : M2568-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GN2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trichloroacetic...	21.080	2.9	ng/ul	403122	5	21.374	2745580	20.0