

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
 Data File : BM030273.D
 Acq On : 02 Jun 2021 23:31
 Operator : CG/JU
 Sample : PB136642BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK642

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030273.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	9	13	15	rBV2	29428	33027	0.97%	0.188%
2	3.187	15	17	19	rVV2	13056	12364	0.36%	0.071%
3	3.211	19	21	24	rVV	19598	21396	0.63%	0.122%
4	3.252	24	28	33	rVB	1960642	2018553	59.31%	11.517%
5	3.593	82	86	91	rVB	46609	61980	1.82%	0.354%
6	4.063	161	166	171	rVB	20817	26822	0.79%	0.153%
7	4.999	320	325	328	rBV6	3722	5501	0.16%	0.031%
8	7.857	803	811	821	rBV	1087606	1731002	50.86%	9.876%
9	10.645	1277	1285	1295	rBV	1322692	2268617	66.66%	12.944%
10	14.480	1928	1937	1945	rBV	2020130	2892286	84.99%	16.502%
11	16.692	2310	2313	2318	rBV6	1540	3462	0.10%	0.020%
12	17.004	2361	2366	2371	rBV	7845	11917	0.35%	0.068%
13	17.216	2395	2402	2412	rBV	2498351	3403182	100.00%	19.417%
14	17.316	2414	2419	2422	rVV3	6258	8924	0.26%	0.051%
15	18.104	2549	2553	2561	rBV3	3827	9065	0.27%	0.052%
16	18.557	2628	2630	2635	rBV5	2520	3860	0.11%	0.022%
17	21.374	3104	3109	3117	rBV	2180923	2687821	78.98%	15.335%
18	23.656	3491	3497	3510	rVB2	1179120	2327276	68.39%	13.278%


Sum of corrected areas: 17527055

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030273.D
Acq On : 02 Jun 2021 23:31
Operator : CG/JU
Sample : PB136642BL
Misc : GCMS CONFIRMATION
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK642

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

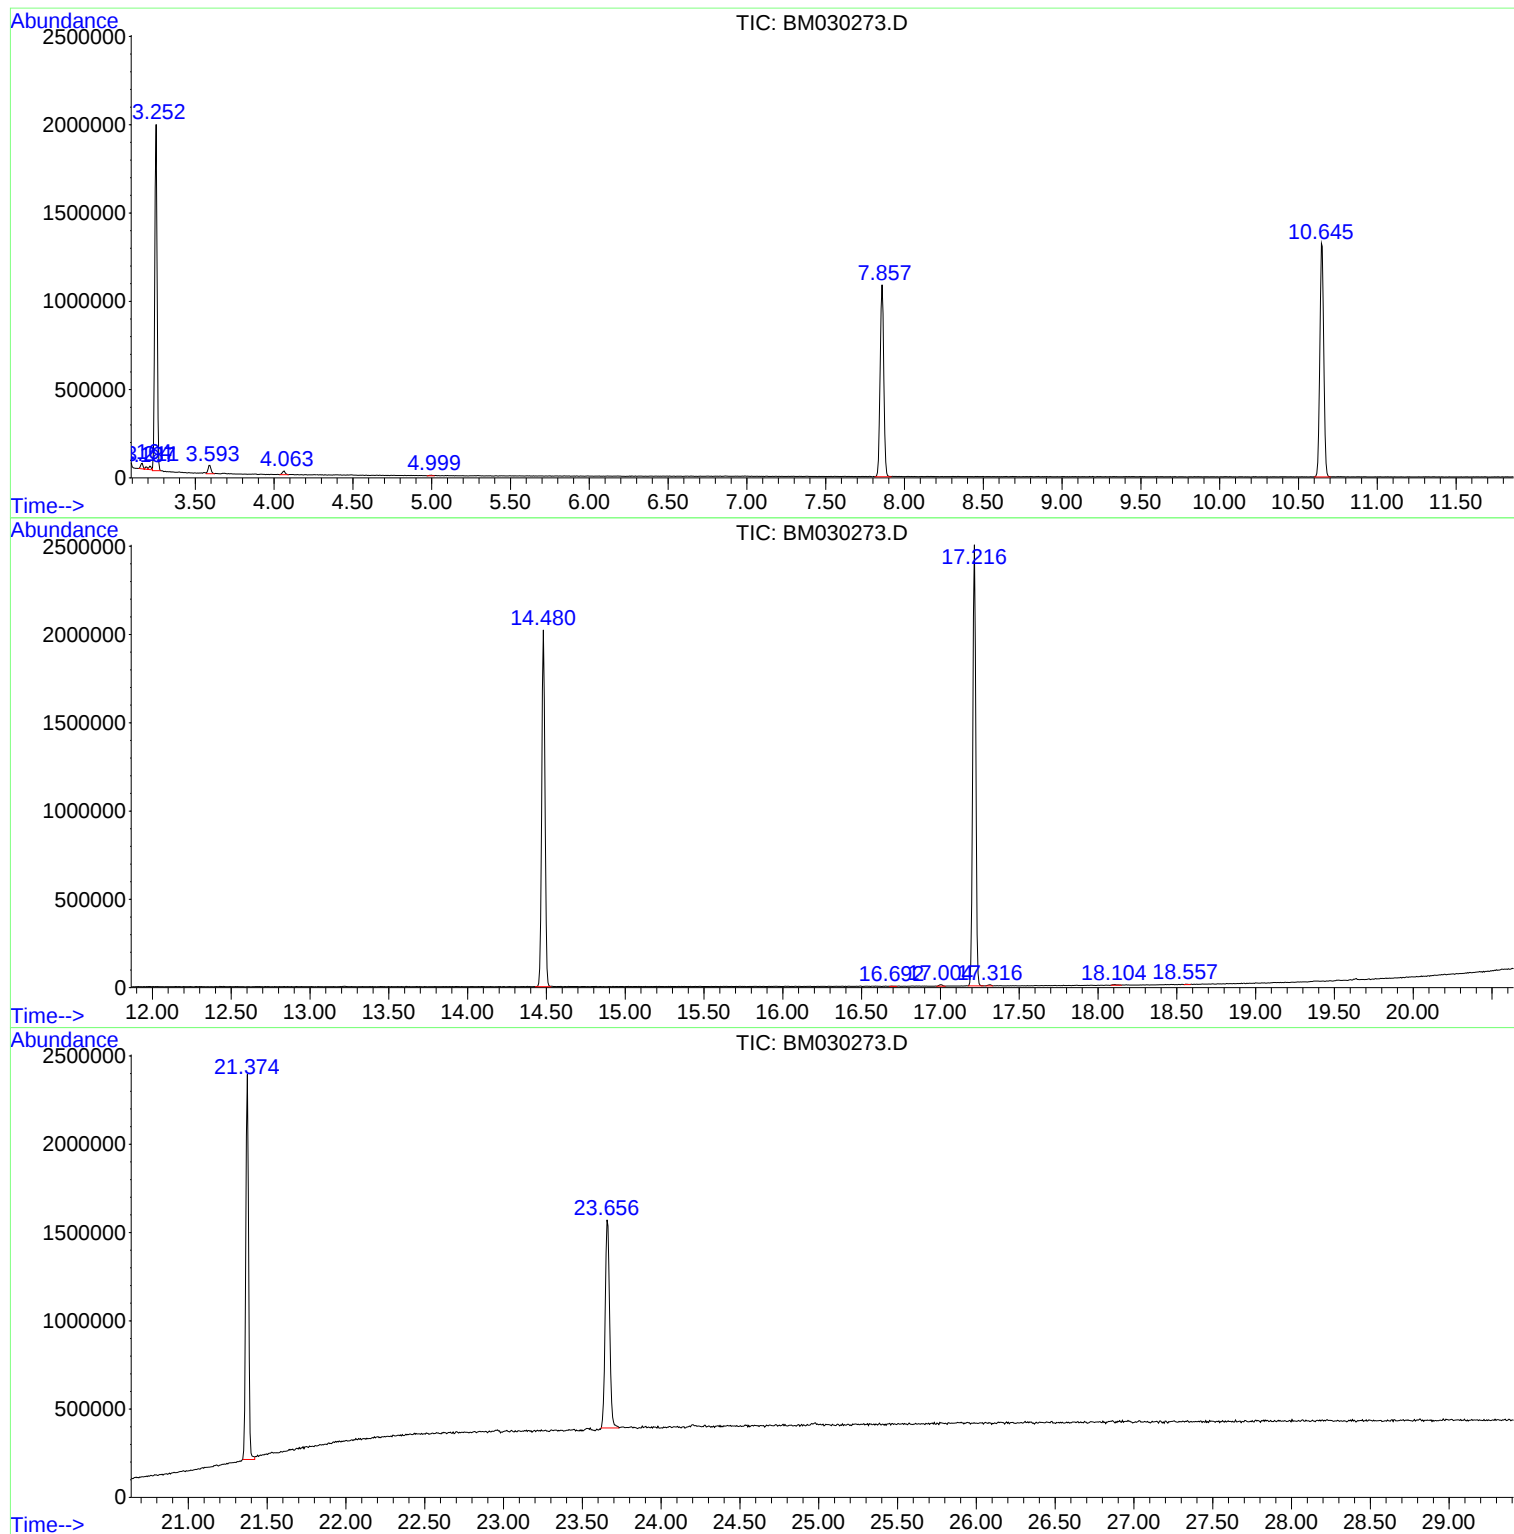

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030273.D
Acq On : 02 Jun 2021 23:31
Operator : CG/JU
Sample : PB136642BL
Misc : GCMS CONFIRMATION
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK642










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.250	23.32 ng/ul	2018550	1,4-Dichlorobenzene-d4	7.857

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	95
2			Heptane	100	C7H16	000142-82-5	94
3			Heptane	100	C7H16	000142-82-5	91
4			Heptane	100	C7H16	000142-82-5	90
5			Oxalic acid, isobutyl pentyl ester	216	C11H20O4	1000309-37-0	59

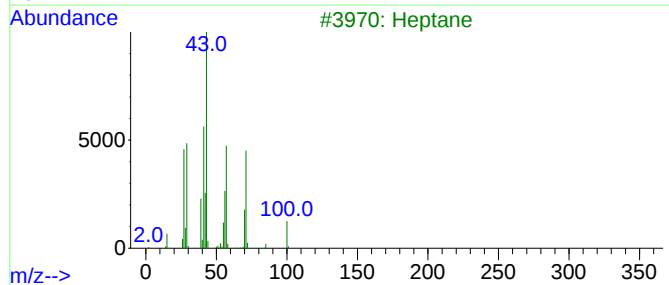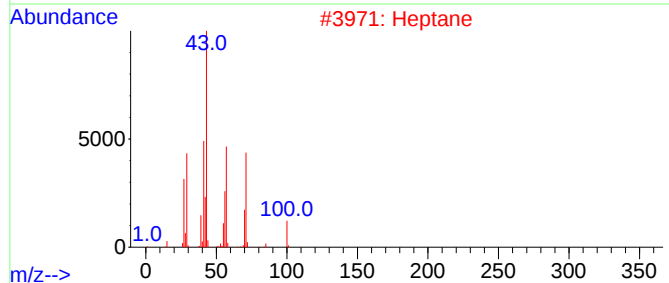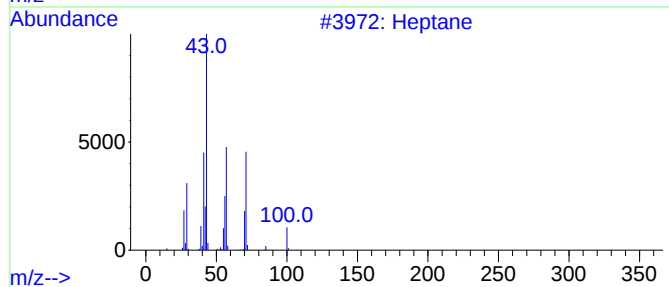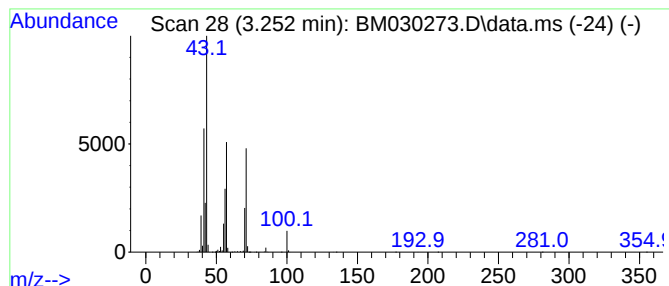

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060221\
Data File : BM030273.D
Acq On : 02 Jun 2021 23:31
Operator : CG/JU
Sample : PB136642BL
Misc : GCMS CONFIRMATION
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK642

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.250	23.3	ng/u1	2018550	1	7.857	1731000	20.0