

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
 Data File : BM035365.D
 Acq On : 02 Jun 2022 16:38
 Operator : CG/JU
 Sample : PB145220BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145220BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.440	393	400	415	rBV	2282770	3361854	21.44%	6.181%
2	7.040	662	672	688	rBV	2182304	3574308	22.79%	6.572%
3	7.851	803	810	824	rBV	460777	731071	4.66%	1.344%
4	9.016	999	1008	1021	rBV	1392477	2352971	15.00%	4.326%
5	10.651	1279	1286	1301	rBV	635484	1123988	7.17%	2.067%
6	13.122	1698	1706	1722	rBV	5576236	8214216	52.38%	15.103%
7	14.492	1932	1939	1952	rBV	1376125	2070927	13.20%	3.808%
8	15.986	2186	2193	2214	rBV	5099745	7596066	48.43%	13.967%
9	17.239	2399	2406	2415	rBV	1880469	2777953	17.71%	5.108%
10	19.868	2847	2853	2858	rBV	12344682	15683283	100.00%	28.837%
11	21.421	3112	3117	3125	rBV	2583245	3390959	21.62%	6.235%
12	23.780	3512	3518	3529	rVB2	1713871	3508880	22.37%	6.452%




Sum of corrected areas: 54386476

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035365.D
Acq On : 02 Jun 2022 16:38
Operator : CG/JU
Sample : PB145220BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

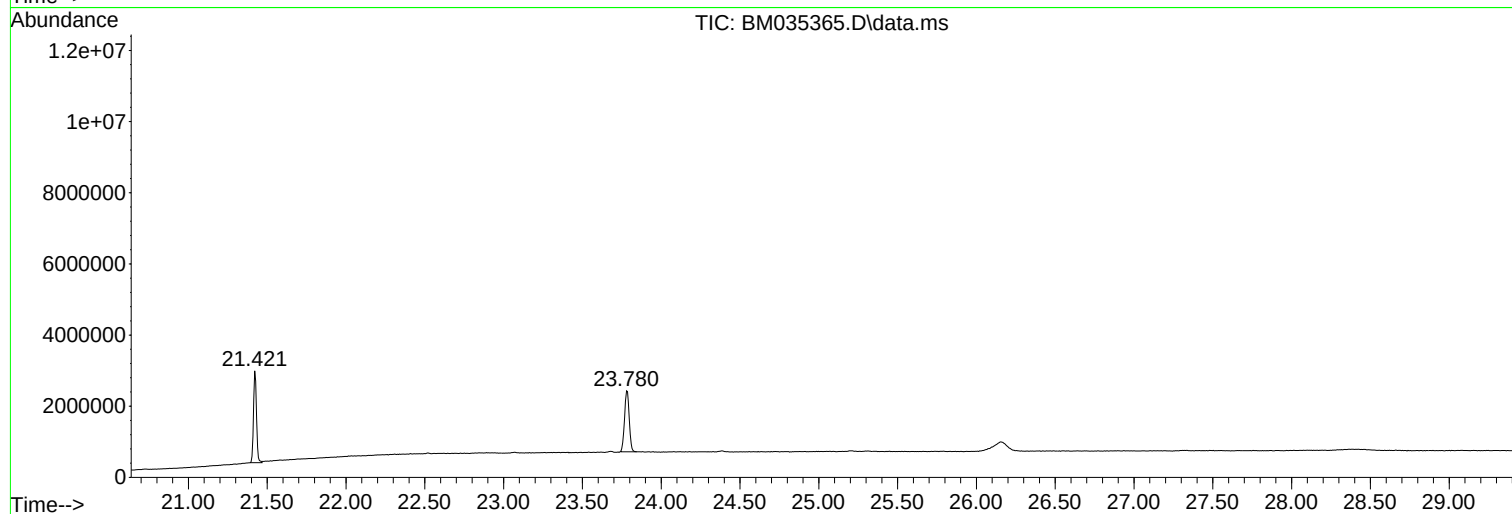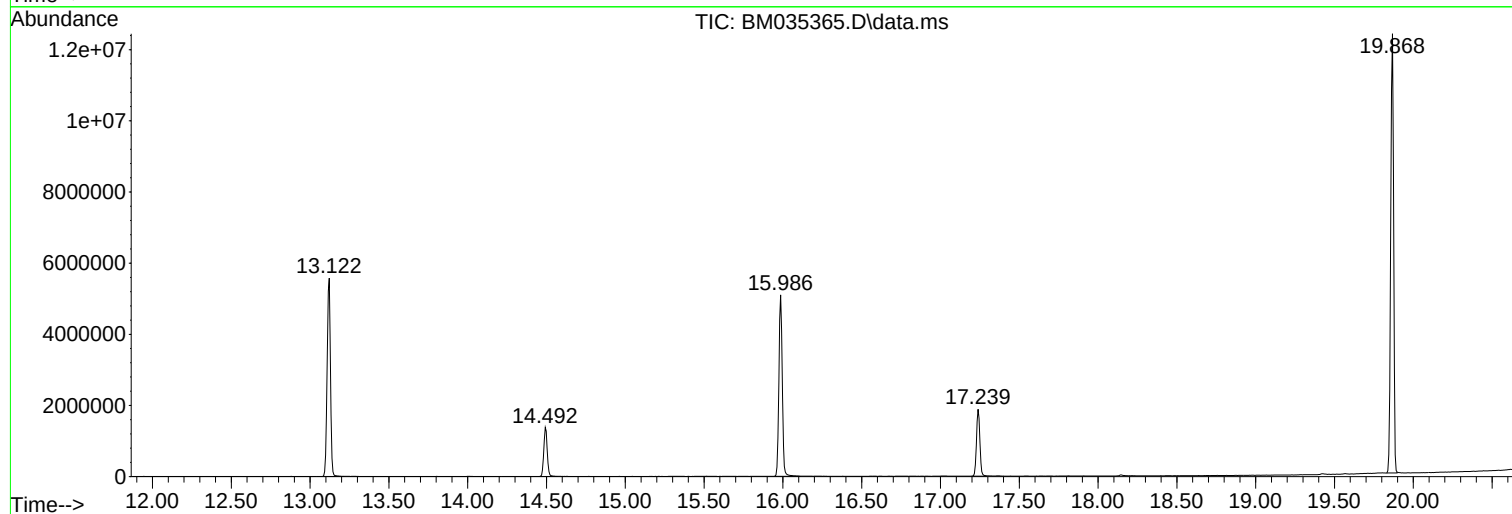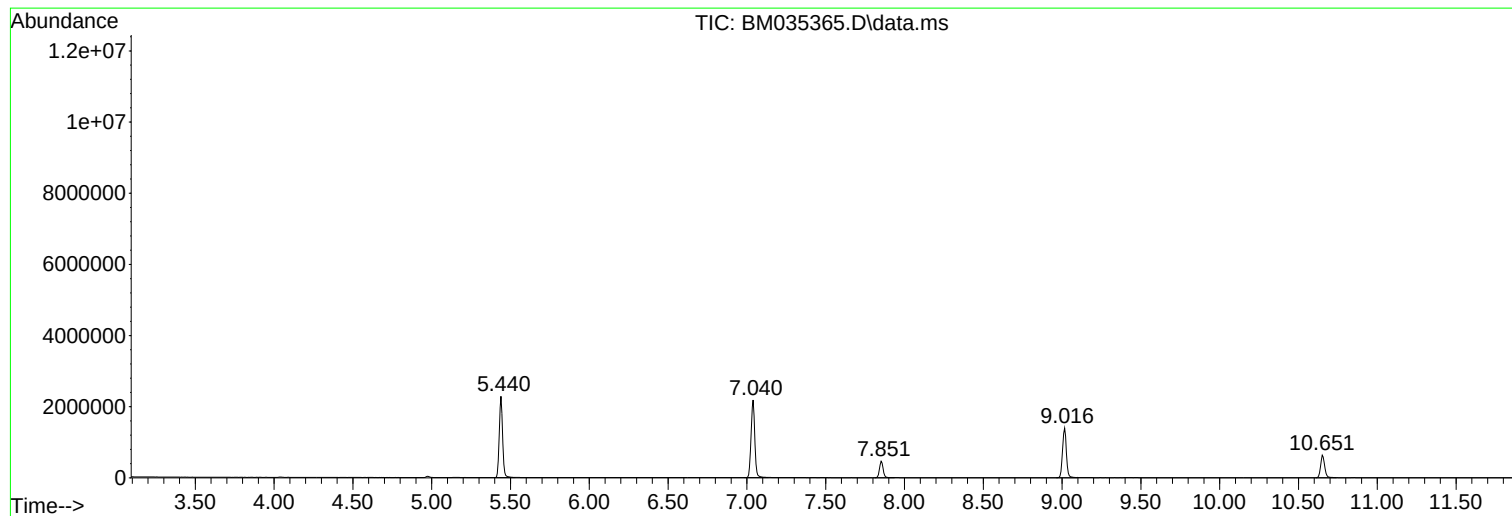

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035365.D
Acq On : 02 Jun 2022 16:38
Operator : CG/JU
Sample : PB145220BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035365.D
Acq On : 02 Jun 2022 16:38
Operator : CG/JU
Sample : PB145220BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc