

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
 Data File : BM035368.D
 Acq On : 02 Jun 2022 18:34
 Operator : CG/JU
 Sample : PB145245BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145245BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.440	393	400	420	rBV	2458567	3647218	24.76%	6.904%
2	7.040	664	672	691	rBV	2341751	3876796	26.32%	7.339%
3	7.851	803	810	827	rVB	495947	791665	5.37%	1.499%
4	9.016	1000	1008	1028	rBV	1490125	2554499	17.34%	4.836%
5	10.651	1279	1286	1305	rBV	664468	1173903	7.97%	2.222%
6	13.116	1697	1705	1721	rBV	5188705	7947288	53.95%	15.044%
7	14.492	1932	1939	1952	rBV	1279454	1952027	13.25%	3.695%
8	15.986	2186	2193	2214	rBV	4845028	7177843	48.73%	13.587%
9	17.239	2399	2406	2417	rBV	1805296	2606468	17.70%	4.934%
10	19.868	2847	2853	2862	rBV	11210441	14729941	100.00%	27.883%
11	21.421	3112	3117	3125	rBV	2602763	3235964	21.97%	6.126%
12	23.780	3512	3518	3530	rVB2	1560227	3133547	21.27%	5.932%




Sum of corrected areas: 52827159

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035368.D
Acq On : 02 Jun 2022 18:34
Operator : CG/JU
Sample : PB145245BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145245BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

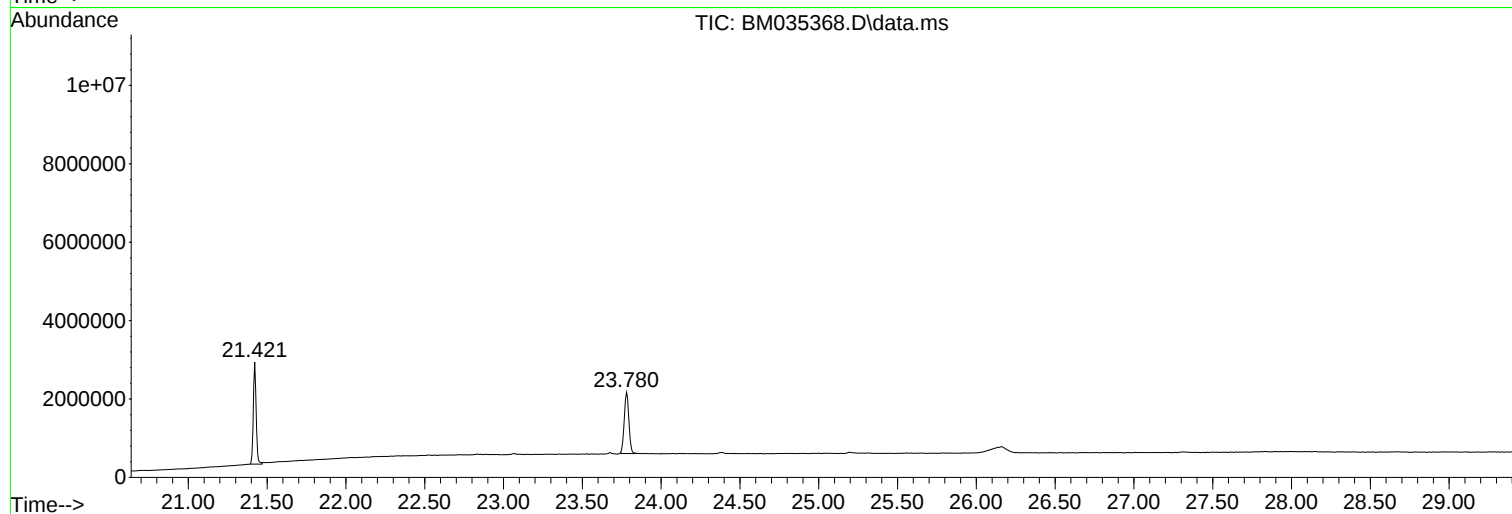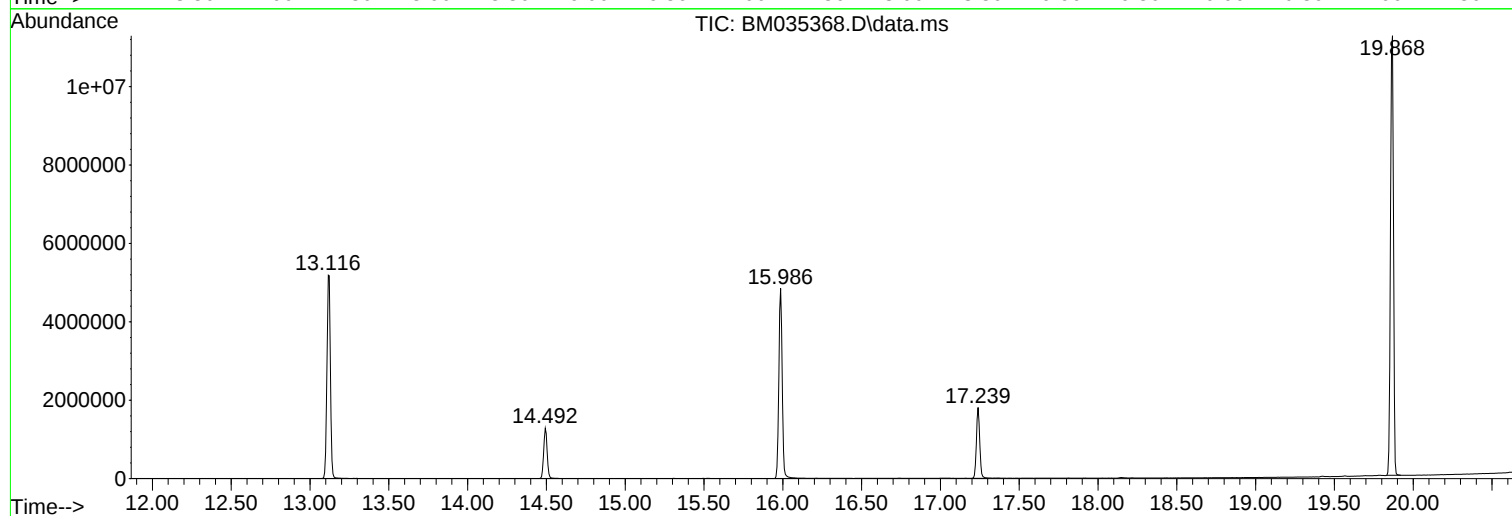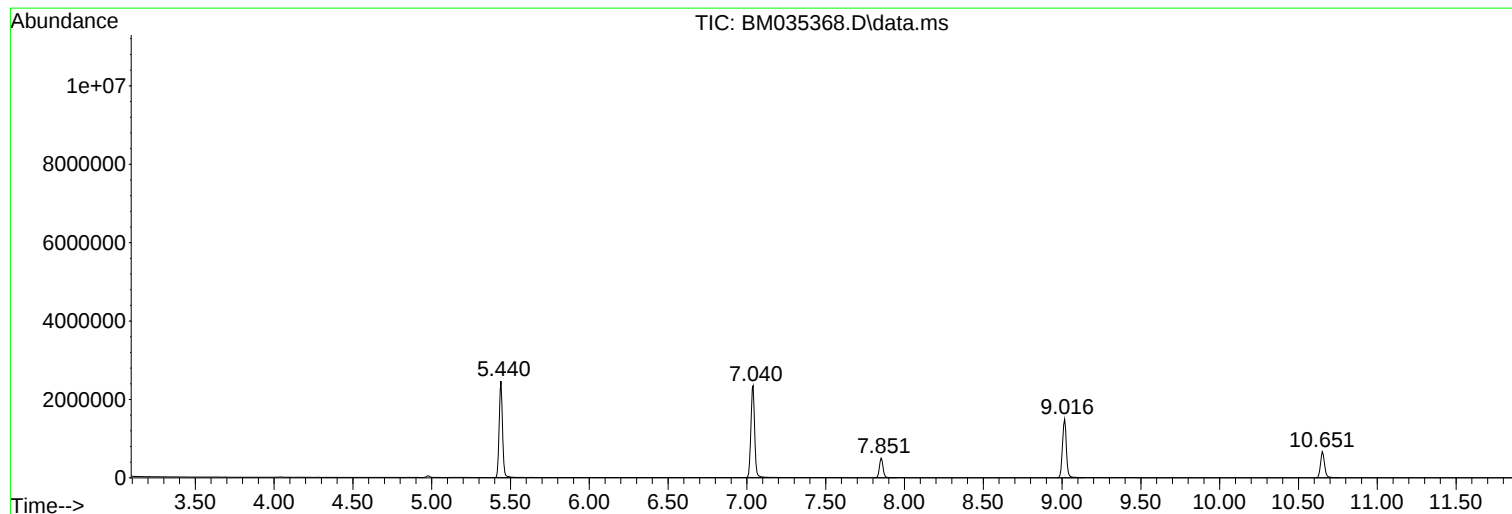

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035368.D
Acq On : 02 Jun 2022 18:34
Operator : CG/JU
Sample : PB145245BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145245BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035368.D
Acq On : 02 Jun 2022 18:34
Operator : CG/JU
Sample : PB145245BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145245BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------