

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
 Data File : BM035369.D
 Acq On : 02 Jun 2022 19:13
 Operator : CG/JU
 Sample : N2986-07
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P027-SS001-1824-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035369.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.440	393	400	413	rBV	1753071	2562193	33.23%	4.938%
2	7.039	664	672	681	rBV	1615240	2576946	33.42%	4.966%
3	7.851	803	810	817	rBV	431023	678134	8.79%	1.307%
4	9.010	1000	1007	1015	rBV	985803	1673436	21.70%	3.225%
5	10.651	1278	1286	1294	rBV	558901	932579	12.09%	1.797%
6	12.686	1606	1632	1639	rBV4	387088	2477288	32.13%	4.774%
7	13.116	1699	1705	1716	rVB	3241367	4589938	59.53%	8.845%
8	14.492	1933	1939	1949	rBV	882688	1262539	16.37%	2.433%
9	14.921	2008	2012	2018	rVB2	123226	173924	2.26%	0.335%
10	15.062	2031	2036	2044	rVB	66082	125681	1.63%	0.242%
11	15.939	2181	2185	2186	rBV	89760	110088	1.43%	0.212%
12	15.986	2186	2193	2196	rBV	2999746	4987132	64.68%	9.611%
13	16.533	2283	2286	2290	rBV	103786	142245	1.84%	0.274%
14	16.633	2299	2303	2322	rVB	501149	1086387	14.09%	2.094%
15	17.239	2400	2406	2411	rBV	1095630	1561128	20.25%	3.008%
16	17.909	2517	2520	2525	rVB2	120311	181811	2.36%	0.350%
17	18.151	2554	2561	2574	rBV	2127006	3254781	42.21%	6.272%
18	18.421	2601	2607	2610	rBV	1031902	1633127	21.18%	3.147%
19	18.462	2610	2614	2630	rVB	1600387	2767747	35.90%	5.334%
20	19.086	2717	2720	2724	rVB3	75305	92658	1.20%	0.179%
21	19.274	2749	2752	2754	rBV2	100632	117693	1.53%	0.227%
22	19.421	2772	2777	2798	rVB	1672189	2488393	32.27%	4.795%
23	19.862	2847	2852	2857	rBV	6210599	7710638	100.00%	14.859%
24	20.156	2898	2902	2910	rVB3	118111	226318	2.94%	0.436%
25	21.133	3064	3068	3076	rBV	598198	734305	9.52%	1.415%
26	21.421	3112	3117	3127	rBV	1764482	2351031	30.49%	4.531%
27	22.521	3301	3304	3309	rVB	279689	347291	4.50%	0.669%
28	23.062	3392	3396	3401	rVB	416093	609137	7.90%	1.174%
29	23.674	3496	3500	3510	rVB	575913	1019677	13.22%	1.965%
30	23.780	3512	3518	3527	rVB	1295413	2543429	32.99%	4.901%
31	24.380	3616	3620	3628	rVB	462080	874344	11.34%	1.685%




Sum of corrected areas: 51892018

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035369.D
Acq On : 02 Jun 2022 19:13
Operator : CG/JU
Sample : N2986-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P027-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

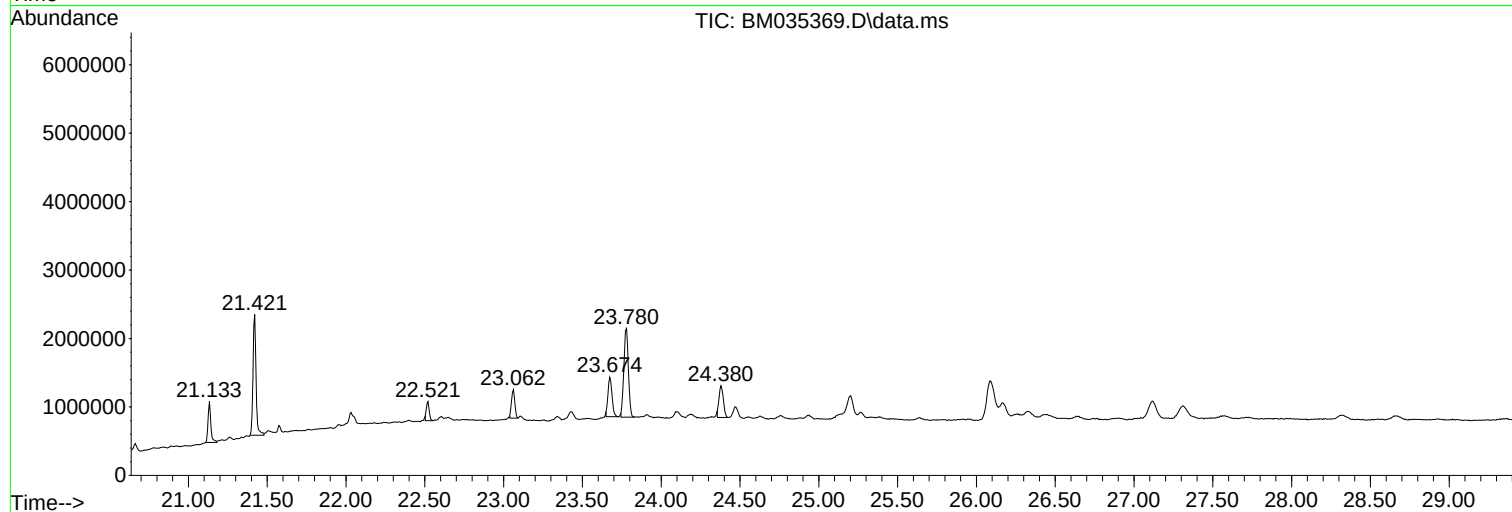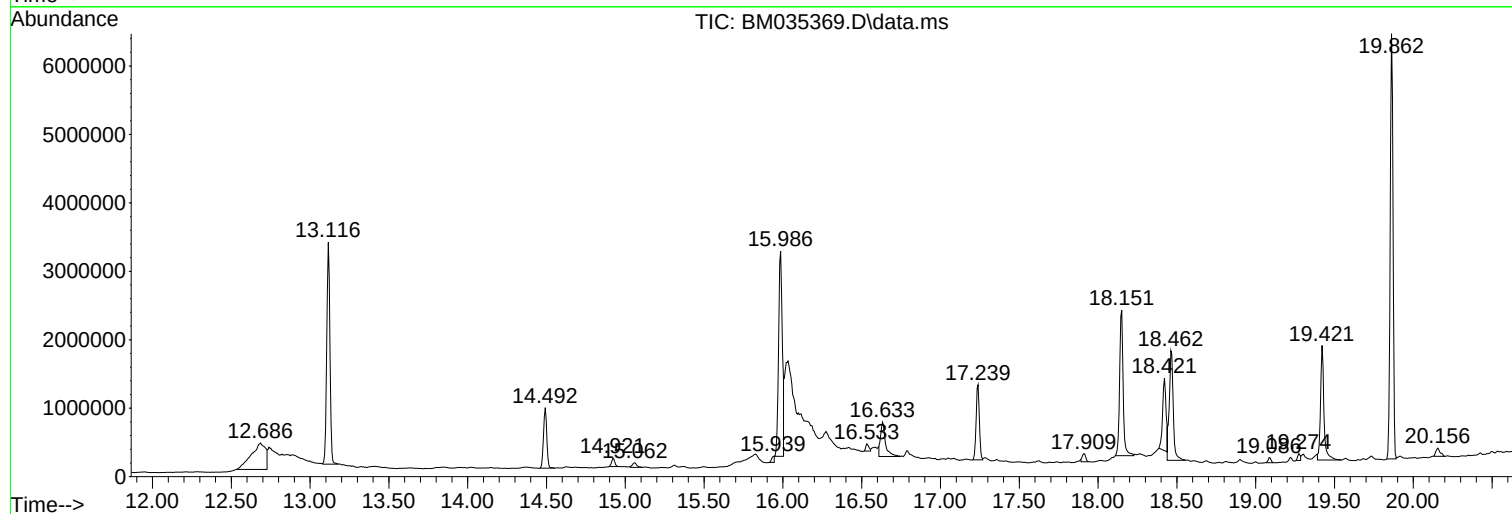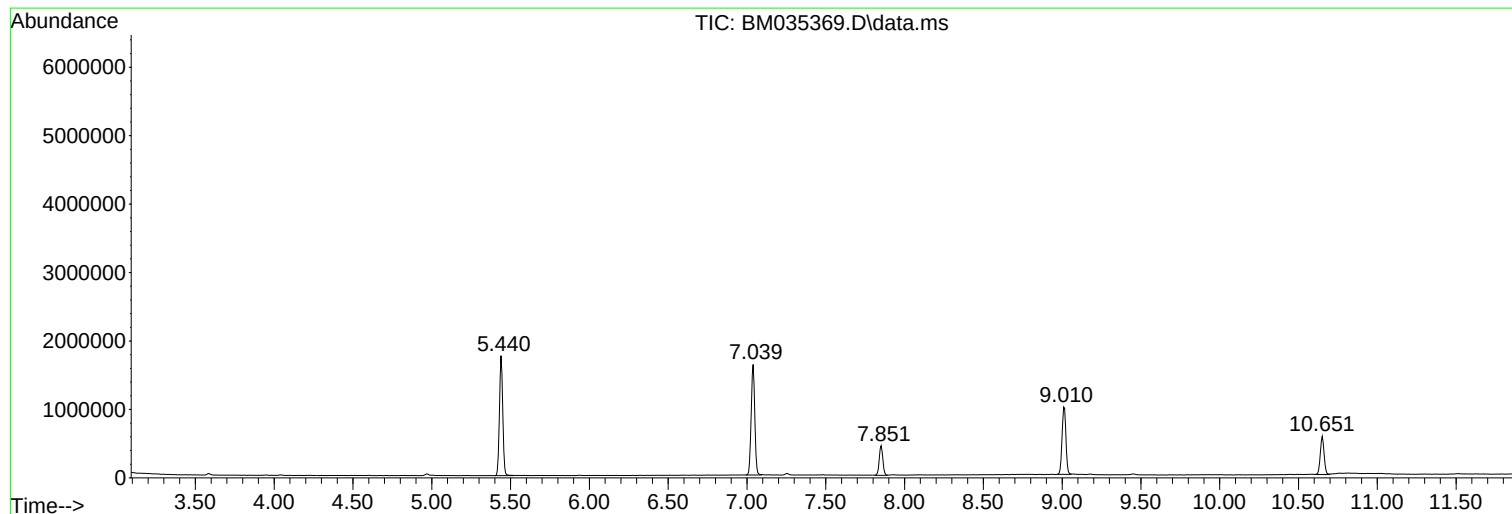

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035369.D
Acq On : 02 Jun 2022 19:13
Operator : CG/JU
Sample : N2986-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P027-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035369.D
Acq On : 02 Jun 2022 19:13
Operator : CG/JU
Sample : N2986-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P027-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------