

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
 Data File : BM035376.D
 Acq On : 02 Jun 2022 23:32
 Operator : CG/JU
 Sample : N2990-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P028-SS001-1218-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.969	315	320	330	rBV	120852	178207	2.31%	0.515%
2	5.434	393	399	411	rBV	1645349	2485376	32.19%	7.184%
3	7.034	661	671	686	rBV	1559991	2620551	33.94%	7.574%
4	7.851	800	810	819	rBV	534986	855361	11.08%	2.472%
5	9.010	999	1007	1026	rBV	1007996	1741424	22.56%	5.033%
6	10.645	1278	1285	1299	rBV	636749	1153180	14.94%	3.333%
7	13.116	1698	1705	1718	rBV	3026482	4563991	59.11%	13.191%
8	14.486	1932	1938	1954	rBV	1024298	1578649	20.45%	4.563%
9	15.980	2185	2192	2215	rBV	2266227	3390566	43.92%	9.800%
10	17.233	2399	2405	2416	rBV	1342472	1946778	25.22%	5.627%
11	18.139	2554	2559	2566	rBV	148097	235075	3.04%	0.679%
12	19.415	2772	2776	2788	rBV2	94789	177235	2.30%	0.512%
13	19.862	2846	2852	2864	rBV	6275335	7720627	100.00%	22.315%
14	21.133	3064	3068	3075	rBV2	301518	408615	5.29%	1.181%
15	21.421	3112	3117	3126	rBV	1905281	2652358	34.35%	7.666%
16	23.774	3511	3517	3531	rVB2	1438513	2890002	37.43%	8.353%




Sum of corrected areas: 34597995

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035376.D
Acq On : 02 Jun 2022 23:32
Operator : CG/JU
Sample : N2990-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P028-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

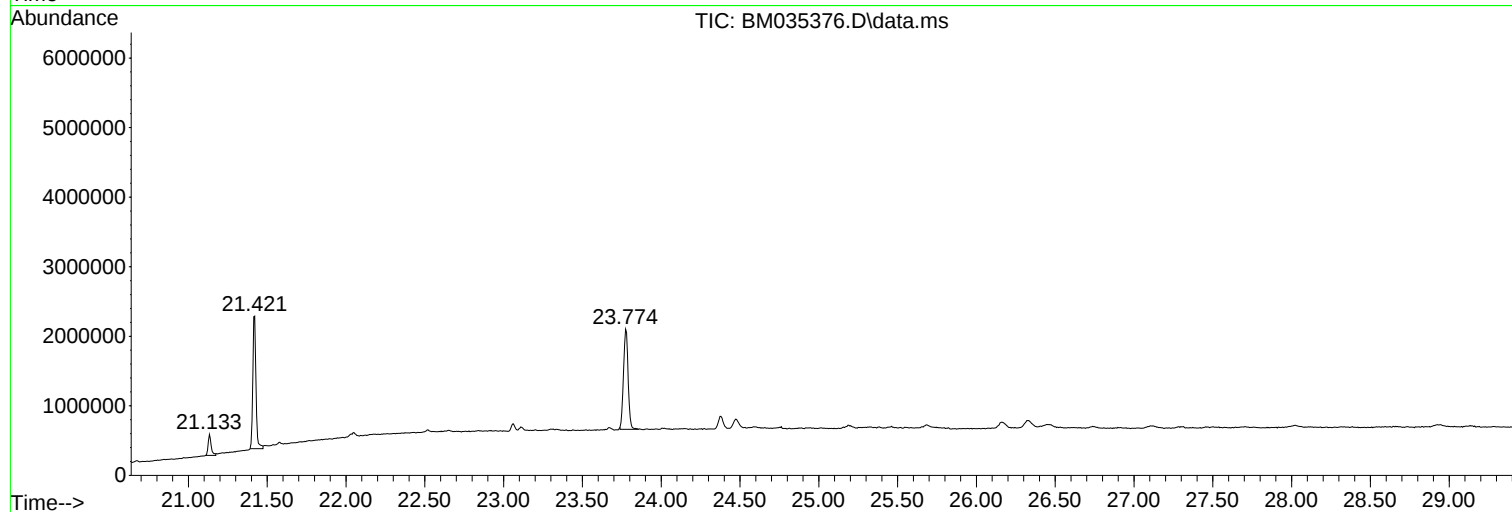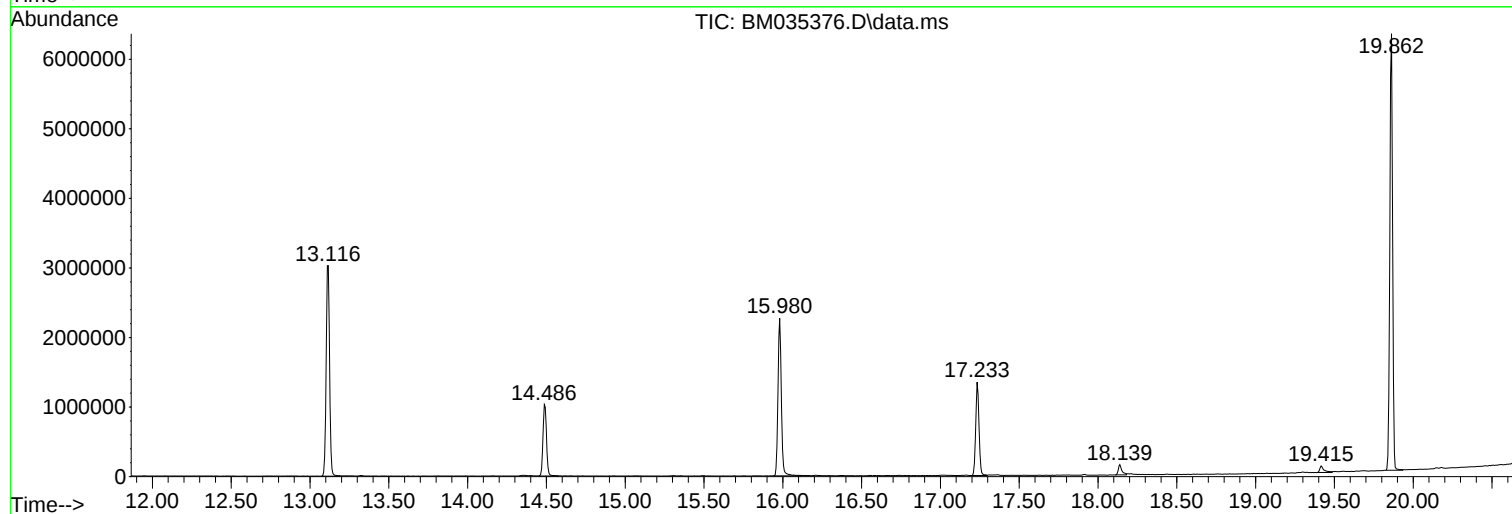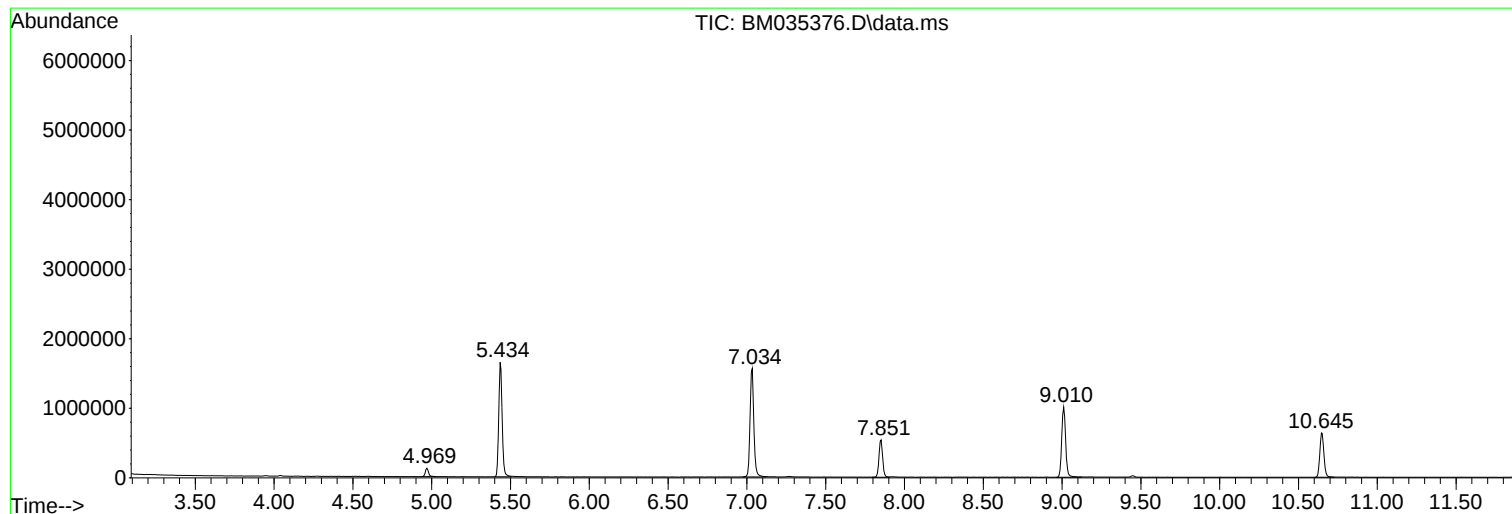

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035376.D
Acq On : 02 Jun 2022 23:32
Operator : CG/JU
Sample : N2990-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P028-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035376.D
Acq On : 02 Jun 2022 23:32
Operator : CG/JU
Sample : N2990-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P028-SS001-1218-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------