

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
 Data File : BM035383.D
 Acq On : 03 Jun 2022 03:50
 Operator : CG/JU
 Sample : N2988-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P015-SS003-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.969	315	320	328	rVB	55191	80141	1.39%	0.226%
2	5.434	393	399	414	rBV	1317405	2019350	35.02%	5.706%
3	7.034	660	671	690	rBV	1186963	2089486	36.23%	5.904%
4	7.845	802	809	818	rBV	558500	897113	15.56%	2.535%
5	9.010	998	1007	1024	rBV	805607	1413426	24.51%	3.994%
6	10.645	1276	1285	1300	rBV	691701	1193141	20.69%	3.372%
7	13.110	1697	1704	1721	rBV	2499721	3725609	64.61%	10.528%
8	14.486	1931	1938	1954	rBV	1086400	1627079	28.22%	4.598%
9	15.980	2185	2192	2213	rBV	1668930	2574928	44.65%	7.276%
10	17.233	2399	2405	2411	rBV	1362739	1919989	33.30%	5.425%
11	18.139	2554	2559	2569	rBV2	266318	420802	7.30%	1.189%
12	19.174	2731	2735	2741	rVB	53120	77728	1.35%	0.220%
13	19.292	2750	2755	2762	rBV	678541	925676	16.05%	2.616%
14	19.415	2772	2776	2785	rVB2	170372	304824	5.29%	0.861%
15	19.627	2809	2812	2813	rBV	92056	104798	1.82%	0.296%
16	19.656	2813	2817	2826	rVB	629111	888507	15.41%	2.511%
17	19.856	2846	2851	2861	rVB	4576197	5766504	100.00%	16.295%
18	20.897	3025	3028	3035	rVB	201068	260804	4.52%	0.737%
19	21.133	3064	3068	3075	rVB3	616828	846365	14.68%	2.392%
20	21.415	3109	3116	3120	rBV2	2198942	3736597	64.80%	10.559%
21	21.450	3120	3122	3134	rVB	632813	852384	14.78%	2.409%
22	23.062	3391	3396	3401	rBV	562116	1208210	20.95%	3.414%
23	23.774	3511	3517	3523	rBV2	1298509	2455092	42.58%	6.938%




Sum of corrected areas: 35388553

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035383.D
Acq On : 03 Jun 2022 03:50
Operator : CG/JU
Sample : N2988-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P015-SS003-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

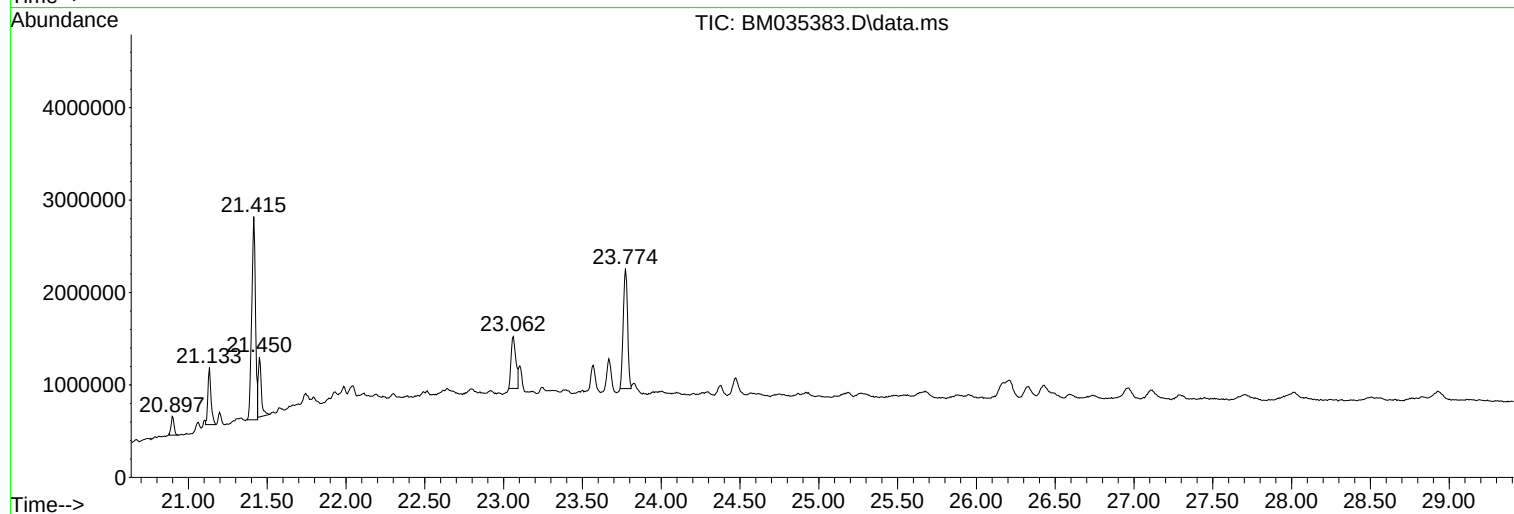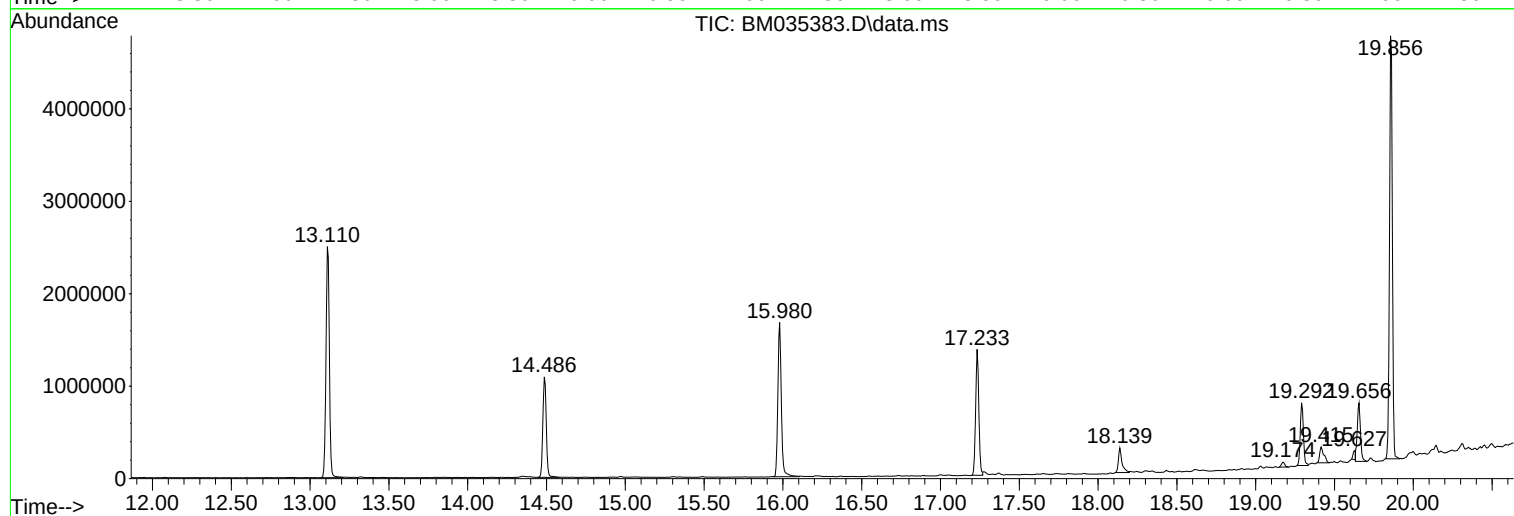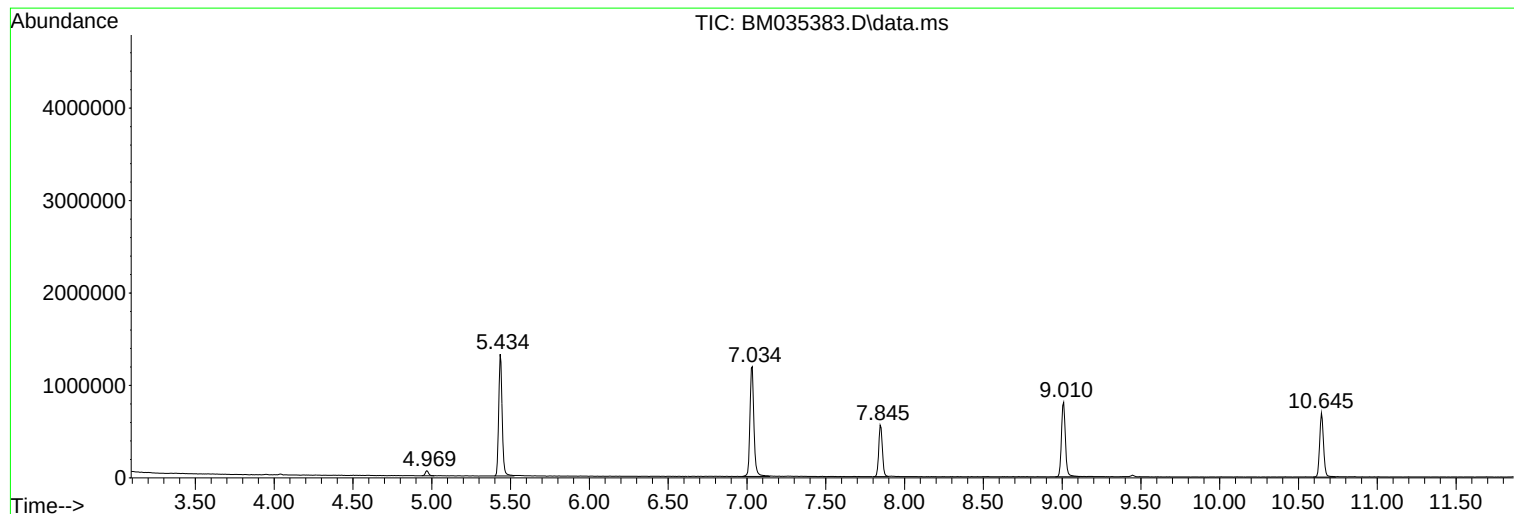

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035383.D
Acq On : 03 Jun 2022 03:50
Operator : CG/JU
Sample : N2988-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P015-SS003-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035383.D
Acq On : 03 Jun 2022 03:50
Operator : CG/JU
Sample : N2988-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P015-SS003-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------