
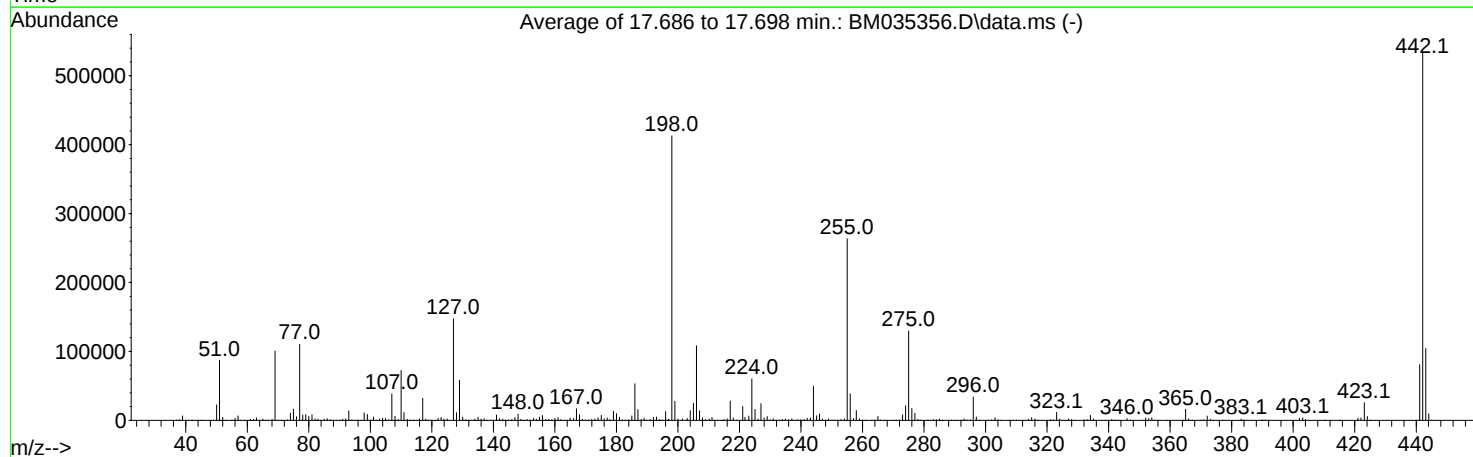


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
 Data File : BM035356.D
 Acq On : 02 Jun 2022 11:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 16:16:23 2022

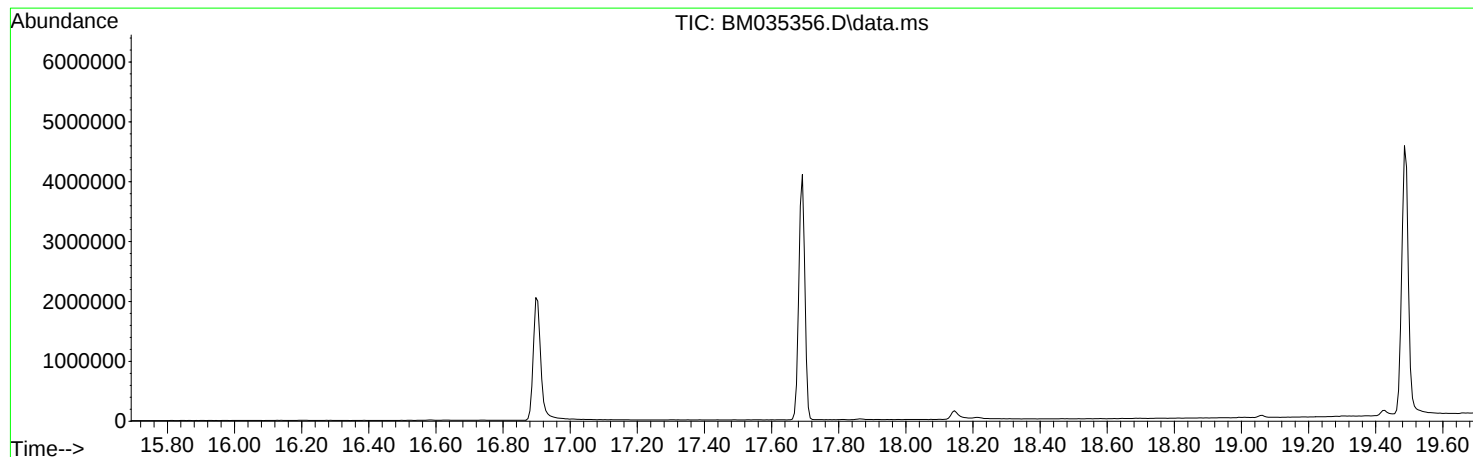




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.1	86986	PASS
68	69	0.00	2	1.6	1578	PASS
69	198	0.00	100	24.3	100515	PASS
70	69	0.00	2	0.6	569	PASS
127	198	10	80	35.7	147477	PASS
197	198	0.00	2	0.4	1650	PASS
198	198	100	100	100.0	412821	PASS
199	198	5	9	6.7	27576	PASS
275	198	10	60	31.4	129592	PASS
365	198	1	100	3.9	15950	PASS
441	198	0.01	100	19.6	80883	PASS
442	442	50	100	100.0	533696	PASS
443	442	15	24	19.5	104328	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035356.D
Acq On : 02 Jun 2022 11:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 02 16:23:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 16:16:23 2022
Response via : Initial Calibration

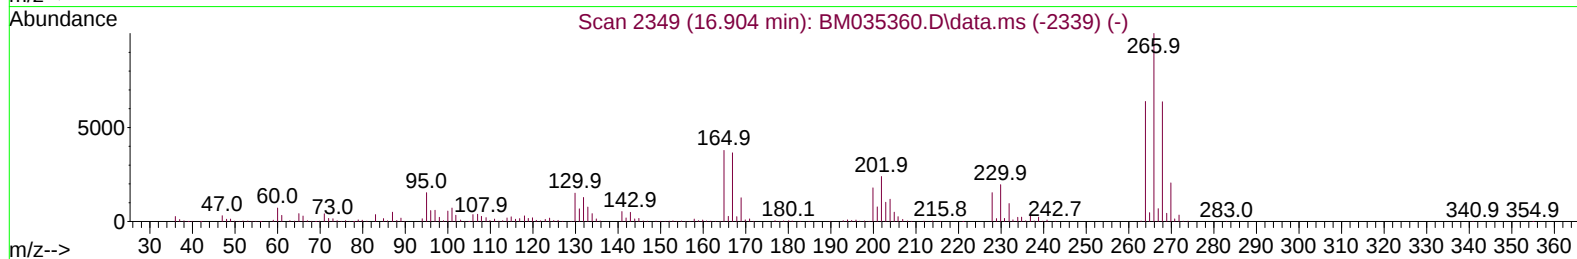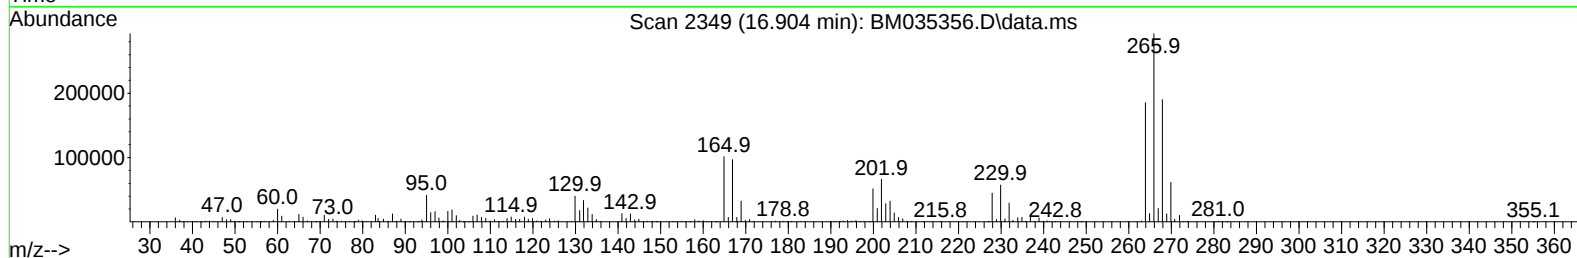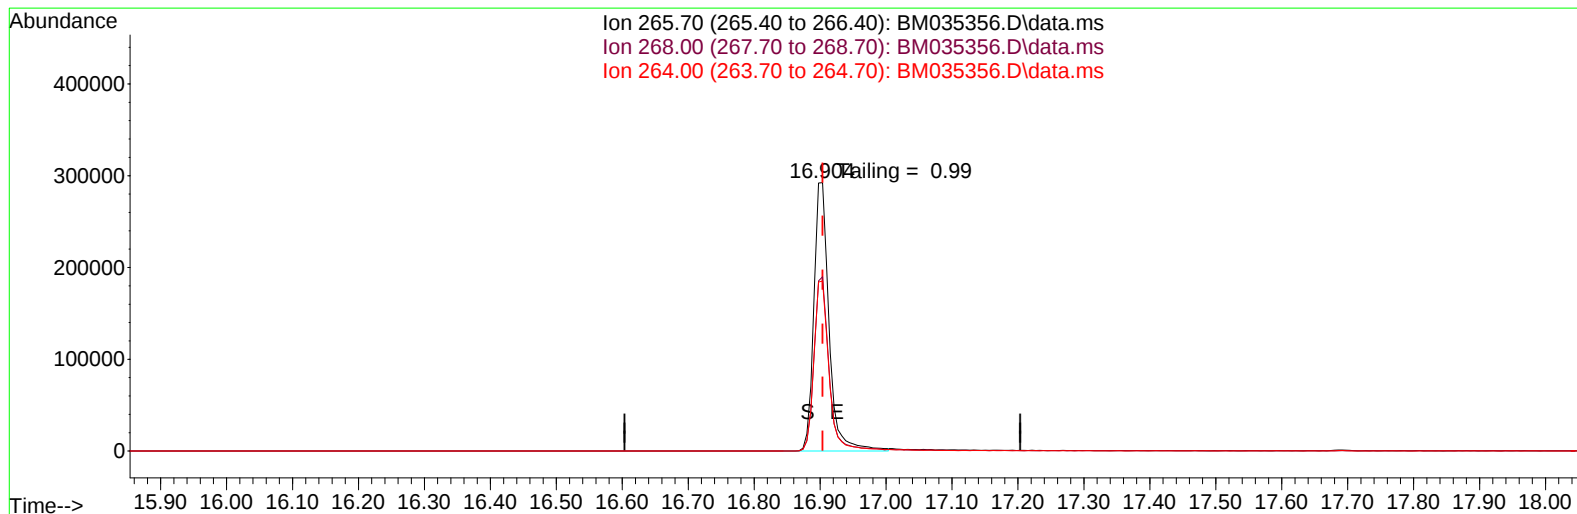

TIC: BM035356.D\data.ms

(70) Pentachlorophenol (C)

16.904min (0.000) 956069.29 ng




response 474712

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.92
264.00	63.30	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
 Data File : BM035356.D
 Acq On : 02 Jun 2022 11:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 02 16:23:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 02 16:16:23 2022
 Response via : Initial Calibration

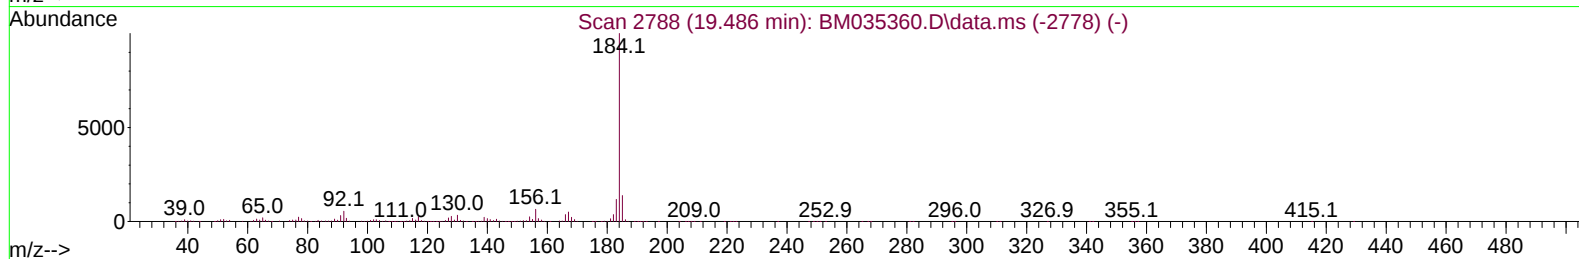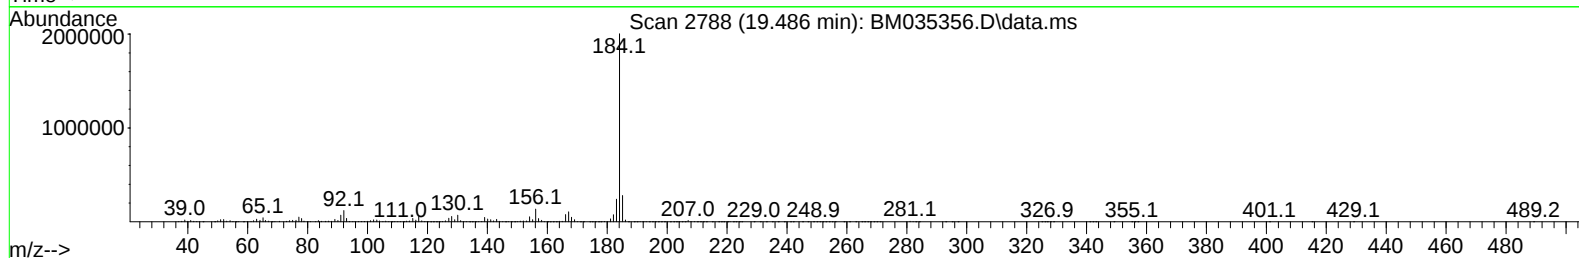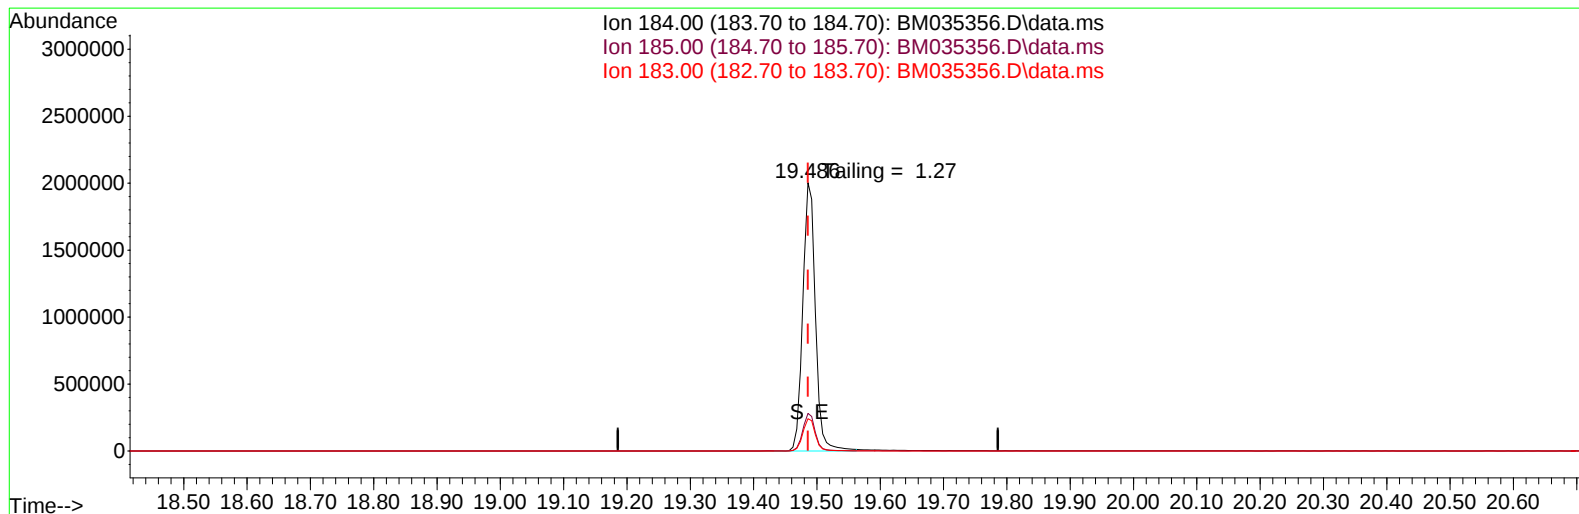

TIC: BM035356.D\data.ms

(77) Benzidine

19.486min (0.000) 503605.67 ng

response 2825082

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.01
183.00	11.90	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/2/2022	BNA_M	<u>BM035356.D</u>
Compound Name	Response	Retention Time
DDT	1639734	20.72
DDD	7900	20.28
DDE	2413	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10313	1650047	0.63

Instrument :
BNA_M
ClientSampleId :
DFTPP