
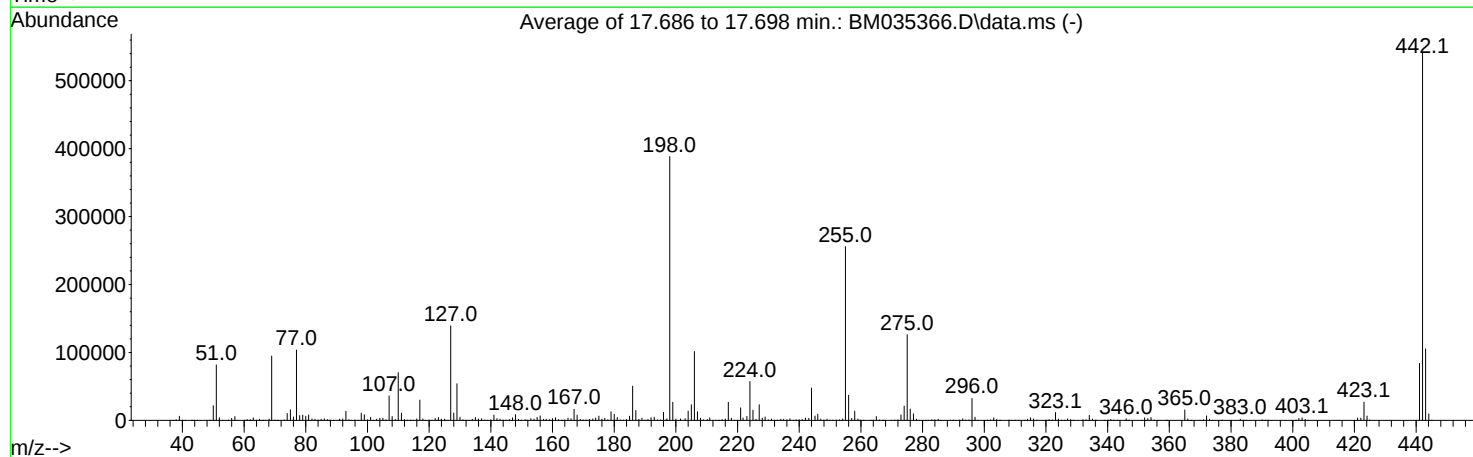


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
 Data File : BM035366.D
 Acq On : 02 Jun 2022 17:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 16:16:23 2022

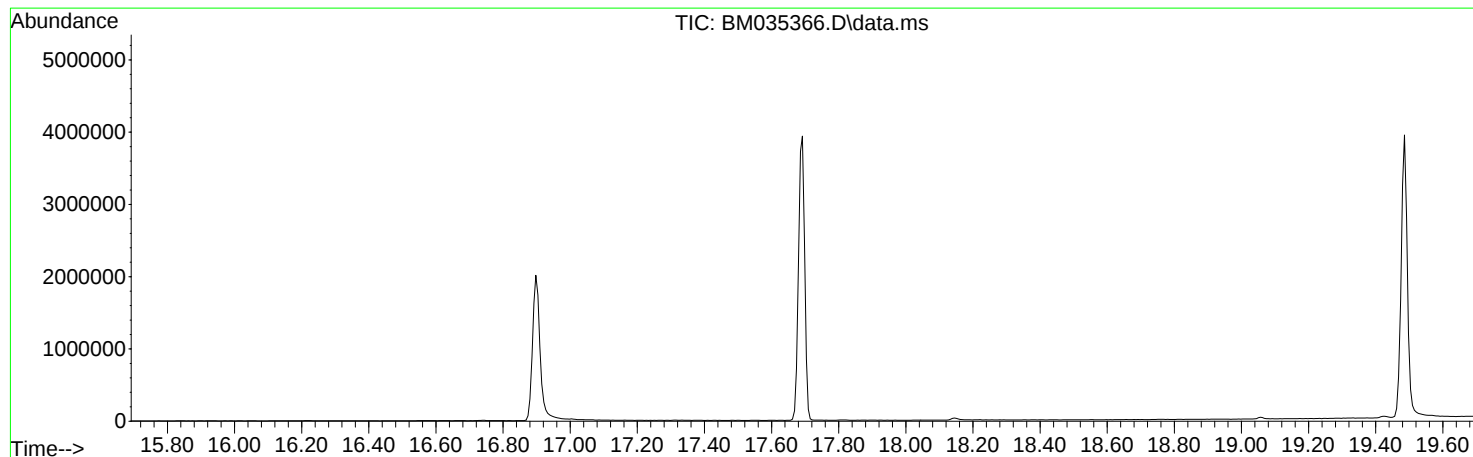




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.0	81656	PASS
68	69	0.00	2	2.0	1874	PASS
69	198	0.00	100	24.4	94801	PASS
70	69	0.00	2	0.6	541	PASS
127	198	10	80	35.8	139203	PASS
197	198	0.00	2	0.6	2164	PASS
198	198	100	100	100.0	388373	PASS
199	198	5	9	6.9	26619	PASS
275	198	10	60	32.5	126179	PASS
365	198	1	100	4.0	15427	PASS
441	198	0.01	100	21.6	83856	PASS
442	442	50	100	100.0	541568	PASS
443	442	15	24	19.4	105248	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035366.D
Acq On : 02 Jun 2022 17:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 03 04:46:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 16:16:23 2022
Response via : Initial Calibration

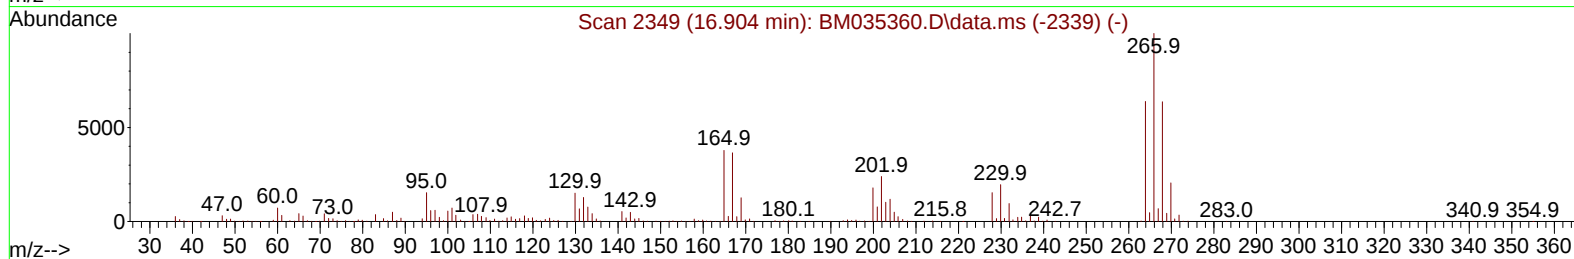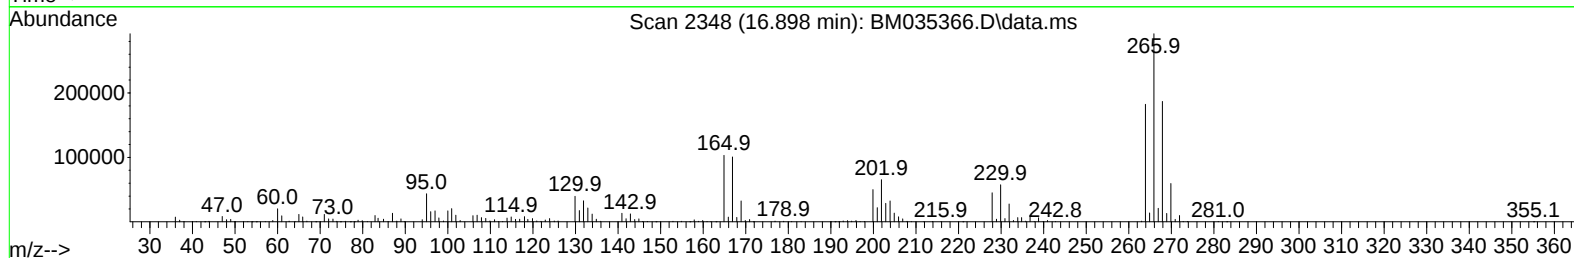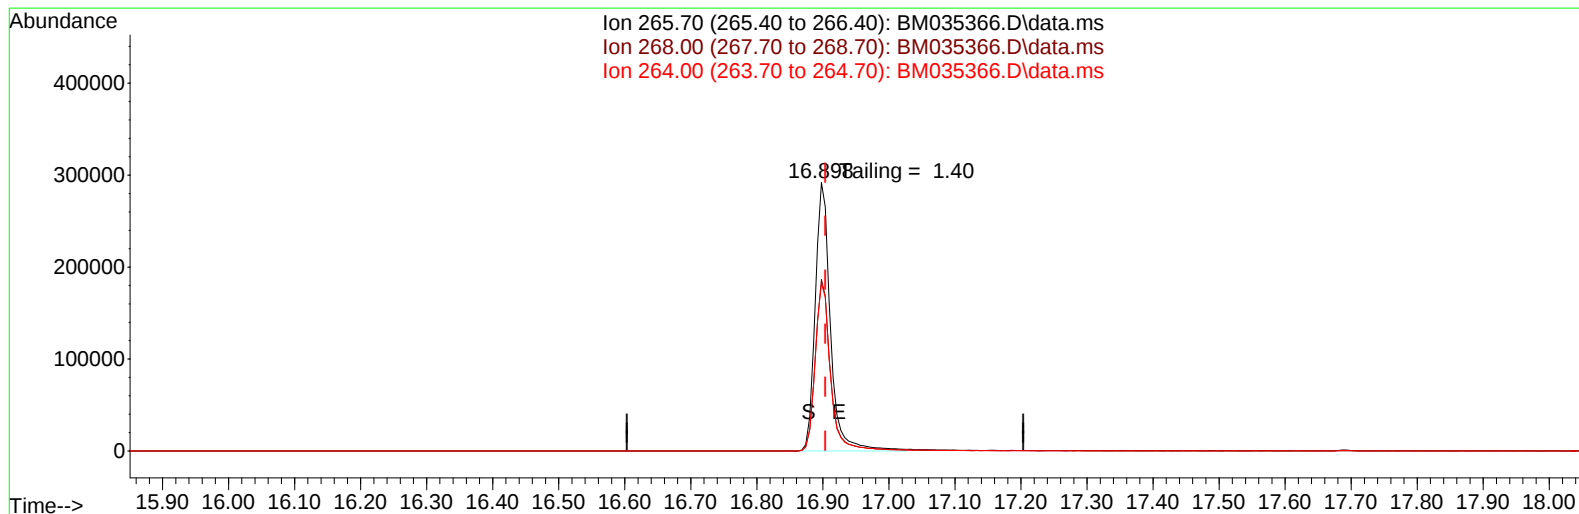

TIC: BM035366.D\data.ms

(70) Pentachlorophenol (C)

16.898min (-0.006) 527289.38 ng




response 472825

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.99
264.00	63.30	62.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060222\
Data File : BM035366.D
Acq On : 02 Jun 2022 17:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 03 04:46:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 16:16:23 2022
Response via : Initial Calibration

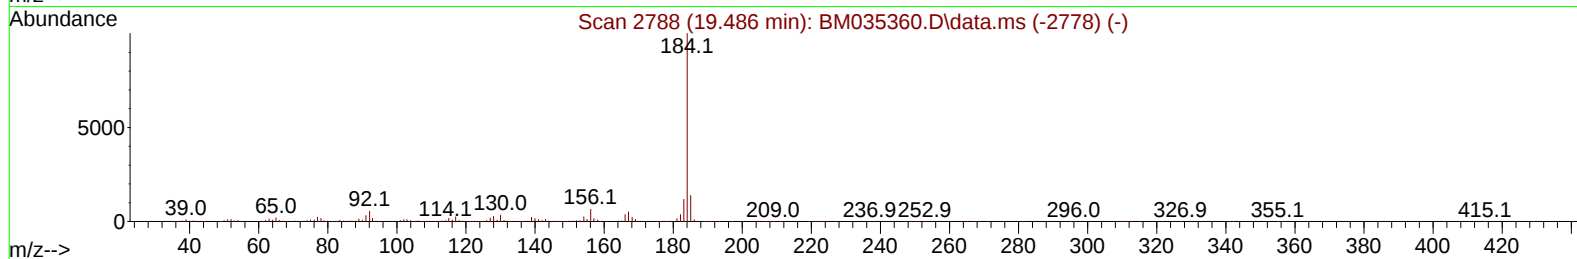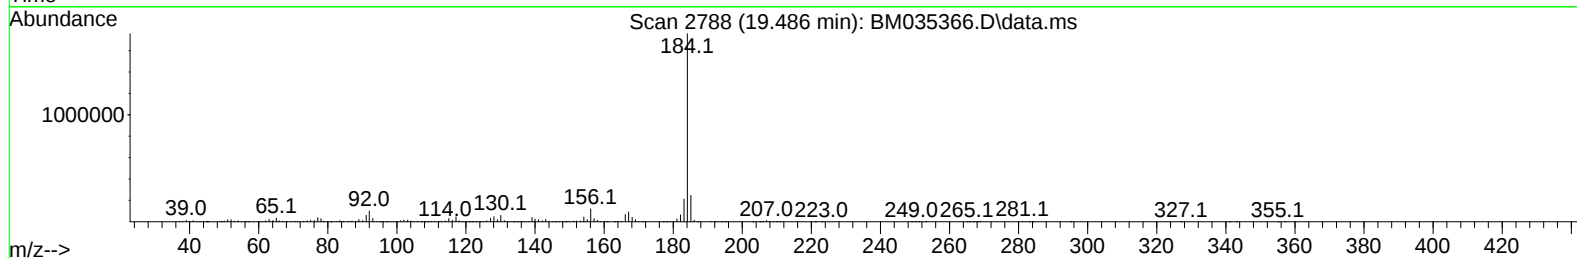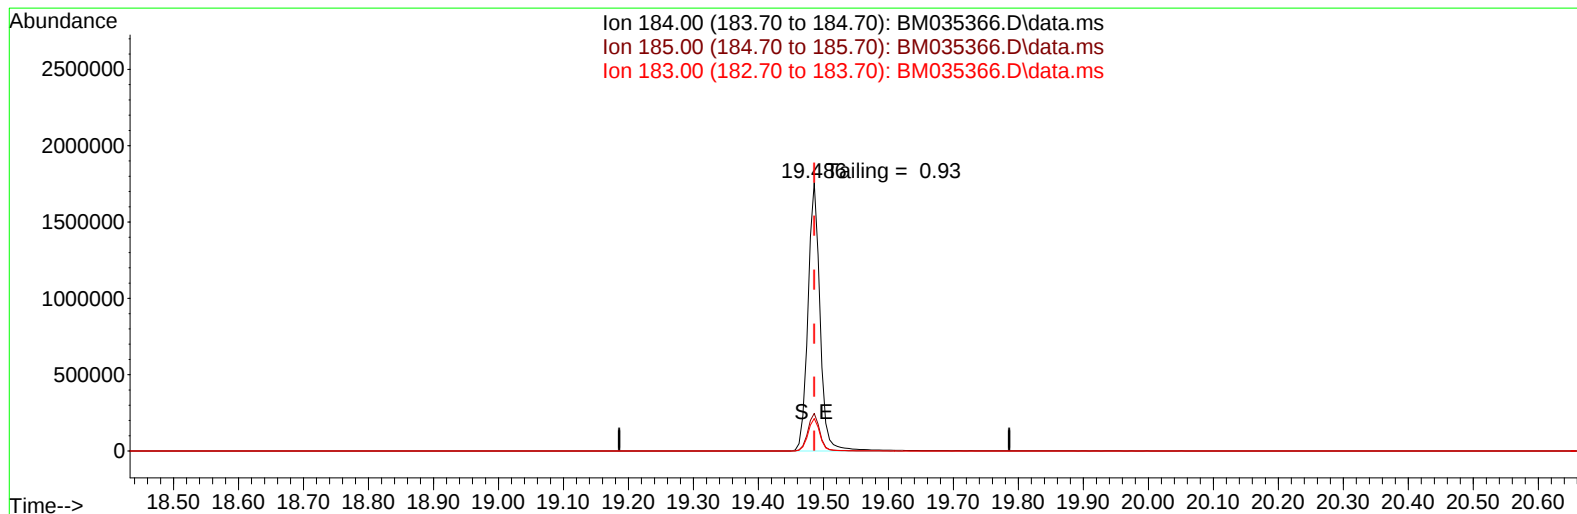

TIC: BM035366.D\data.ms

(77) Benzidine

19.486min (+ 0.000) 105656.54 ng

response 2289264

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.05
183.00	11.90	12.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/2/2022	BNA_M	<u>BM035366.D</u>
Compound Name	Response	Retention Time
DDT	1391074	20.721
DDD	21873	20.28
DDE	2038	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23911	1414985	1.69

Instrument :
BNA_M
ClientSampleId :
DFTPP