

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060315\
 Data File : BM001540.D
 Acq On : 03 Jun 2015 18:24
 Operator : TP/IZ
 Sample : SSTDICC010
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010

Manual Integrations
 APPROVED

apatel
 6/5/2015 8:04:00 AM

Quant Time: Jun 04 03:59:46 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 04 03:14:13 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	29178	5.00	ng	0.00
6) Naphthalene-d8	10.49	136	104831	5.00	ng	0.00
12) Acenaphthene-d10	14.35	164	49962	5.00	ng	0.00
18) Phenanthrene-d10	17.09	188	126260	5.00	ng	0.00
25) Chrysene-d12	21.28	240	79060	5.00	ng	0.00
32) Perylene-d12	23.53	264	77779	5.00	ng	0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.28	112	65256	10.16	ng	0.00
5) Phenol-d6	6.86	99	82279	10.37	ng	0.00
7) Nitrobenzene-d5	8.86	82	76328	11.49	ng	0.00
13) 2,4,6-Tribromophenol	15.83	330	20616	19.26	ng	0.00
14) 2-Fluorobiphenyl	12.97	172	142296	9.51	ng	0.00
27) Terphenyl-d14	19.73	244	97081	9.93	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.21	88	25462	8.35	ng	96
3) n-Nitrosodimethylamine	3.51	42	43512	10.46	ng	97
8) Nitrobenzene	8.90	77	80892	11.47	ng	99
9) Naphthalene	10.52	128	210067	9.50	ng	98
10) Hexachlorobutadiene	10.82	225	36008	9.34	ng	100
11) 2-Methylnaphthalene	12.16	142	134088	9.65	ng	99
15) Acenaphthylene	14.07	152	225491	10.53	ng	100
16) Acenaphthene	14.41	154	131394	9.90	ng	95
17) Fluorene	15.39	166	118175	5.67	ng	99
19) 4-Bromophenyl-phenylether	16.27	248	40126	18.55	ng	# 88
20) Hexachlorobenzene	16.41	284	24132	5.39	ng	# 100
21) Pentachlorophenol	16.75	266	16616	8.49	ng	95
22) Phenanthrene	17.12	178	327380	13.62	ng	99
23) Anthracene	17.23	178	157525m	6.19	ng	
24) Fluoranthene	19.15	202	234892	10.35	ng	99
26) Pyrene	19.52	202	244408	10.18	ng	100
28) Benzo(a)anthracene	21.27	228	219826	10.27	ng	97
29) Chrysene	21.31	228	190835	9.46	ng	97
30) Bis(2-ethylhexyl)phthalate	21.21	149	178482	11.66	ng	99
31) Indeno(1,2,3-cd)pyrene	25.78	276	221416	9.92	ng	99
33) Benzo(b)fluoranthene	22.85	252	217070	9.86	ng	96
34) Benzo(k)fluoranthene	22.90	252	180515	9.20	ng	97
35) Benzo(a)pyrene	23.43	252	187287	9.85	ng	97
36) Dibenzo(a,h)anthracene	25.80	278	173140	9.23	ng	95
37) Benzo(g,h,i)perylene	26.48	276	179359	9.14	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060315\
Data File : BM001540.D
Acq On : 03 Jun 2015 18:24
Operator : TP/IZ
Sample : SSTDIC010
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
SSTDIC010

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:00 AM

Quant Time: Jun 04 03:59:46 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 04 03:14:13 2015
Response via : Initial Calibration

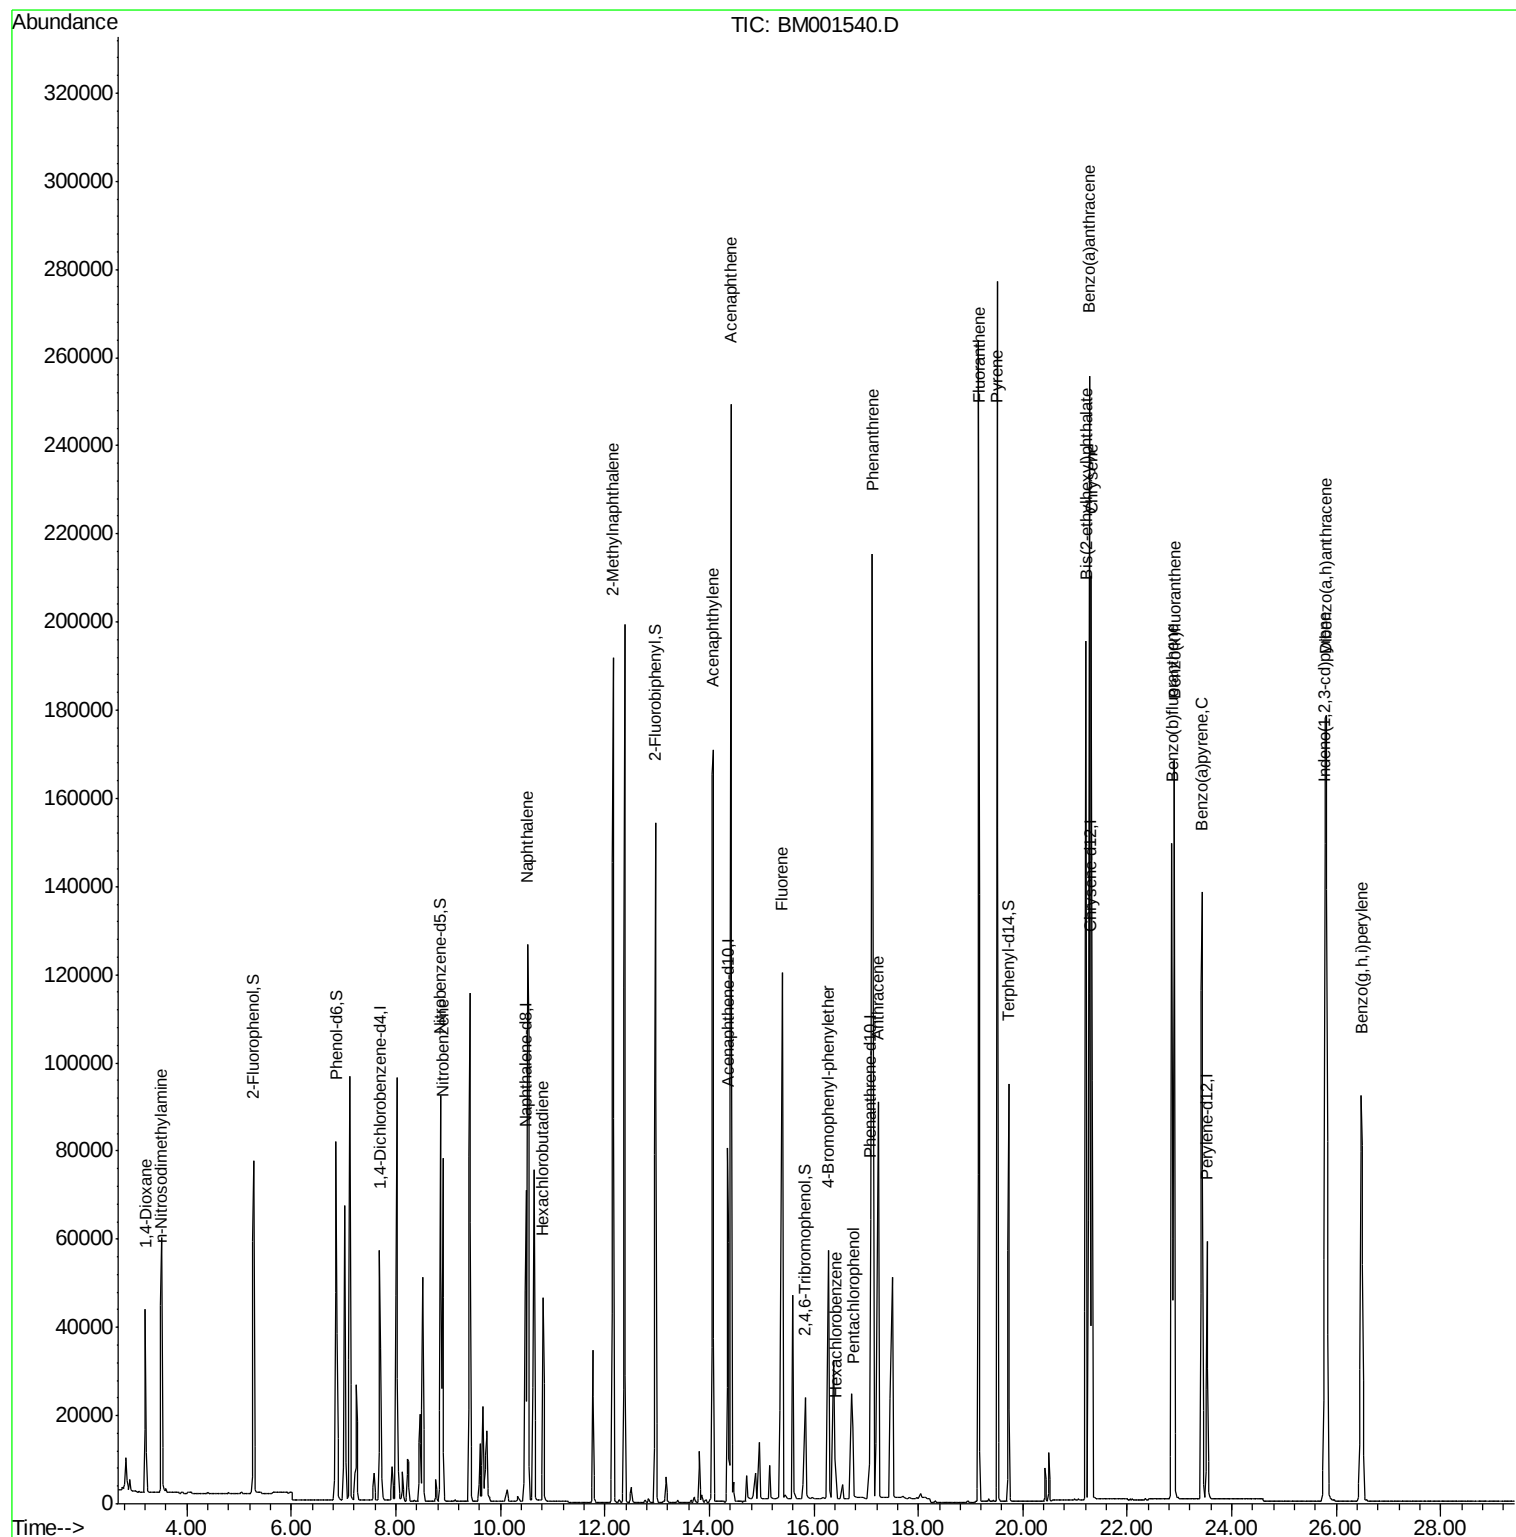

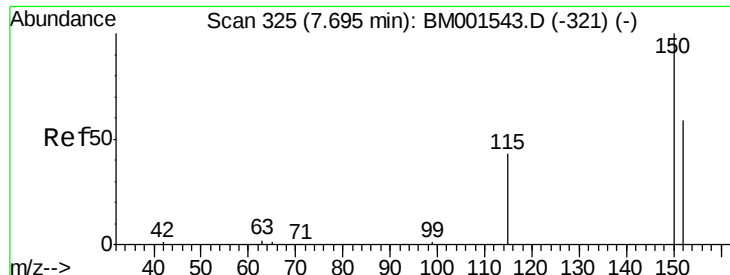

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.69 min Scan# 325

Delta R.T. -0.00 min

Lab File: BM001540.D


Acq: 03 Jun 2015 18:24

Instrument :

BNA_M

ClientSampleId :

SSTDIC010

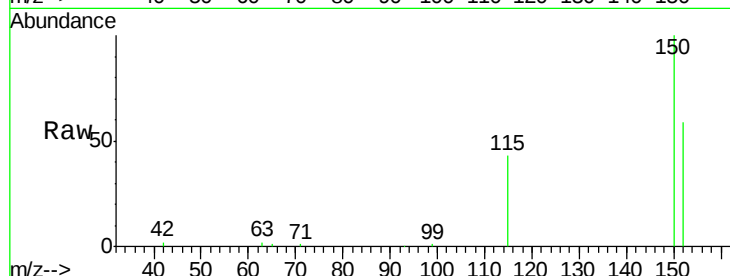

Tgt Ion:152 Resp: 29178

Ion Ratio Lower Upper




152 100

150 169.8 135.0 202.4

115 73.6 57.8 86.8

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:00 AM

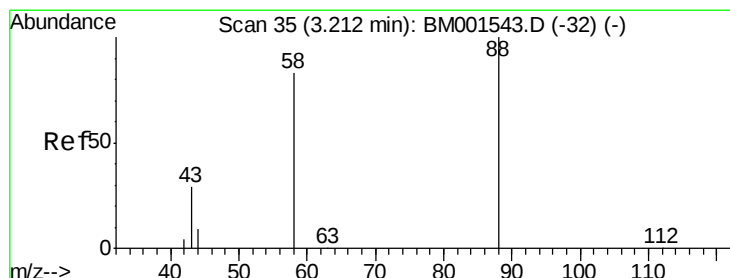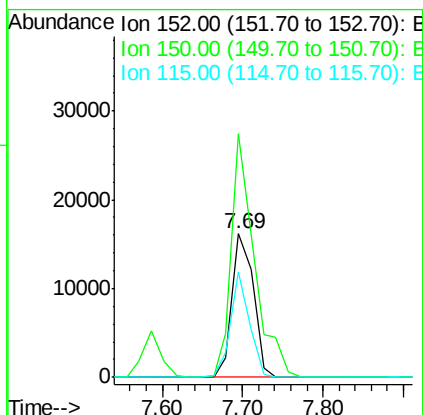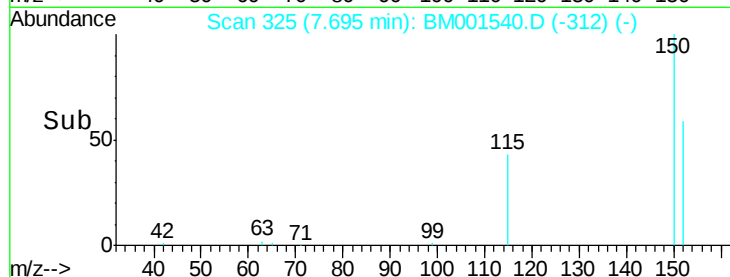

#2

1,4-Dioxane

Concen: 8.35 ng

RT: 3.21 min Scan# 35

Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24




Tgt Ion: 88 Resp: 25462


Ion Ratio Lower Upper

88 100

58 85.9 65.0 97.4

43 40.2 31.1 46.7

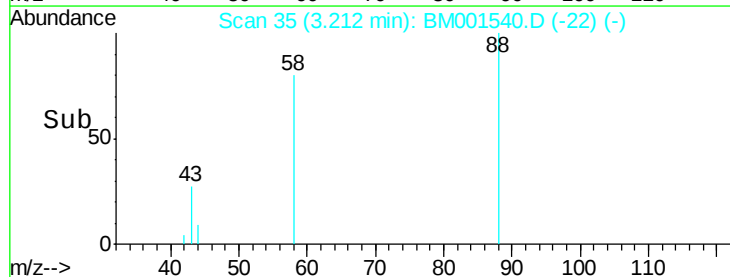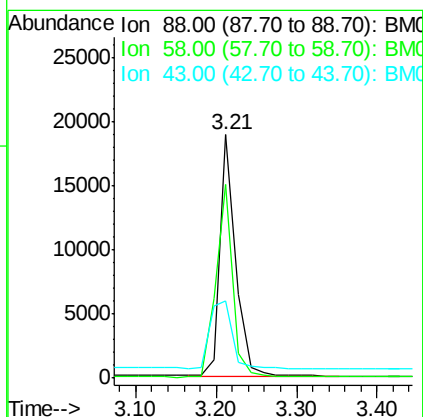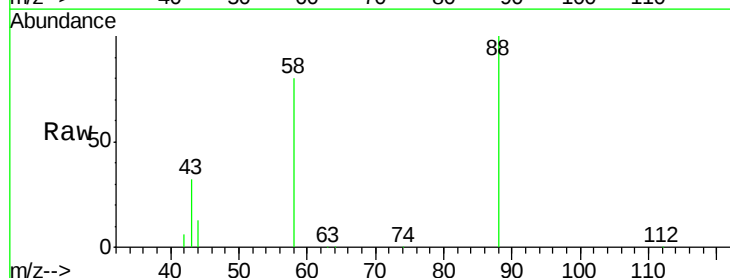

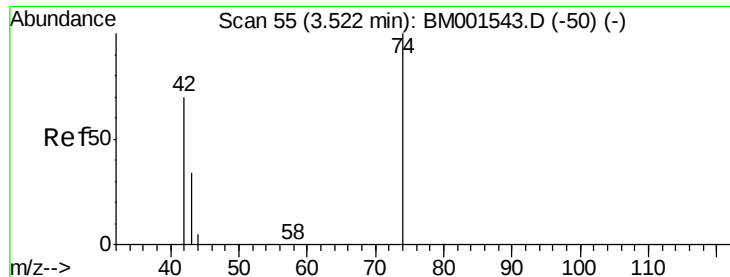





#3
n-Nitrosodimethylamine
Concen: 10.46 ng
RT: 3.51 min Scan# 54
Delta R.T. -0.02 min
Lab File: BM001540.D
Acq: 03 Jun 2015 18:24

Instrument :
BNA_M
ClientSampleId :
SSTDIC010

Tgt Ion	Ratio	Lower	Upper
42	100		
74	99.5	82.0	123.0
44	6.1	5.8	8.6




Manual Integrations
APPROVED


apatel
6/5/2015 8:04:00 AM

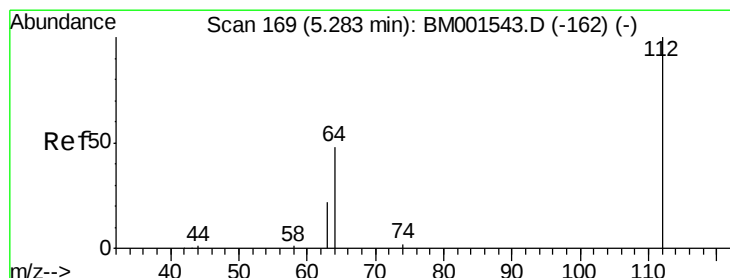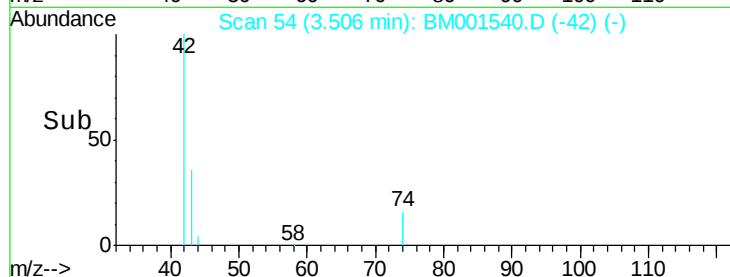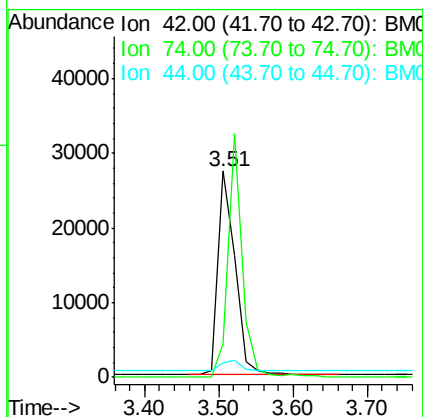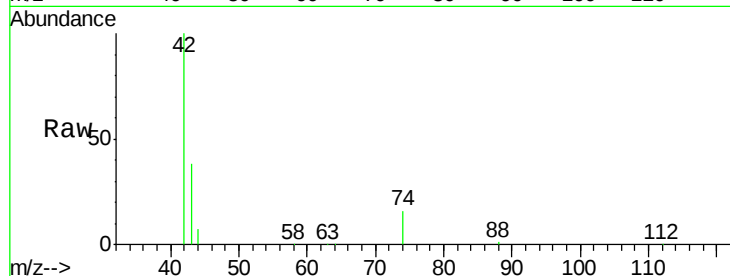

#4
2-Fluorophenol
Concen: 10.16 ng
RT: 5.28 min Scan# 169
Delta R.T. -0.00 min
Lab File: BM001540.D
Acq: 03 Jun 2015 18:24

Tgt Ion	Ratio	Lower	Upper
112	100		
64	66.9	53.0	79.4
63	36.7	29.2	43.8

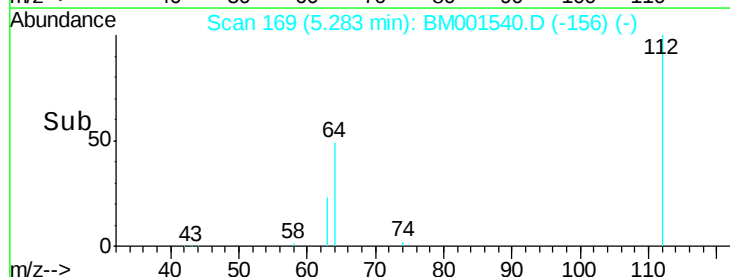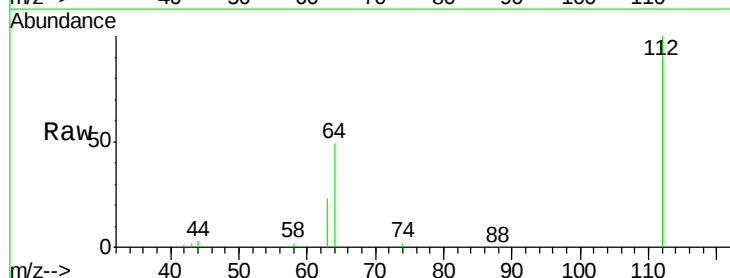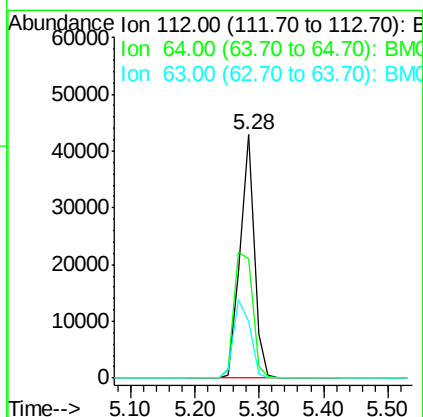



#5

Phenol-d6

Concen: 10.37 ng

RT: 6.86 min Scan# 271

Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Instrument :

BNA_M





ClientSampleId :

SSTDIC010

Tgt Ion:	99	Resp:	82279
Ion Ratio	Lower	Upper	
99	100		
42	26.2	20.9	31.3
71	35.4	28.5	42.7

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:00 AM

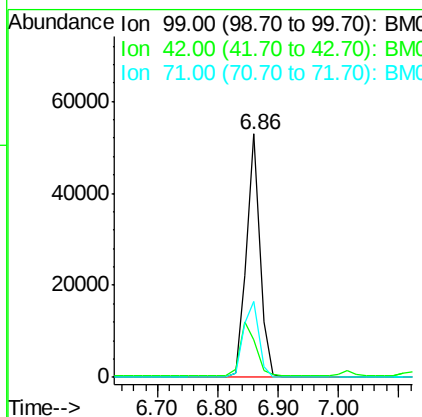

#6

Naphthalene-d8

Concen: 5.00 ng




RT: 10.49 min Scan# 553


Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Tgt Ion:	136	Resp:	104831
Ion Ratio	Lower	Upper	
136	100		
137	11.3	9.1	13.7
54	6.1	4.6	6.8
68	4.2	3.2	4.8

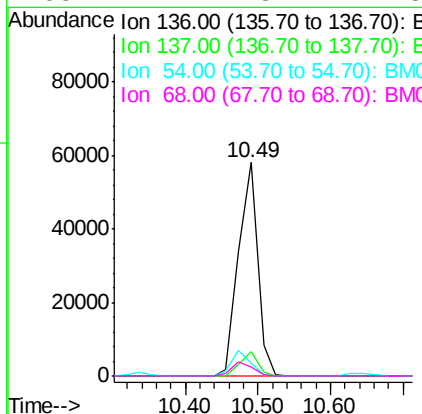

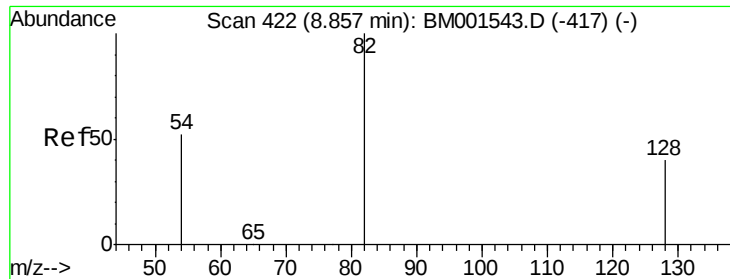

#7

Nitrobenzene-d5

Concen: 11.49 ng

RT: 8.86 min Scan# 422

Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Instrument :

BNA_M





ClientSampleId :

SSTDICC010

Tgt Ion:	82	Resp:	76328
Ion Ratio	Lower	Upper	
82	100		
128	38.3	32.3	48.5
54	54.3	43.0	64.4

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:00 AM

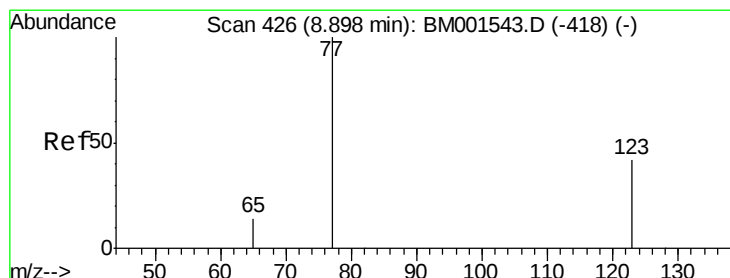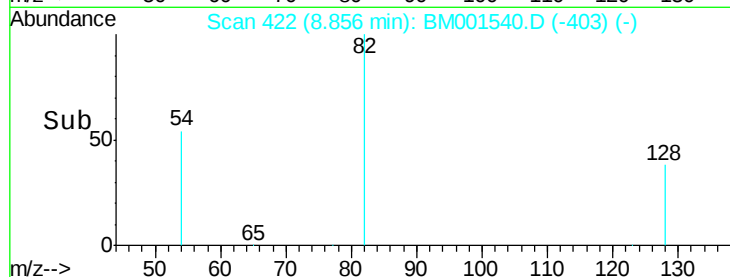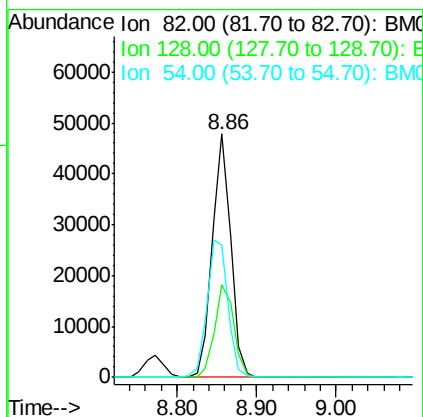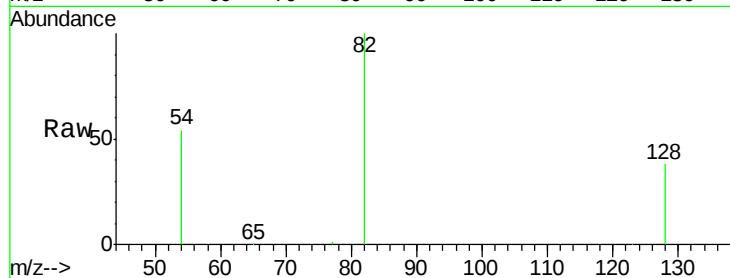

#8

Nitrobenzene

Concen: 11.47 ng




RT: 8.90 min Scan# 426


Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Tgt Ion:	77	Resp:	80892
Ion Ratio	Lower	Upper	
77	100		
123	41.7	32.5	48.7
65	14.6	11.8	17.6

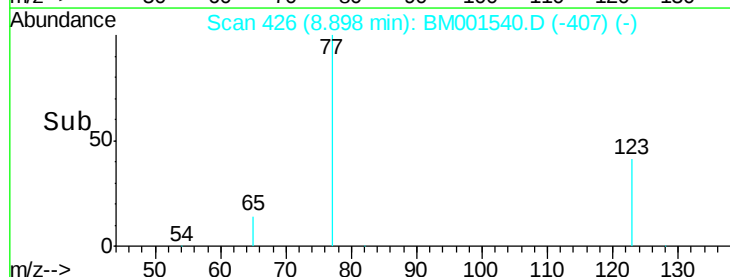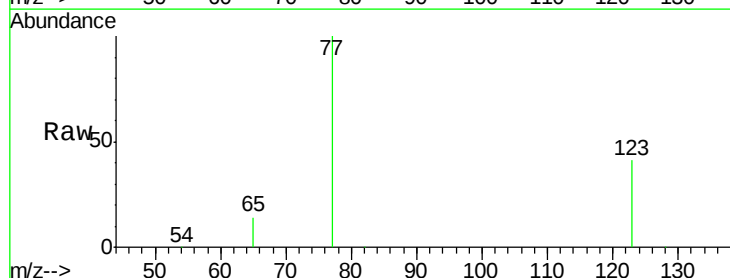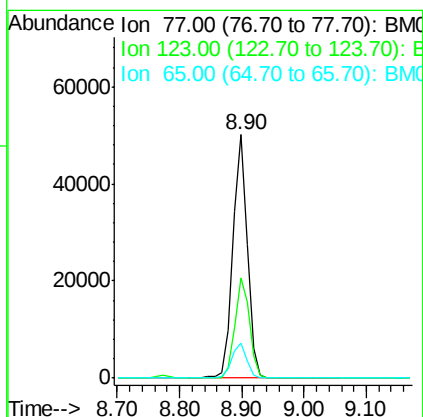



#9

Naphthalene

Concen: 9.50 ng

RT: 10.52 min Scan# 555

Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Instrument :

BNA_M





ClientSampleId :

SSTDICC010

Tgt Ion:	128	Resp:	210067
Ion Ratio		Lower	Upper
128	100		
129	10.1	8.5	12.7
127	13.9	11.7	17.5

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:00 AM

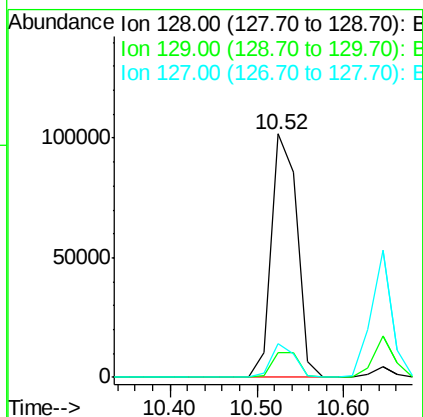

#10

Hexachlorobutadiene

Concen: 9.34 ng




RT: 10.82 min Scan# 572


Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Tgt Ion:	225	Resp:	36008
Ion Ratio		Lower	Upper
225	100		
223	62.7	50.2	75.2
227	63.5	50.5	75.7

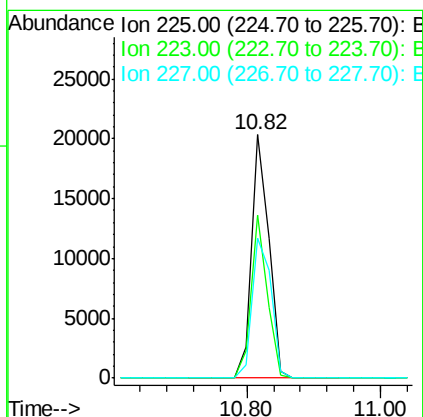

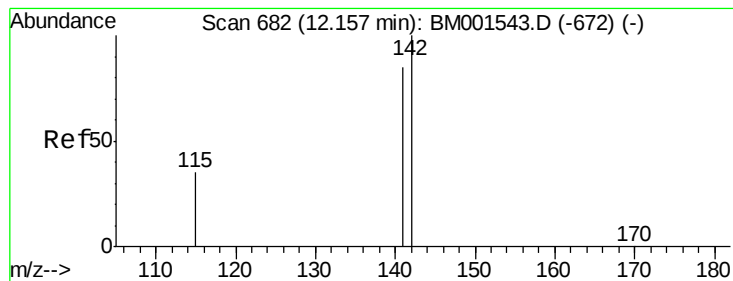

#11

2-Methylnaphthalene

Concen: 9.65 ng

RT: 12.16 min Scan# 682

Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Instrument :

BNA_M





ClientSampleId :

SSTDIC010

Tgt Ion:	142	Resp:	134088
Ion Ratio	Lower	Upper	
142	100		
141	85.6	68.1	102.1
115	35.1	28.3	42.5

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:00 AM

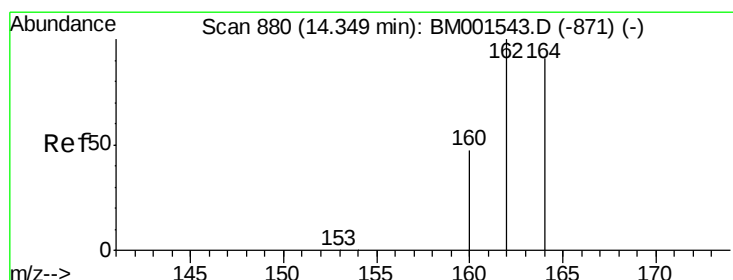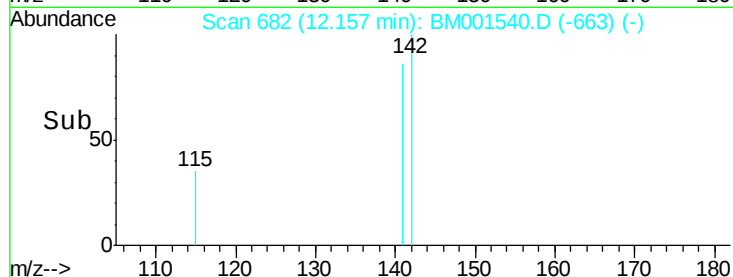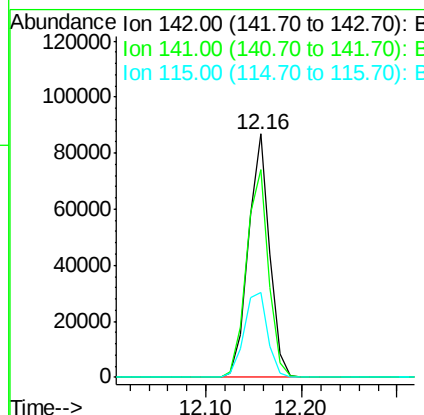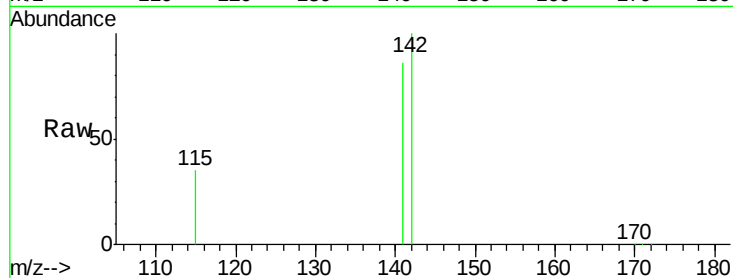

#12

Acenaphthene-d10

Concen: 5.00 ng




RT: 14.35 min Scan# 880


Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Tgt Ion:	164	Resp:	49962
Ion Ratio	Lower	Upper	
164	100		
162	111.3	88.0	132.0
160	52.8	41.0	61.4

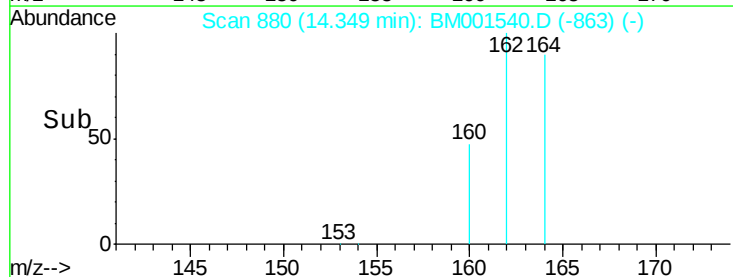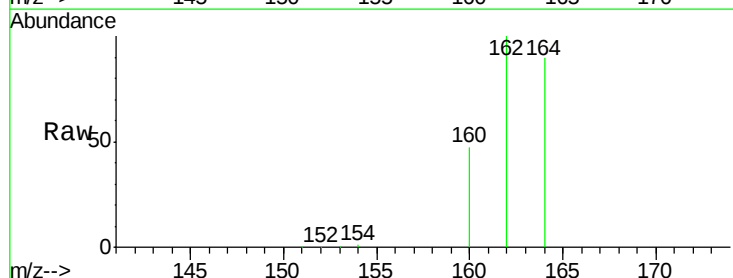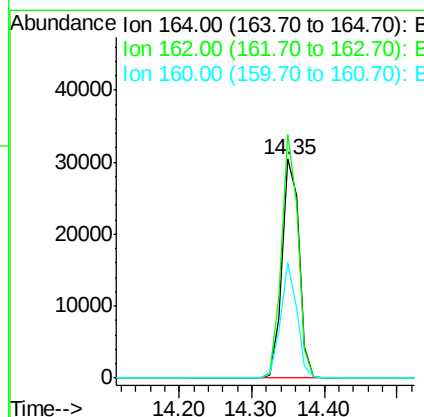




#13
 2,4,6-Tribromophenol
 Concen: 19.26 ng
 RT: 15.83 min Scan# 943
 Delta R.T. -0.00 min
 Lab File: BM001540.D
 Acq: 03 Jun 2015 18:24

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010




Tgt Ion	Ratio	Resp	Lower	Upper
330	100	20616		
332	84.8	69.6	104.4	
141	0.0	0.0	0.0	

Manual Integrations
 APPROVED

apatel
 6/5/2015 8:04:00 AM






Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

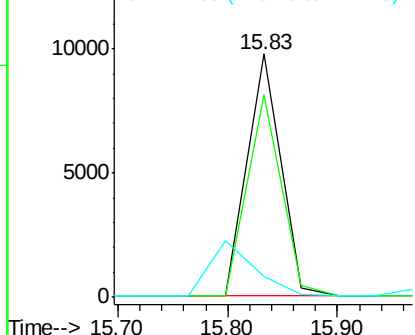


#14
 2-Fluorobiphenyl
 Concen: 9.51 ng
 RT: 12.97 min Scan# 760
 Delta R.T. -0.00 min
 Lab File: BM001540.D
 Acq: 03 Jun 2015 18:24

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	142296		
171	34.7	27.6	41.4	
170	23.3	18.4	27.6	

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

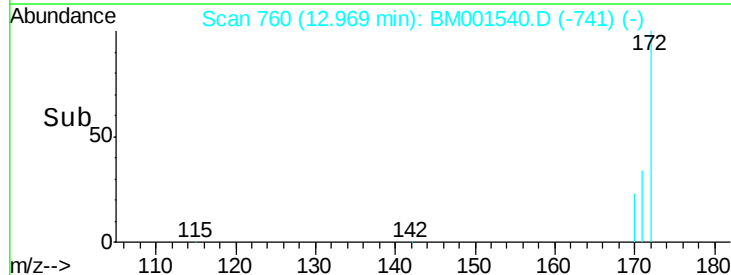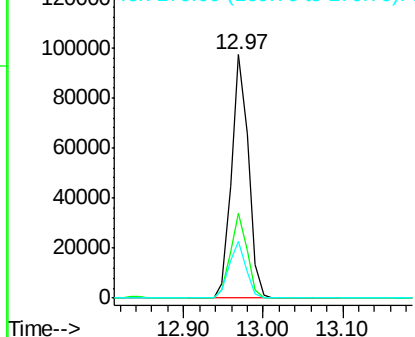







#15
Acenaphthylene
Concen: 10.53 ng
RT: 14.07 min Scan# 857
Delta R.T. 0.01 min
Lab File: BM001540.D
Acq: 03 Jun 2015 18:24

Instrument :
BNA_M
ClientSampleId :
SSTDIC010

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.3	22.9
153	12.9	10.3	15.5




Manual Integrations
APPROVED


apatel
6/5/2015 8:04:00 AM

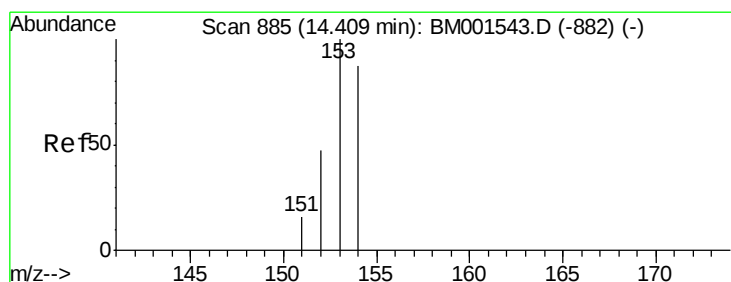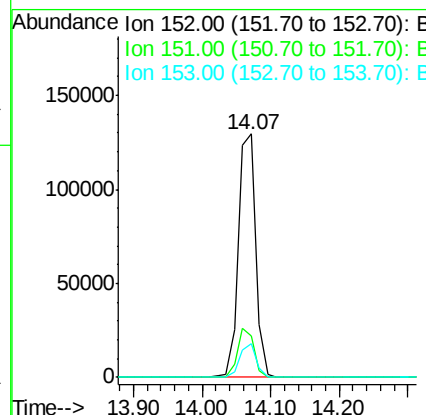

#16
Acenaphthene
Concen: 9.90 ng
RT: 14.41 min Scan# 885
Delta R.T. -0.00 min
Lab File: BM001540.D
Acq: 03 Jun 2015 18:24

Tgt Ion	Ratio	Lower	Upper
154	100		
153	106.7	89.8	134.8
152	51.1	43.0	64.6

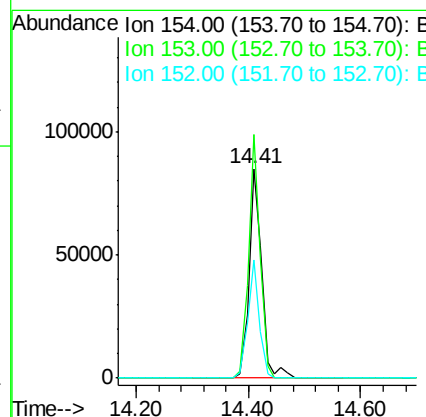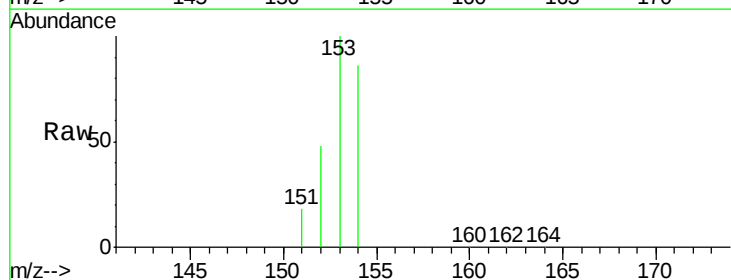



#17

Fluorene

Concen: 5.67 ng

RT: 15.39 min Scan# 930

Delta R.T. -0.00 min

Lab File: BM001540.D


Acq: 03 Jun 2015 18:24

Instrument :

BNA_M

ClientSampleId :




SSTDICC010



Tgt Ion:	166	Resp:	118175
Ion Ratio	Lower	Upper	
166	100		
165	84.0	68.2	102.2
167	14.9	12.1	18.1

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:00 AM

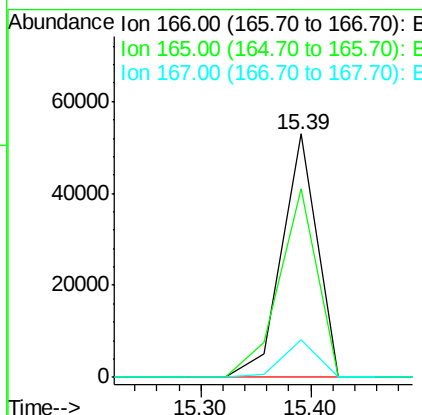

#18

Phenanthrene-d10

Concen: 5.00 ng




RT: 17.09 min Scan# 980


Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Tgt Ion:	188	Resp:	126260
Ion Ratio	Lower	Upper	
188	100		
94	1.3	1.0	1.4
80	1.4	0.8	1.2#

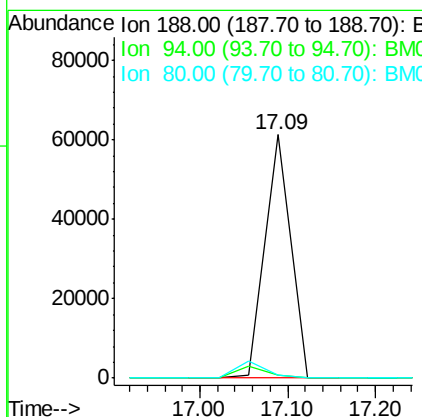







#19
4-Bromophenyl-phenylether
Concen: 18.55 ng
RT: 16.27 min Scan# 956
Delta R.T. -0.00 min
Lab File: BM001540.D
Acq: 03 Jun 2015 18:24

Instrument :
BNA_M
ClientSampleId :
SSTDICC010

Tgt Ion	Ratio	Lower	Upper
248	100		
250	66.4	55.2	82.8
141	98.7	64.7	97.1




Manual Integrations
APPROVED


apatel
6/5/2015 8:04:00 AM

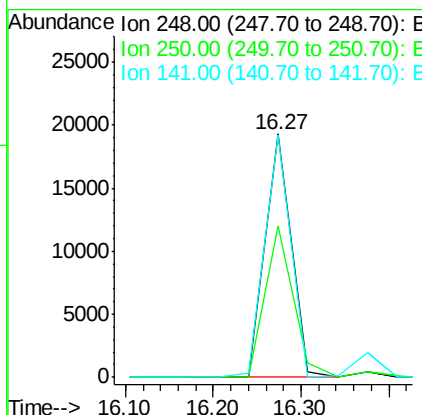

#20
Hexachlorobenzene
Concen: 5.39 ng
RT: 16.41 min Scan# 960
Delta R.T. -0.00 min
Lab File: BM001540.D
Acq: 03 Jun 2015 18:24

Tgt Ion	Ratio	Lower	Upper
284	100		
142	0.0	0.0	0.0
249	0.0	0.0	0.0

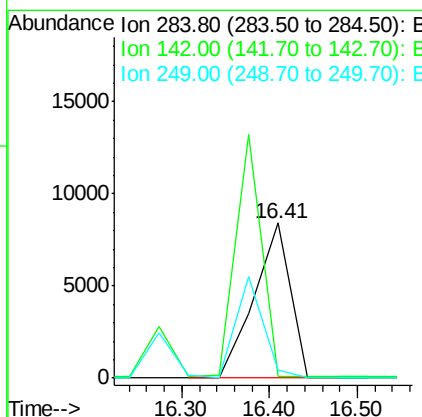



#21

Pentachlorophenol

Concen: 8.49 ng

RT: 16.75 min Scan# 970

Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Instrument :

BNA_M





ClientSampleId :

SSTDICC010

Tgt Ion:	266	Resp:	16616
Ion Ratio	Lower	Upper	
266	100		
268	80.7	67.2	100.8
264	48.8	43.7	65.5

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:00 AM

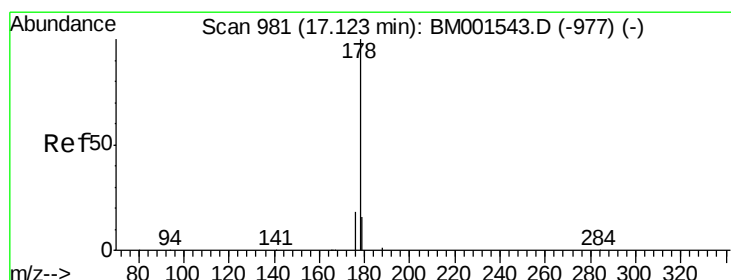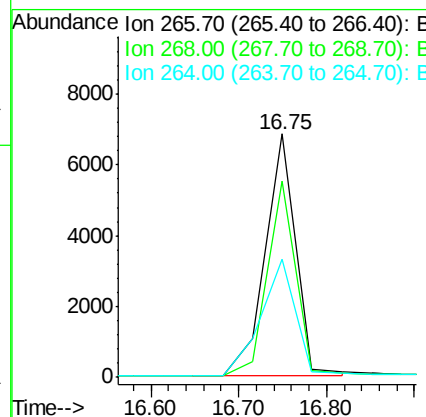

#22

Phenanthrene

Concen: 13.62 ng




RT: 17.12 min Scan# 981


Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Tgt Ion:	178	Resp:	327380
Ion Ratio	Lower	Upper	
178	100		
176	18.6	14.7	22.1
179	15.1	12.7	19.1

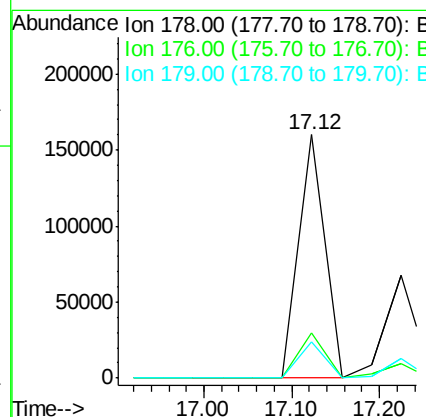







#23
 Anthracene
 Concen: 6.19 ng m
 RT: 17.23 min Scan# 984
 Delta R.T. -0.00 min
 Lab File: BM001540.D
 Acq: 03 Jun 2015 18:24

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010

Tgt Ion	Ratio	Lower	Upper
178	100		
176	12.4	36.6	54.8#
179	16.1	28.7	43.1#




Manual Integrations
 APPROVED


apatel
 6/5/2015 8:04:00 AM

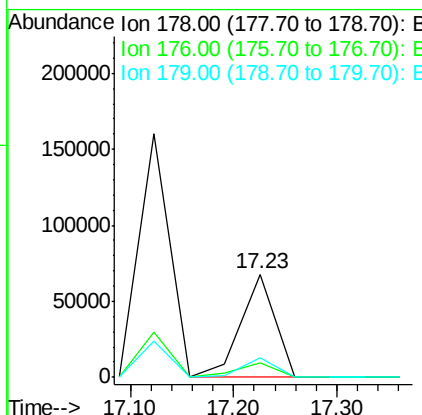

#24
 Fluoranthene
 Concen: 10.35 ng
 RT: 19.15 min Scan# 1089
 Delta R.T. -0.00 min
 Lab File: BM001540.D
 Acq: 03 Jun 2015 18:24

Tgt Ion	Ratio	Lower	Upper
202	100		
101	13.2	10.2	15.2
203	17.4	13.8	20.8

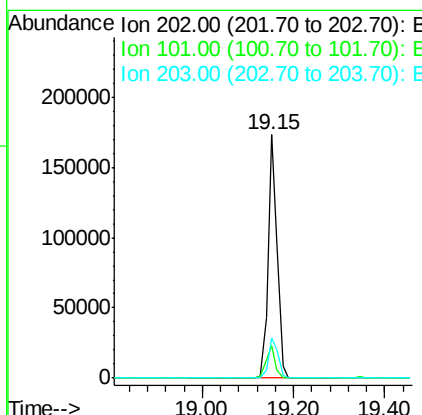



#25

Chrysene-d12

Concen: 5.00 ng

RT: 21.28 min Scan# 1252

Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Instrument :

BNA_M


ClientSampleId :

SSTDIC010




Tgt Ion	Ratio	Lower	Upper
240	100		
120	12.5	5.6	8.4#
236	31.0	22.4	33.6

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:00 AM



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

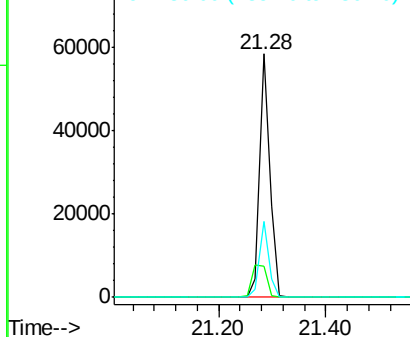

#26

Pyrene

Concen: 10.18 ng


RT: 19.52 min Scan# 1119

Delta R.T. -0.00 min



Lab File: BM001540.D


Acq: 03 Jun 2015 18:24

Tgt Ion	Ratio	Lower	Upper
202	100		
200	20.8	16.6	25.0
203	17.4	13.8	20.8



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E

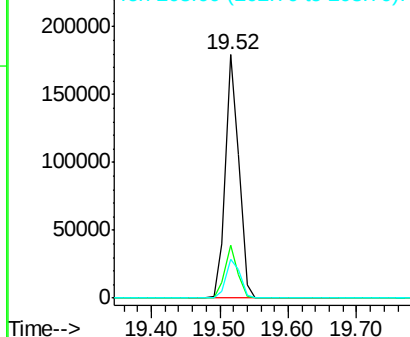

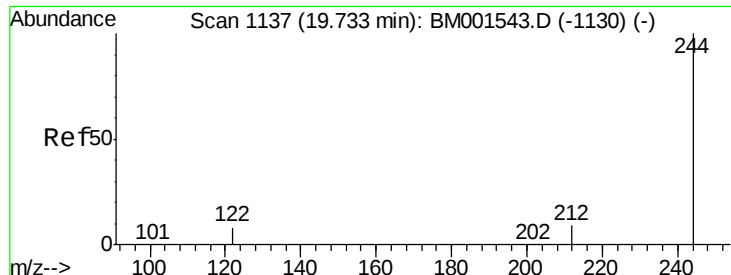





#27
 Terphenyl-d14
 Concen: 9.93 ng
 RT: 19.73 min Scan# 1137
 Delta R.T. -0.00 min
 Lab File: BM001540.D
 Acq: 03 Jun 2015 18:24

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010

Tgt Ion	Ratio	Lower	Upper
244	100		
212	9.5	8.0	12.0
122	11.2	7.3	10.9




Manual Integrations
 APPROVED


apatel
 6/5/2015 8:04:00 AM

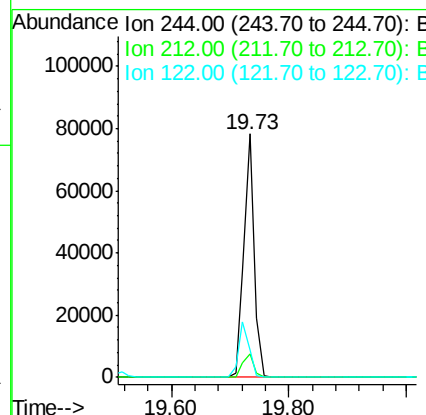

#28
 Benzo(a)anthracene
 Concen: 10.27 ng
 RT: 21.27 min Scan# 1251
 Delta R.T. -0.00 min
 Lab File: BM001540.D
 Acq: 03 Jun 2015 18:24

Tgt Ion	Ratio	Lower	Upper
228	100		
226	25.4	19.0	28.4
229	20.1	16.9	25.3

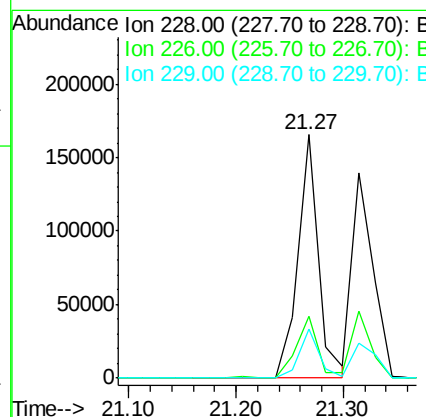



#29

Chrysene

Concen: 9.46 ng

RT: 21.31 min Scan# 1254

Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Instrument :

BNA_M





ClientSampleId :

SSTDICC010

Tgt	Ion	228	Resp:	190835
	Ion	Ratio	Lower	Upper
228	100			
226	32.9	25.2	37.8	
229	16.8	14.7	22.1	

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:00 AM

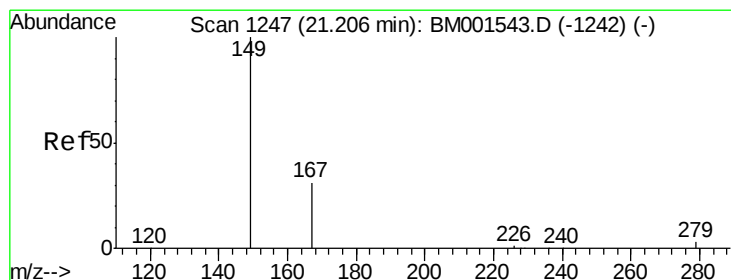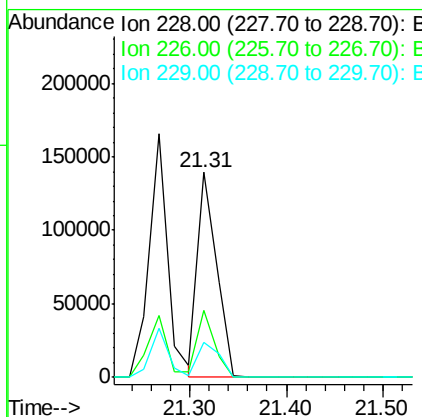

#30

Bis(2-ethylhexyl)phthalate

Concen: 11.66 ng




RT: 21.21 min Scan# 1247


Delta R.T. -0.00 min

Lab File: BM001540.D

Acq: 03 Jun 2015 18:24

Tgt	Ion	149	Resp:	178482
	Ion	Ratio	Lower	Upper
149	100			
167	26.0	20.5	30.7	
279	2.0	1.7	2.5	

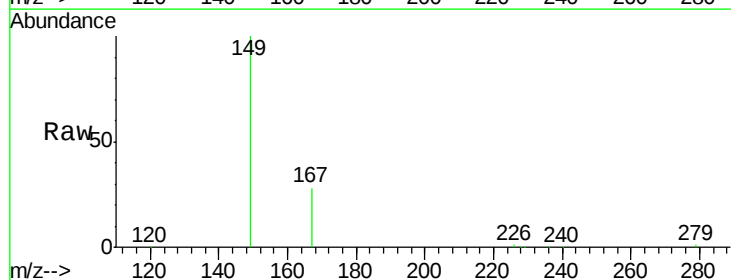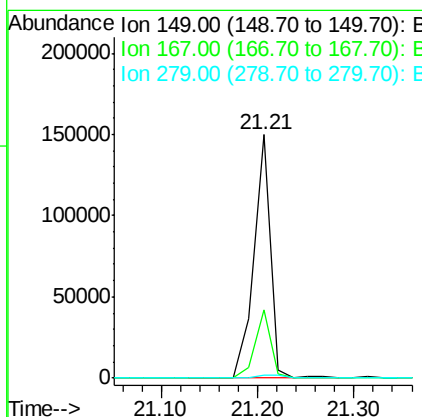

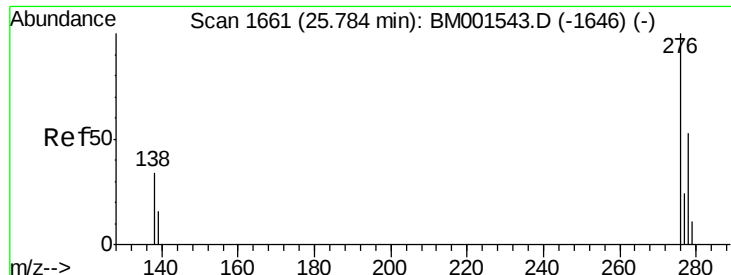





#31
 Indeno(1,2,3-cd)pyrene
 Concen: 9.92 ng
 RT: 25.78 min Scan# 1661
 Delta R.T. -0.00 min
 Lab File: BM001540.D
 Acq: 03 Jun 2015 18:24

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	36.1	28.3	42.5
277	24.6	19.6	29.4




Manual Integrations
 APPROVED


apatel
 6/5/2015 8:04:00 AM

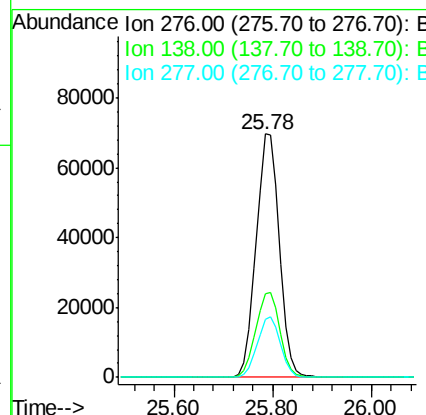

#32
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.53 min Scan# 1445
 Delta R.T. 0.01 min
 Lab File: BM001540.D
 Acq: 03 Jun 2015 18:24

Tgt Ion	Ratio	Resp Lower	Resp Upper
264	100		
260	24.1	21.1	31.7
265	22.6	17.1	25.7

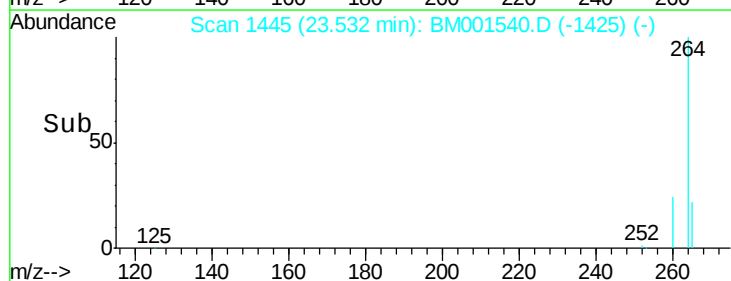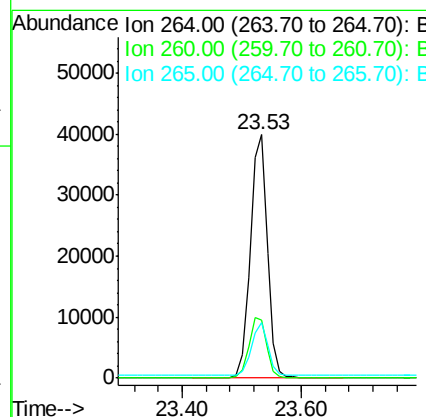



#33

Benzo(b)fluoranthene

Concen: 9.86 ng

RT: 22.85 min Scan# 1380

Delta R.T. 0.01 min

Lab File: BM001540.D


Acq: 03 Jun 2015 18:24

Instrument :

BNA_M

ClientSampleId :



SSTDICC010



Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.0	17.8	26.6
125	12.7	12.5	18.7

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:00 AM

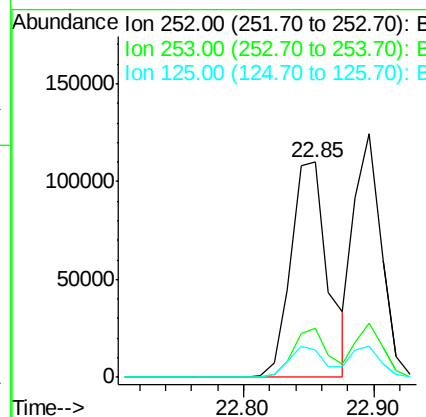

#34

Benzo(k)fluoranthene


Concen: 9.20 ng

RT: 22.90 min Scan# 1384



Delta R.T. 0.01 min


Lab File: BM001540.D

Acq: 03 Jun 2015 18:24



Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.1	17.2	25.8
125	13.0	12.5	18.7

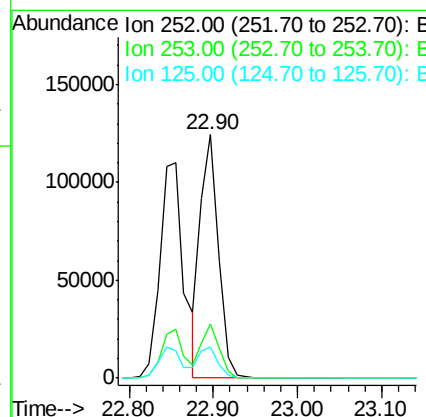







#35
Benzo(a)pyrene
Concen: 9.85 ng
RT: 23.43 min Scan# 1435
Delta R.T. 0.01 min
Lab File: BM001540.D
Acq: 03 Jun 2015 18:24

Instrument :
BNA_M
ClientSampleId :
SSTDIC010

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.1	17.6	26.4
125	14.7	14.3	21.5




Manual Integrations
APPROVED




apatel
6/5/2015 8:04:00 AM

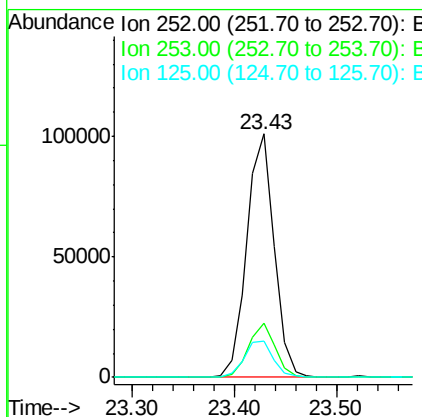

#36
Dibenzo(a,h)anthracene
Concen: 9.23 ng
RT: 25.80 min Scan# 1663
Delta R.T. -0.00 min
Lab File: BM001540.D
Acq: 03 Jun 2015 18:24

Tgt Ion	Ratio	Lower	Upper
278	100		
139	25.3	18.0	27.0
279	22.7	19.8	29.8

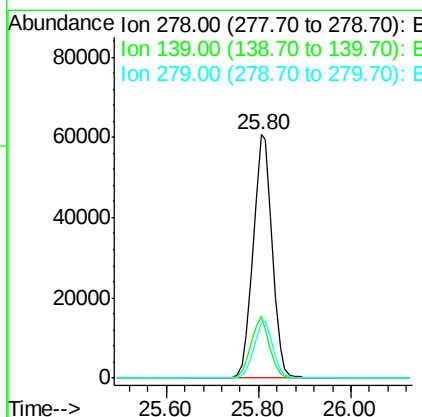

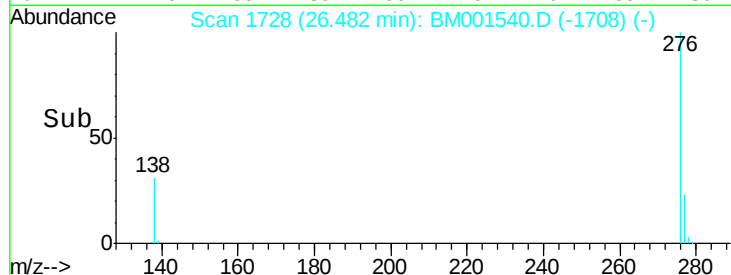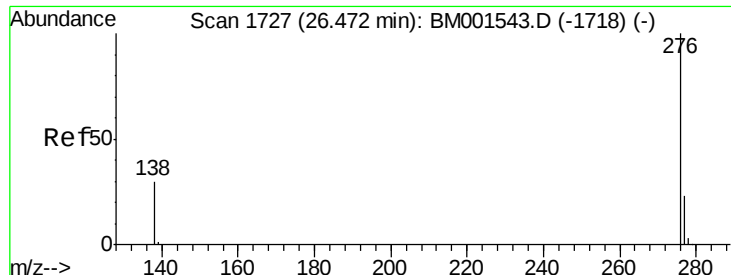

#37
 Benzo(g,h,i)perylene
 Concen: 9.14 ng
 RT: 26.48 min Scan# 1728
 Delta R.T. 0.01 min
 Lab File: BM001540.D
 Acq: 03 Jun 2015 18:24

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC010

Tgt Ion:	276	Resp:	179359
Ion Ratio	Lower	Upper	
276	100		
277	23.3	19.3	28.9
138	30.7	25.0	37.6

Manual Integrations
 APPROVED

apatel
 6/5/2015 8:04:00 AM

