

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060315\
 Data File : BM001543.D
 Acq On : 03 Jun 2015 20:12
 Operator : TP/IZ
 Sample : SSTDICCC001
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICCC001

Manual Integrations
 APPROVED

apatel
 6/5/2015 8:04:11 AM

Quant Time: Jun 04 04:02:14 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 04 03:14:13 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	26032	5.00	ng	0.00
6) Naphthalene-d8	10.49	136	93290	5.00	ng	0.00
12) Acenaphthene-d10	14.35	164	46533	5.00	ng	0.00
18) Phenanthrene-d10	17.09	188	107811	5.00	ng	0.00
25) Chrysene-d12	21.28	240	72860	5.00	ng	0.00
32) Perylene-d12	23.52	264	66329	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.28	112	5891	1.03	ng	0.00
5) Phenol-d6	6.86	99	7212	1.02	ng	0.00
7) Nitrobenzene-d5	8.86	82	6558	1.11	ng	0.00
13) 2,4,6-Tribromophenol	15.83	330	1916	1.92	ng	0.00
14) 2-Fluorobiphenyl	12.97	172	13569	0.97	ng	0.00
27) Terphenyl-d14	19.73	244	9242	1.03	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.21	88	2545	0.94	ng	100
3) n-Nitrosodimethylamine	3.52	42	3892	1.05	ng	100
8) Nitrobenzene	8.90	77	6925	1.10	ng	100
9) Naphthalene	10.52	128	19421	0.99	ng	100
10) Hexachlorobutadiene	10.82	225	3401	0.99	ng	100
11) 2-Methylnaphthalene	12.16	142	12396	1.00	ng	100
15) Acenaphthylene	14.06	152	20116	1.01	ng	100
16) Acenaphthene	14.41	154	11960	0.97	ng	100
17) Fluorene	15.39	166	9674	0.50	ng	100
19) 4-Bromophenyl-phenylether	16.27	248	4233	2.29	ng	100
20) Hexachlorobenzene	16.41	284	2193	0.57	ng	# 100
21) Pentachlorophenol	16.75	266	1160	0.69	ng	100
22) Phenanthrene	17.12	178	31199	1.52	ng	100
23) Anthracene	17.23	178	13836m	0.64	ng	
24) Fluoranthene	19.15	202	21923	1.13	ng	100
26) Pyrene	19.52	202	22723	1.03	ng	100
28) Benzo(a)anthracene	21.27	228	19668	1.00	ng	100
29) Chrysene	21.31	228	18310	0.98	ng	100
30) Bis(2-ethylhexyl)phthalate	21.21	149	14162	1.00	ng	100
31) Indeno(1,2,3-cd)pyrene	25.78	276	19581	0.95	ng	100
33) Benzo(b)fluoranthene	22.84	252	18116	0.97	ng	100
34) Benzo(k)fluoranthene	22.89	252	17354	1.04	ng	100
35) Benzo(a)pyrene	23.42	252	16590	1.02	ng	100
36) Dibenzo(a,h)anthracene	25.81	278	15370	0.96	ng	100
37) Benzo(g,h,i)perylene	26.47	276	16073	0.96	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM060315\
Data File : BM001543.D
Acq On : 03 Jun 2015 20:12
Operator : TP/IZ
Sample : SSTDICCC001
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
SSTDICCC001

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM

Quant Time: Jun 04 04:02:14 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 04 03:14:13 2015
Response via : Initial Calibration





#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.70 min Scan# 325

Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12

Instrument :

BNA_M

ClientSampleId :

SSTDICCC001

Tgt Ion: 152 Resp: 26032

Ion Ratio Lower Upper


152 100

150 168.7 135.0 202.4




115 72.3 57.8 86.8

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E



#2

1,4-Dioxane

Concen: 0.94 ng

RT: 3.21 min Scan# 35

Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12


Tgt Ion: 88 Resp: 2545

Ion Ratio Lower Upper



88 100




58 81.2 65.0 97.4

43 38.9 31.1 46.7



Abundance Ion 88.00 (87.70 to 88.70): BM0
Ion 58.00 (57.70 to 58.70): BM0
Ion 43.00 (42.70 to 43.70): BM0



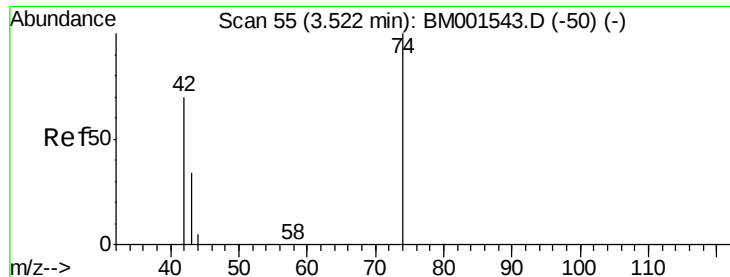





#3
n-Nitrosodimethylamine
Concen: 1.05 ng
RT: 3.52 min Scan# 55
Delta R.T. 0.00 min
Lab File: BM001543.D
Acq: 03 Jun 2015 20:12

Tgt Ion:	42	Resp:	3892
Ion	Ratio	Lower	Upper
42	100		
74	102.7	82.0	123.0
44	7.2	5.8	8.6

Instrument :
BNA_M
ClientSampleId :
SSTDICCC001


Manual Integrations
APPROVED


apatel
6/5/2015 8:04:11 AM



#4
2-Fluorophenol
Concen: 1.03 ng
RT: 5.28 min Scan# 169
Delta R.T. 0.00 min
Lab File: BM001543.D
Acq: 03 Jun 2015 20:12

Tgt Ion:	112	Resp:	5891
Ion	Ratio	Lower	Upper
112	100		
64	66.2	53.0	79.4
63	36.5	29.2	43.8





#5

Phenol-d6

Concen: 1.02 ng

RT: 6.86 min Scan# 271

Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12

Instrument :

BNA_M


ClientSampleId :

SSTDICCC001

Tgt Ion:	99	Resp:	7212
Ion Ratio	Lower	Upper	
99	100		
42	26.1	20.9	31.3
71	35.6	28.5	42.7

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM





Abundance Ion 99.00 (98.70 to 99.70): BM001543.D (-265) (-)

Ion 42.00 (41.70 to 42.70): BM001543.D (-265) (-)

Ion 71.00 (70.70 to 71.70): BM001543.D (-265) (-)

6.86

Time-->



#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.49 min Scan# 553

Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12

Tgt Ion:	136	Resp:	93290
Ion Ratio	Lower	Upper	
136	100		
137	11.4	9.1	13.7
54	5.7	4.6	6.8
68	4.0	3.2	4.8

Abundance Ion 136.00 (135.70 to 136.70): BM001543.D (-548) (-)



Ion 137.00 (136.70 to 137.70): BM001543.D (-548) (-)


Ion 54.00 (53.70 to 54.70): BM001543.D (-548) (-)

Ion 68.00 (67.70 to 68.70): BM001543.D (-548) (-)

10.49

Time-->





#7

Nitrobenzene-d5

Concen: 1.11 ng

RT: 8.86 min Scan# 422

Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12

Instrument :

BNA_M





ClientSampleId :

SSTDICCC001

Tgt Ion:	82	Resp:	6558
Ion	Ratio	Lower	Upper
82	100		
128	40.4	32.3	48.5
54	53.7	43.0	64.4

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM



#8

Nitrobenzene

Concen: 1.10 ng




RT: 8.90 min Scan# 426


Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12

Tgt Ion:	77	Resp:	6925
Ion	Ratio	Lower	Upper
77	100		
123	40.6	32.5	48.7
65	14.7	11.8	17.6





#9

Naphthalene

Concen: 0.99 ng

RT: 10.52 min Scan# 555

Delta R.T. 0.00 min

Lab File: BM001543.D


Acq: 03 Jun 2015 20:12

Instrument :

BNA_M

ClientSampleId :




SSTDICCC001



Tgt Ion:	128	Resp:	19421
Ion Ratio	Lower	Upper	
128	100		
129	10.6	8.5	12.7
127	14.6	11.7	17.5

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM



#10

Hexachlorobutadiene

Concen: 0.99 ng




RT: 10.82 min Scan# 572


Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12

Tgt Ion:	225	Resp:	3401
Ion Ratio	Lower	Upper	
225	100		
223	62.7	50.2	75.2
227	63.1	50.5	75.7



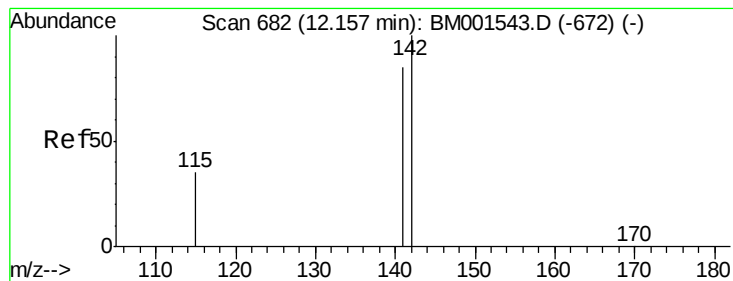

#11

2-Methylnaphthalene

Concen: 1.00 ng

RT: 12.16 min Scan# 682

Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12

Instrument :

BNA_M





ClientSampleId :

SSTDICCC001

Tgt Ion:	142	Resp:	12396
Ion Ratio	Lower	Upper	
142	100		
141	85.1	68.1	102.1
115	35.4	28.3	42.5

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM

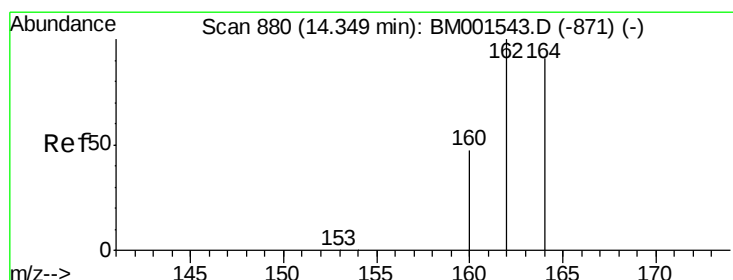

#12

Acenaphthene-d10

Concen: 5.00 ng




RT: 14.35 min Scan# 880


Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12


Tgt Ion:	164	Resp:	46533
Ion Ratio	Lower	Upper	
164	100		
162	110.0	88.0	132.0
160	51.2	41.0	61.4





#13
 2,4,6-Tribromophenol
 Concen: 1.92 ng
 RT: 15.83 min Scan# 943
 Delta R.T. 0.00 min
 Lab File: BM001543.D
 Acq: 03 Jun 2015 20:12




Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC001



Tgt Ion	Ratio	Resp	Lower	Upper
330	100	1916		
332	87.0	69.6	104.4	
141	0.0	0.0	0.0	




Manual Integrations
 APPROVED


apatel
 6/5/2015 8:04:11 AM



#14
 2-Fluorobiphenyl
 Concen: 0.97 ng
 RT: 12.97 min Scan# 760
 Delta R.T. 0.00 min
 Lab File: BM001543.D
 Acq: 03 Jun 2015 20:12

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	13569		
171	34.5	27.6	41.4	
170	23.0	18.4	27.6	





#15

Acenaphthylene

Concen: 1.01 ng

RT: 14.06 min Scan# 856

Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12

Instrument :

BNA_M




ClientSampleId :

SSTDICCC001

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.1	15.3	22.9
153	12.9	10.3	15.5

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM



#16

Acenaphthene

Concen: 0.97 ng





RT: 14.41 min Scan# 885


Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12

Tgt Ion	Ratio	Lower	Upper
154	100		
153	112.3	89.8	134.8
152	53.8	43.0	64.6









#17
Fluorene
 Concen: 0.50 ng
 RT: 15.39 min Scan# 930
 Delta R.T. 0.00 min
 Lab File: BM001543.D
 Acq: 03 Jun 2015 20:12

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC001

Tgt Ion	Ratio	Lower	Upper
166	100		
165	85.3	68.2	102.2
167	15.0	12.1	18.1




Manual Integrations
 APPROVED


apatel
 6/5/2015 8:04:11 AM



#18
Phenanthrene-d10
 Concen: 5.00 ng
 RT: 17.09 min Scan# 980
 Delta R.T. 0.00 min
 Lab File: BM001543.D
 Acq: 03 Jun 2015 20:12

Tgt Ion	Ratio	Lower	Upper
188	100		
94	1.2	1.0	1.4
80	1.0	0.8	1.2









#19
4-Bromophenyl-phenylether
Concen: 2.29 ng
RT: 16.27 min Scan# 956
Delta R.T. 0.00 min
Lab File: BM001543.D
Acq: 03 Jun 2015 20:12

Instrument :
BNA_M
ClientSampleId :
SSTDICCC001

Tgt Ion	Ratio	Lower	Upper
248	100		
250	69.0	55.2	82.8
141	80.9	64.7	97.1




Manual Integrations
APPROVED


apatel
6/5/2015 8:04:11 AM



#20
Hexachlorobenzene
Concen: 0.57 ng
RT: 16.41 min Scan# 960
Delta R.T. 0.00 min
Lab File: BM001543.D
Acq: 03 Jun 2015 20:12

Tgt Ion	Ratio	Lower	Upper
284	100		
142	0.0	0.0	0.0
249	0.0	0.0	0.0









#21
 Pentachlorophenol
 Concen: 0.69 ng
 RT: 16.75 min Scan# 970
 Delta R.T. 0.00 min
 Lab File: BM001543.D
 Acq: 03 Jun 2015 20:12

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC001

Tgt Ion	Ratio	Lower	Upper
266	100		
268	84.0	67.2	100.8
264	54.6	43.7	65.5




Manual Integrations
 APPROVED


apatel
 6/5/2015 8:04:11 AM



#22
 Phenanthrene
 Concen: 1.52 ng
 RT: 17.12 min Scan# 981
 Delta R.T. 0.00 min
 Lab File: BM001543.D
 Acq: 03 Jun 2015 20:12

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.4	14.7	22.1
179	15.9	12.7	19.1









#23
 Anthracene
 Concen: 0.64 ng m
 RT: 17.23 min Scan# 984
 Delta R.T. 0.00 min
 Lab File: BM001543.D
 Acq: 03 Jun 2015 20:12

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC001

Tgt Ion	Ratio	Lower	Upper
178	100		
176	0.0	36.6	54.8#
179	14.7	28.7	43.1#




Manual Integrations
 APPROVED


apatel
 6/5/2015 8:04:11 AM



#24
 Fluoranthene
 Concen: 1.13 ng
 RT: 19.15 min Scan# 1089
 Delta R.T. 0.00 min
 Lab File: BM001543.D
 Acq: 03 Jun 2015 20:12

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.7	10.2	15.2
203	17.3	13.8	20.8









#25
Chrysene-d12
Concen: 5.00 ng
RT: 21.28 min Scan# 1252
Delta R.T. 0.00 min
Lab File: BM001543.D
Acq: 03 Jun 2015 20:12

Instrument :
BNA_M
ClientSampleId :
SSTDICCC001

Tgt Ion	Ratio	Lower	Upper
240	100		
120	7.0	5.6	8.4
236	28.0	22.4	33.6




Manual Integrations
APPROVED


apatel
6/5/2015 8:04:11 AM



#26
Pyrene
Concen: 1.03 ng
RT: 19.52 min Scan# 1119
Delta R.T. 0.00 min
Lab File: BM001543.D
Acq: 03 Jun 2015 20:12

Tgt Ion	Ratio	Lower	Upper
202	100		
200	20.8	16.6	25.0
203	17.3	13.8	20.8



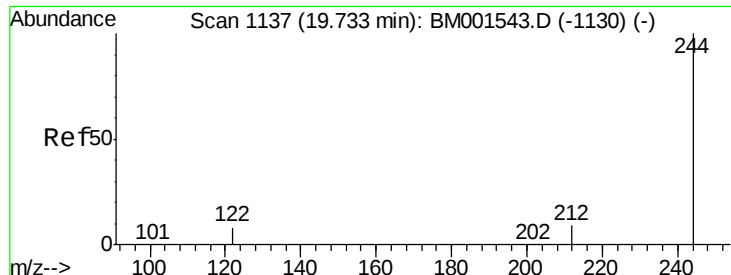

#27

Terphenyl-d14

Concen: 1.03 ng

RT: 19.73 min Scan# 1137

Delta R.T. 0.00 min

Lab File: BM001543.D


Acq: 03 Jun 2015 20:12

Instrument :

BNA_M

ClientSampleId :




SSTDICCC001



Tgt Ion:	244	Resp:	9242
Ion Ratio	Lower	Upper	
244	100		
212	10.0	8.0	12.0
122	9.1	7.3	10.9

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM



#28

Benzo(a)anthracene

Concen: 1.00 ng




RT: 21.27 min Scan# 1251


Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12

Tgt Ion:	228	Resp:	19668
Ion Ratio	Lower	Upper	
228	100		
226	23.7	19.0	28.4
229	21.1	16.9	25.3





#29

Chrysene

Concen: 0.98 ng

RT: 21.31 min Scan# 1254

Delta R.T. 0.00 min

Lab File: BM001543.D


Acq: 03 Jun 2015 20:12

Instrument :

BNA_M

ClientSampleId :




SSTDICCC001



Tgt Ion:	228	Resp:	18310
Ion Ratio	Lower	Upper	
228	100		
226	31.5	25.2	37.8
229	18.4	14.7	22.1

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM



#30

Bis(2-ethylhexyl)phthalate

Concen: 1.00 ng




RT: 21.21 min Scan# 1247


Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12

Tgt Ion:	149	Resp:	14162
Ion Ratio	Lower	Upper	
149	100		
167	25.6	20.5	30.7
279	2.1	1.7	2.5



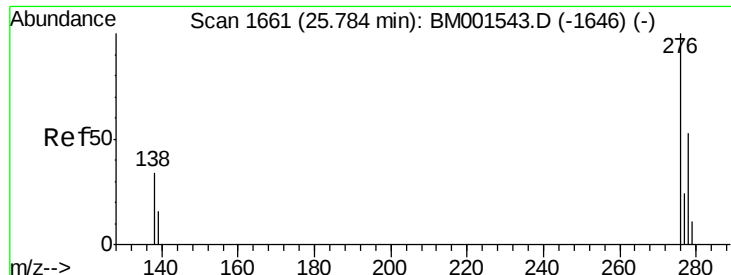

#31

Indeno(1,2,3-cd)pyrene

Concen: 0.95 ng

RT: 25.78 min Scan# 1661

Delta R.T. 0.00 min

Lab File: BM001543.D


Acq: 03 Jun 2015 20:12

Instrument :

BNA_M

ClientSampleId :

SSTDICCC001



Tgt Ion: 276 Resp: 19581

Ion Ratio Lower Upper




276 100

138 35.5 28.3 42.5

277 24.7 19.6 29.4

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM



#32

Perylene-d12

Concen: 5.00 ng

RT: 23.52 min Scan# 1444

Delta R.T. 0.00 min

Lab File: BM001543.D

Acq: 03 Jun 2015 20:12




Tgt Ion: 264 Resp: 66329


Ion Ratio Lower Upper

264 100

260 26.4 21.1 31.7

265 21.4 17.1 25.7





#33

Benzo(b)fluoranthene

Concen: 0.97 ng

RT: 22.84 min Scan# 1379

Delta R.T. 0.00 min

Lab File: BM001543.D


Acq: 03 Jun 2015 20:12

Instrument :

BNA_M

ClientSampleId :



SSTDICCC001



Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.2	17.8	26.6
125	15.6	12.5	18.7

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM



#34

Benzo(k)fluoranthene


Concen: 1.04 ng

RT: 22.89 min Scan# 1383



Delta R.T. 0.00 min


Lab File: BM001543.D

Acq: 03 Jun 2015 20:12



Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.5	17.2	25.8
125	15.6	12.5	18.7






#35
Benzo(a)pyrene
Concen: 1.02 ng
RT: 23.42 min Scan# 1434
Delta R.T. 0.00 min
Lab File: BM001543.D
Acq: 03 Jun 2015 20:12

Instrument :
BNA_M
ClientSampleId :
SSTDICCC001




Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.0	17.6	26.4
125	17.9	14.3	21.5

Manual Integrations
APPROVED

apatel
6/5/2015 8:04:11 AM






Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E




#36
Dibenzo(a,h)anthracene
Concen: 0.96 ng
RT: 25.81 min Scan# 1663
Delta R.T. 0.00 min
Lab File: BM001543.D
Acq: 03 Jun 2015 20:12

Tgt Ion	Ratio	Lower	Upper
278	100		
139	22.5	18.0	27.0
279	24.8	19.8	29.8


Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E



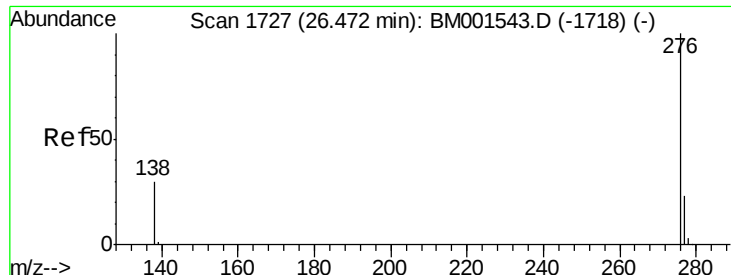

#37
 Benzo(g,h,i)perylene
 Concen: 0.96 ng
 RT: 26.47 min Scan# 1727
 Delta R.T. 0.00 min
 Lab File: BM001543.D
 Acq: 03 Jun 2015 20:12

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICCC001



Tgt	Ion	276	Resp:	16073
Ion	Ratio	Lower	Upper	
276	100			
277	24.1	19.3	28.9	
138	31.3	25.0	37.6	

Manual Integrations
 APPROVED

apatel
 6/5/2015 8:04:11 AM

