


Data Path : Z:\HPCHEM1\BNA_M\Data\BM060315\
 Data File : BM001539.D
 Acq On : 03 Jun 2015 17:48
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 04 19:28:43 2015

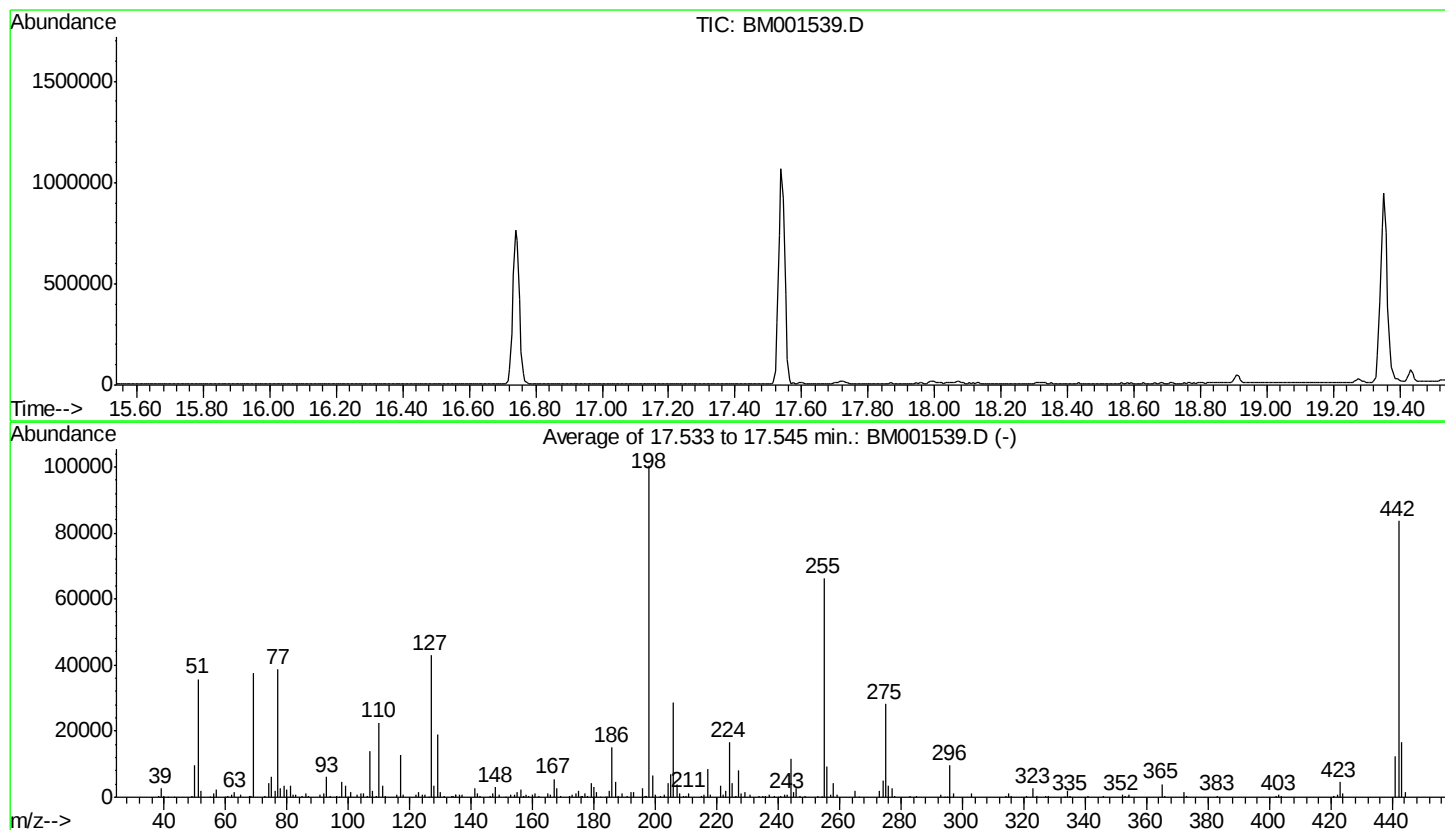

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	35712	PASS
68	69	0.00	2	1.5	571	PASS
69	198	0.00	100	37.4	37488	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.8	42954	PASS
197	198	0.00	2	0.6	556	PASS
198	198	100	100	100.0	100354	PASS
199	198	5	9	6.7	6707	PASS
275	198	10	60	28.2	28250	PASS
365	198	1	100	4.1	4069	PASS
441	442	0.01	24	14.8	12393	PASS
442	198	50	100	83.4	83664	PASS
443	442	15	24	20.0	16765	PASS