
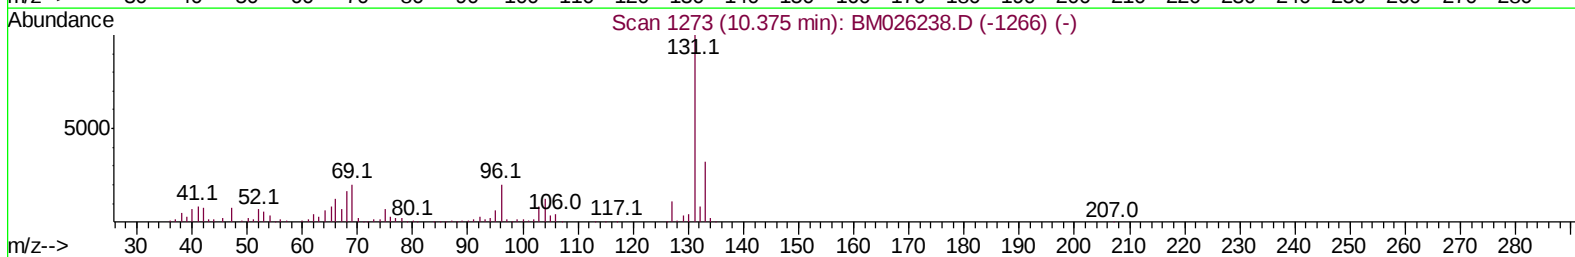
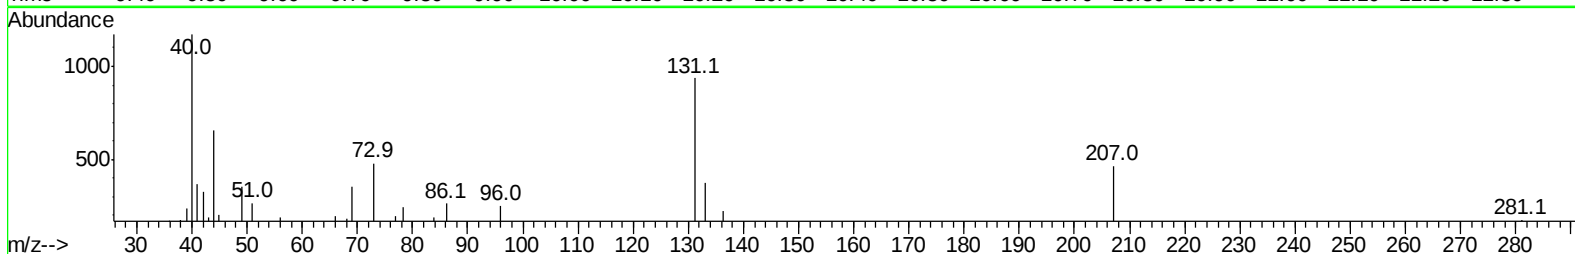


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060320\
Data File : BM026245.D
Acq On : 03 Jun 2020 14:11
Operator : JU/CG
Sample : L2836-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Jun 03 14:47:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 03 12:10:52 2020
Response via : Initial Calibration

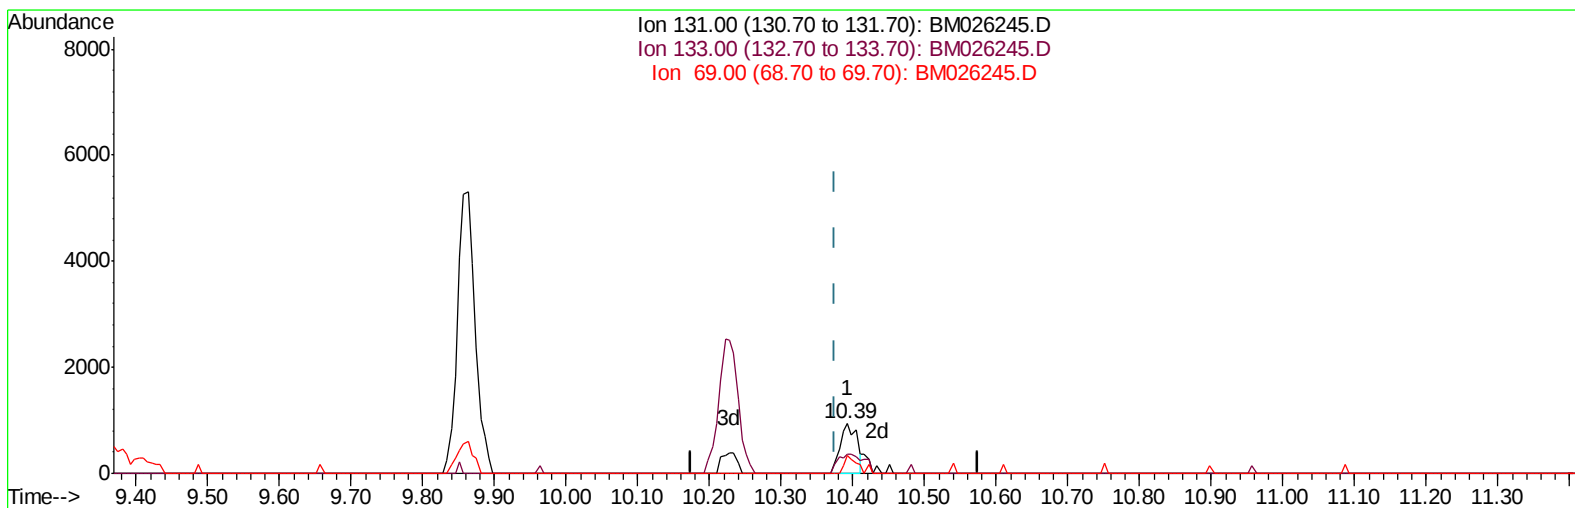




TIC: BM026245.D

(29) 4-Chloroaniline-d4 (S)
10.392min (+0.018) 0.16ng/ul
response 1505

Ion	Exp%	Act%
131.00	100	100
133.00	34.00	40.00
69.00	21.90	37.33#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060320\
Data File : BM026245.D
Acq On : 03 Jun 2020 14:11
Operator : JU/CG
Sample : L2836-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Jun 03 14:47:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 03 12:10:52 2020
Response via : Initial Calibration

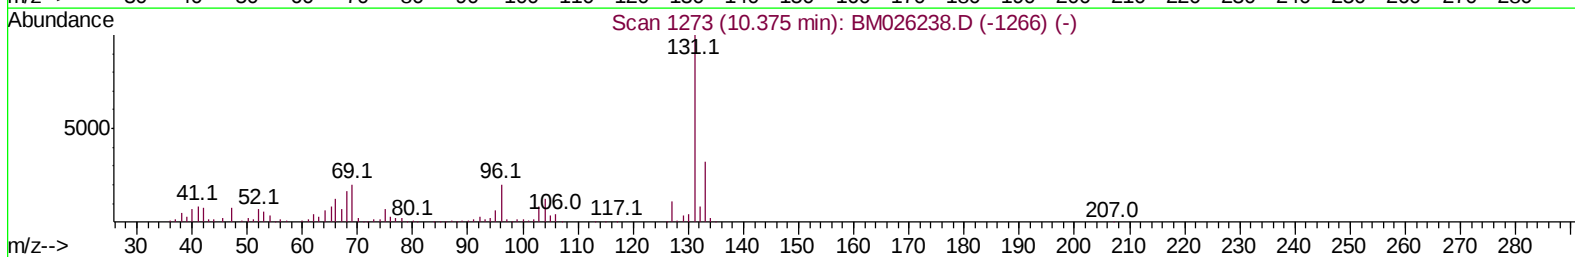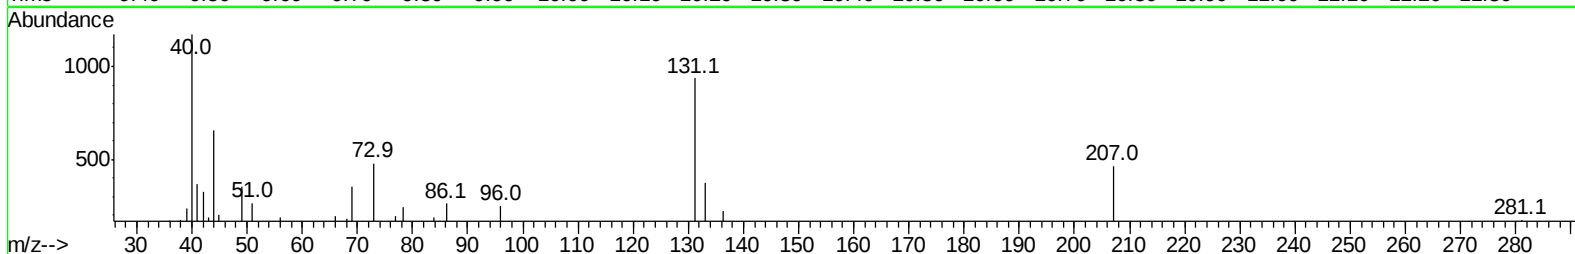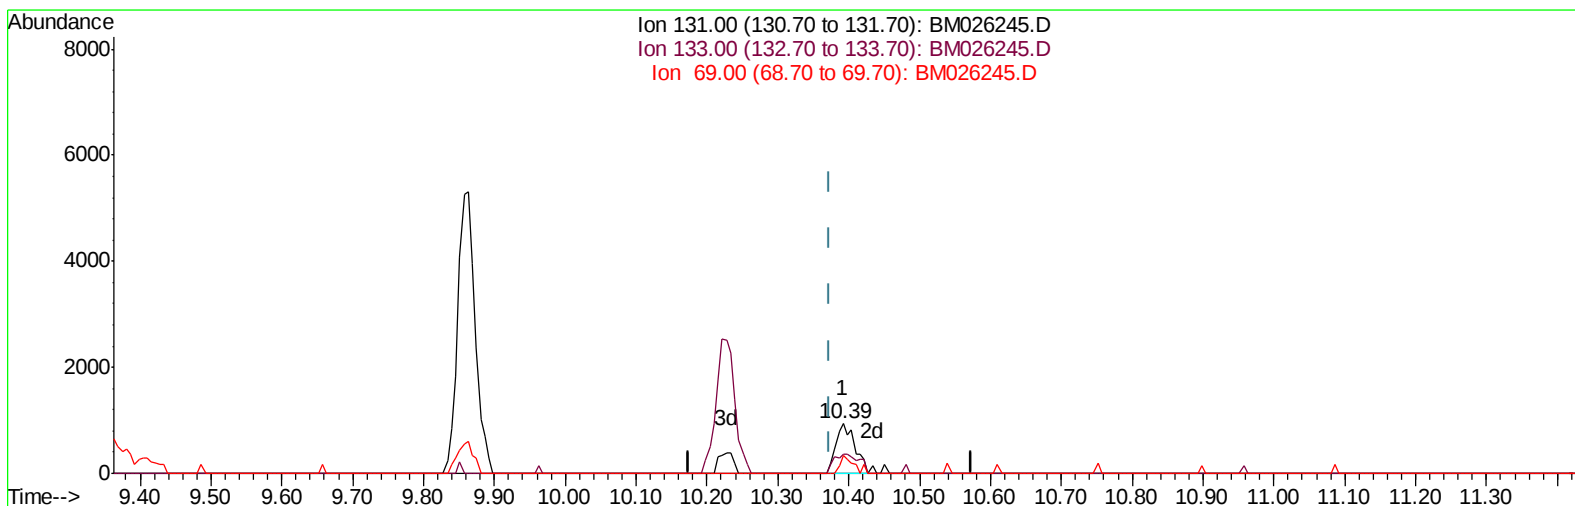

TIC: BM026245.D

(29) 4-Chloroaniline-d4 (S)

10.392min (+0.018) 0.19ng/ul m

response 1731

Ion	Exp%	Act%
131.00	100	100
133.00	34.00	40.00
69.00	21.90	37.33#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060320\
 Data File : BM026245.D
 Acq On : 03 Jun 2020 14:11
 Operator : JU/CG
 Sample : L2836-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Jun 03 14:49:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 03 12:10:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	139342	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	560630	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	323715	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	693898	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	725580	20.00	ng/ul	0.00
86) Perylene-d12	23.18	264	785201	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	21776	4.71	ng/uL	0.00
5) Phenol-d5	6.66	99	90793	7.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	261586	29.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	239232	24.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.18	113	155631	16.34	ng/ul	0.00
19) Nitrobenzene-d5	8.61	128	138580	30.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	149416	33.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	246305	27.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	1731m	0.19	ng/ul	0.02
44) Dimethylphthalate-d6	13.54	166	823145	31.71	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	945493	30.74	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	25802	5.61	ng/ul	0.00
58) Fluorene-d10	15.12	176	716716	31.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.24	200	111221	27.49	ng/ul	0.00
71) Anthracene-d10	16.96	188	1113474	32.56	ng/ul	0.00
79) Pyrene-d10	19.26	212	1260503	33.82	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.05	264	1322292	31.64	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM060320\
Data File : BM026245.D
Acq On : 03 Jun 2020 14:11
Operator : JU/CG
Sample : L2836-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Jun 03 14:49:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 03 12:10:52 2020
Response via : Initial Calibration

