

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060320\
 Data File : BM026246.D
 Acq On : 03 Jun 2020 14:48
 Operator : JU/CG
 Sample : L2836-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFXC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	25	29	37	rVB	44552	65401	1.88%	0.192%
2	3.263	62	64	68	rVB5	3891	4036	0.12%	0.012%
3	3.463	95	98	102	rVB3	7103	7631	0.22%	0.022%
4	3.669	128	133	138	rBV3	10875	17198	0.49%	0.050%
5	3.752	143	147	153	rVB2	8075	12953	0.37%	0.038%
6	4.199	218	223	227	rBV5	3079	6299	0.18%	0.018%
7	5.528	444	449	455	rVB5	3128	6741	0.19%	0.020%
8	6.663	636	642	651	rVV	186087	281277	8.07%	0.825%
9	6.816	662	668	679	rBV	550433	841159	24.13%	2.469%
10	7.004	693	700	709	rBV	603603	937814	26.90%	2.752%
11	7.463	772	778	788	rVB	613321	937738	26.90%	2.752%
12	8.181	894	900	910	rBV	468325	707403	20.29%	2.076%
13	8.610	966	973	983	rBV	678022	1075757	30.85%	3.157%
14	9.322	1087	1094	1110	rBV	540744	879523	25.23%	2.581%
15	9.857	1179	1185	1199	rBV	690985	1198486	34.37%	3.517%
16	10.222	1239	1247	1258	rBV	771326	1283633	36.82%	3.767%
17	10.404	1270	1278	1285	rVB9	3470	7863	0.23%	0.023%
18	11.075	1387	1392	1394	rBV4	2439	3507	0.10%	0.010%
19	11.828	1515	1520	1528	rVB3	11101	19155	0.55%	0.056%
20	13.416	1787	1790	1794	rBV5	3599	4247	0.12%	0.012%
21	13.533	1804	1810	1822	rBV	1314014	1816750	52.11%	5.332%
22	13.798	1847	1855	1866	rBV	1438162	2041503	58.55%	5.991%
23	13.974	1881	1885	1887	rBV5	4544	5677	0.16%	0.017%
24	14.110	1902	1908	1917	rBV	1099157	1581283	45.35%	4.641%
25	14.345	1942	1948	1966	rBV	96378	214440	6.15%	0.629%
26	14.574	1982	1987	1989	rBV5	4224	4741	0.14%	0.014%
27	15.110	2072	2078	2091	rBV	1888136	2679257	76.84%	7.863%
28	15.245	2096	2101	2114	rVV	638260	900626	25.83%	2.643%
29	15.357	2114	2120	2125	rVB	23270	37782	1.08%	0.111%
30	15.868	2203	2207	2210	rBV3	8433	11347	0.33%	0.033%
31	15.898	2210	2212	2217	rVB5	7870	8954	0.26%	0.026%
32	16.663	2336	2342	2347	rVV5	13861	21426	0.61%	0.063%
33	16.727	2347	2353	2362	rVB8	4591	10104	0.29%	0.030%
34	16.863	2370	2376	2386	rBV	1341486	1842302	52.84%	5.407%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060320\
 Data File : BM026246.D
 Acq On : 03 Jun 2020 14:48
 Operator : JU/CG
 Sample : L2836-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFXC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	16.963	2386	2393	2405	rVV	2086248	2954243	84.73%	8.670%
36	17.404	2463	2468	2473	rVB2	12002	16624	0.48%	0.049%
37	17.574	2491	2497	2500	rVB5	6730	8534	0.24%	0.025%
38	17.798	2530	2535	2539	rBV8	5771	9826	0.28%	0.029%
39	17.898	2550	2552	2557	rBV5	3274	4354	0.12%	0.013%
40	18.092	2582	2585	2590	rVB3	10763	11926	0.34%	0.035%
41	18.733	2691	2694	2701	rVB8	8388	15569	0.45%	0.046%
42	18.898	2718	2722	2727	rBV	25379	36970	1.06%	0.108%
43	19.151	2761	2765	2770	rBV2	23249	33096	0.95%	0.097%
44	19.262	2778	2784	2791	rBV	2656385	3486611	100.00%	10.232%
45	21.068	3086	3091	3099	rBV	1723709	2192093	62.87%	6.433%
46	22.586	3347	3349	3353	rVB	112832	127945	3.67%	0.375%
47	23.050	3422	3428	3435	rBV	2129385	3447760	98.89%	10.118%
48	23.180	3444	3450	3460	rVB	1291929	2255024	64.68%	6.618%


Sum of corrected areas: 34074588

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060320\
Data File : BM026246.D
Acq On : 03 Jun 2020 14:48
Operator : JU/CG
Sample : L2836-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFXC7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

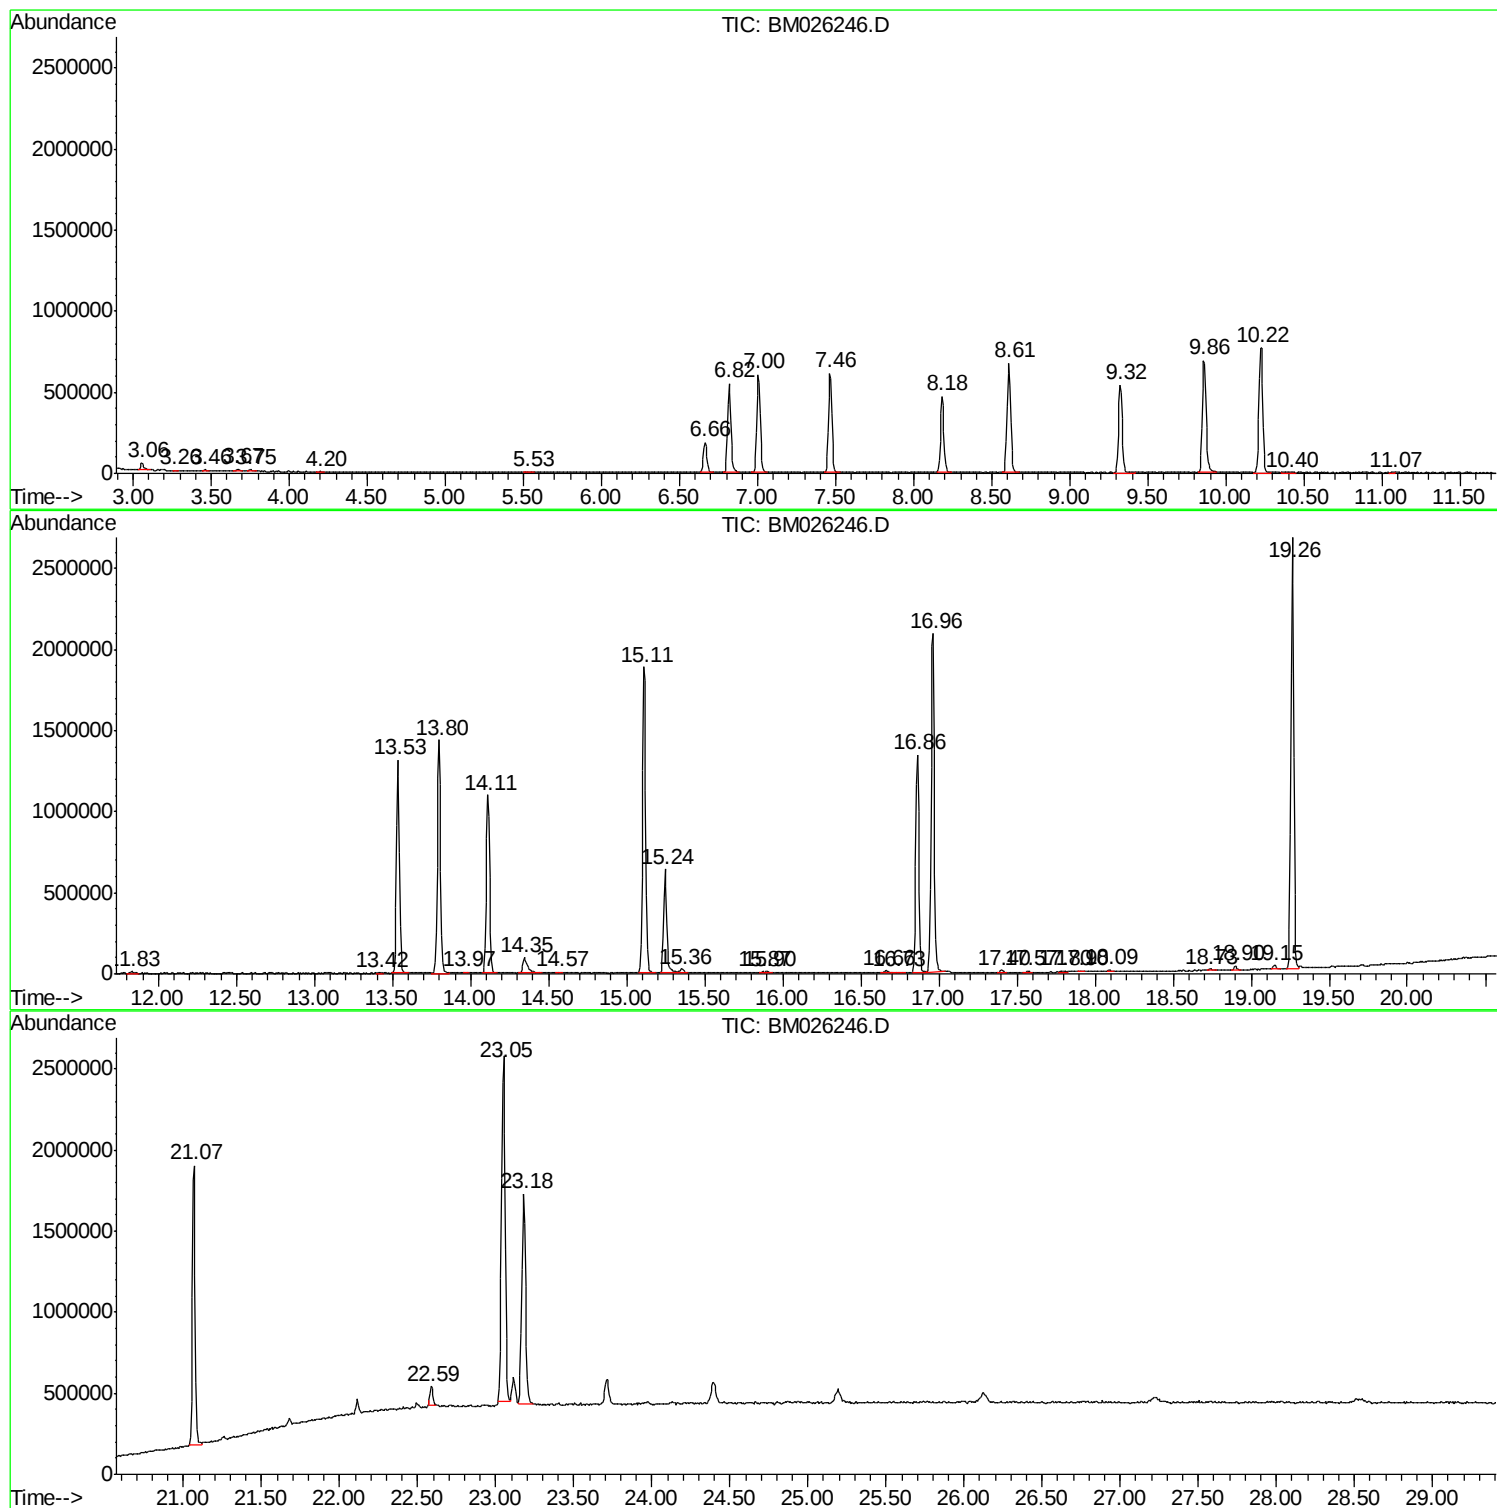

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060320\
Data File : BM026246.D
Acq On : 03 Jun 2020 14:48
Operator : JU/CG
Sample : L2836-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFXC7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM060320\
Data File : BM026246.D
Acq On : 03 Jun 2020 14:48
Operator : JU/CG
Sample : L2836-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFXC7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc