

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060324\
 Data File : BM045798.D
 Acq On : 03 Jun 2024 09:36
 Operator : MA/JU
 Sample : PB160893BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK893

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.057	8	12	22	rVB	73596	118368	2.81%	0.212%
2	3.469	79	82	103	rBV	553397	1343697	31.90%	2.404%
3	3.751	126	130	134	rVB	20744	28385	0.67%	0.051%
4	4.175	198	202	206	rVB	31265	43117	1.02%	0.077%
5	6.622	612	618	623	rBV8	4143	9971	0.24%	0.018%
6	6.722	629	635	648	rVB	1228981	1983670	47.10%	3.549%
7	6.834	648	654	669	rBV	918380	1532252	36.38%	2.741%
8	7.034	681	688	700	rVB	1239266	1959850	46.53%	3.507%
9	7.469	755	762	769	rBV	1075576	1604357	38.09%	2.871%
10	8.039	854	859	863	rBV7	2723	5024	0.12%	0.009%
11	8.239	886	893	910	rVV	1379185	2250076	53.42%	4.026%
12	8.633	953	960	977	rVB	1270638	1988995	47.22%	3.559%
13	9.251	1062	1065	1068	rBV5	4030	5896	0.14%	0.011%
14	9.345	1074	1081	1091	rBV	963671	1559510	37.03%	2.790%
15	9.892	1167	1174	1188	rBV	1279532	2197796	52.18%	3.932%
16	10.175	1219	1222	1225	rBV4	2919	4882	0.12%	0.009%
17	10.239	1225	1233	1243	rVV	1368164	2174805	51.64%	3.891%
18	10.422	1257	1264	1282	rBV	1063965	2258121	53.61%	4.040%
19	11.251	1400	1405	1407	rVB5	2701	4309	0.10%	0.008%
20	11.845	1500	1506	1511	rBV2	21978	35540	0.84%	0.064%
21	12.557	1624	1627	1628	rVB3	4707	4633	0.11%	0.008%
22	13.086	1712	1717	1719	rBV5	4516	5463	0.13%	0.010%
23	13.563	1792	1798	1811	rBV	2189877	3056444	72.57%	5.469%
24	13.804	1830	1839	1851	rBV	2460839	3495415	82.99%	6.254%
25	14.110	1883	1891	1899	rBV	1804025	2590911	61.52%	4.636%
26	14.404	1935	1941	1961	rBV	818960	1385703	32.90%	2.479%
27	15.109	2054	2061	2075	rBV	3077836	4121083	97.85%	7.373%
28	15.245	2078	2084	2092	rBV	845897	1134092	26.93%	2.029%
29	15.351	2098	2102	2108	rVB2	15016	22360	0.53%	0.040%
30	15.680	2155	2158	2161	rBV5	3069	5213	0.12%	0.009%
31	16.545	2302	2305	2309	rVB6	4807	5541	0.13%	0.010%
32	16.645	2318	2322	2326	rBV5	5407	9841	0.23%	0.018%
33	16.856	2352	2358	2367	rBV	1993174	2720610	64.59%	4.868%
34	16.956	2367	2375	2386	rBV	2909671	3954873	93.90%	7.076%
35	17.251	2422	2425	2428	rBV5	3754	4908	0.12%	0.009%
36	18.821	2688	2692	2696	rVB3	32294	41257	0.98%	0.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060324\
Data File : BM045798.D
Acq On : 03 Jun 2024 09:36
Operator : MA/JU
Sample : PB160893BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK893

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Title : SVOA CALIBRATION

37	18.892	2700	2704	2710	rVB	30295	40929	0.97%	0.073%
38	18.974	2716	2718	2725	rVB8	7374	9200	0.22%	0.016%
39	19.215	2756	2759	2760	rBV3	19720	20268	0.48%	0.036%
40	19.250	2760	2765	2774	rVB	3299578	4211807	100.00%	7.536%
41	20.262	2934	2937	2940	rBV5	19960	23306	0.55%	0.042%
42	21.068	3069	3074	3083	rBV	1742206	2252508	53.48%	4.030%
43	22.356	3290	3293	3299	rVB2	59969	88412	2.10%	0.158%
44	23.603	3498	3505	3515	rBV2	1520948	3143136	74.63%	5.624%
45	23.791	3529	3537	3547	rVB	1105689	2434553	57.80%	4.356%




Sum of corrected areas: 55891087

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060324\
Data File : BM045798.D
Acq On : 03 Jun 2024 09:36
Operator : MA/JU
Sample : PB160893BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK893

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

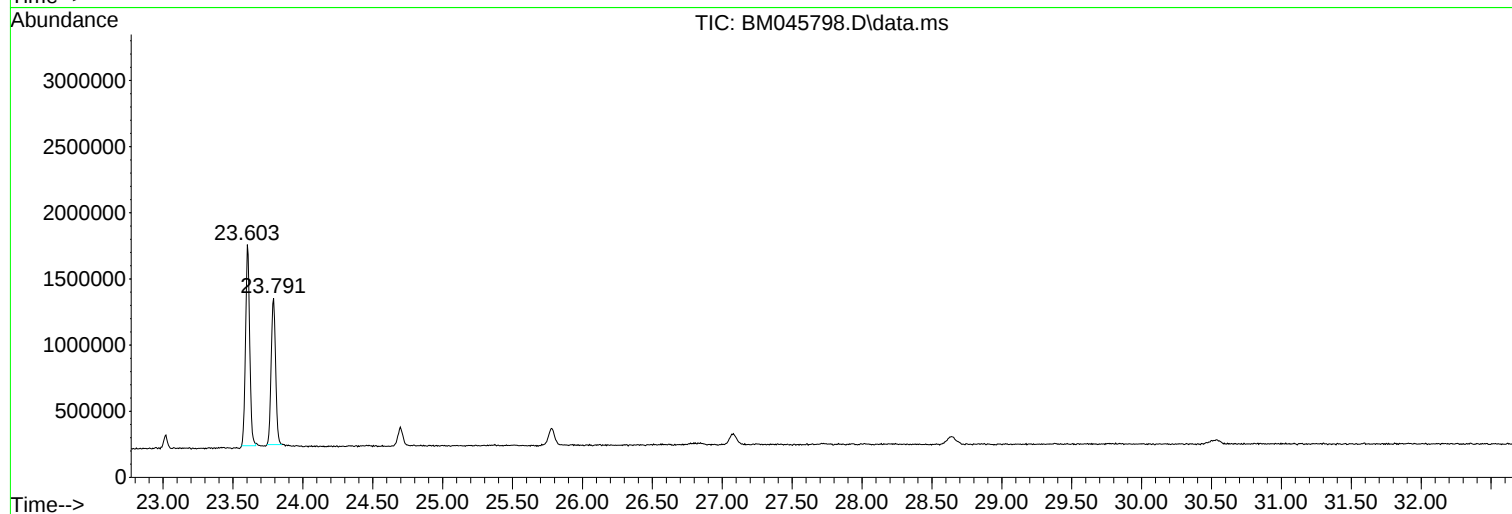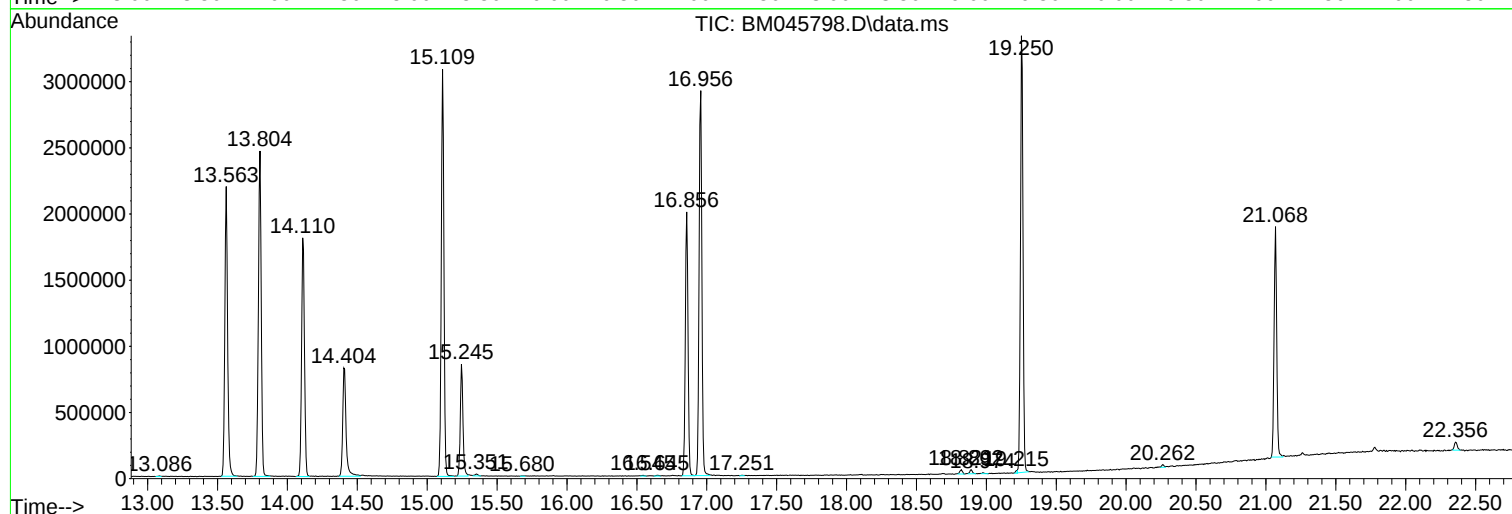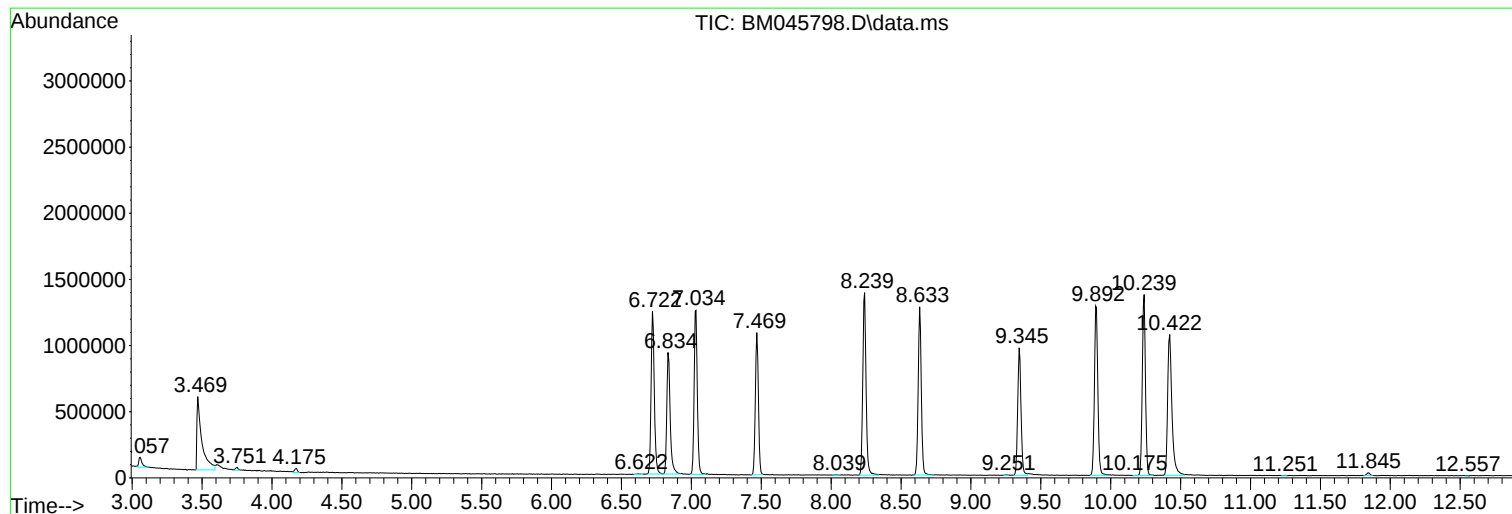

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060324\
Data File : BM045798.D
Acq On : 03 Jun 2024 09:36
Operator : MA/JU
Sample : PB160893BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK893

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060324\
Data File : BM045798.D
Acq On : 03 Jun 2024 09:36
Operator : MA/JU
Sample : PB160893BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK893

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc