

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060324\
 Data File : BM045808.D
 Acq On : 03 Jun 2024 17:08
 Operator : MA/JU
 Sample : PB161265BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	8	12	22	rVB	86159	137077	2.65%	0.212%
2	3.470	79	82	103	rBV	622866	1528440	29.58%	2.367%
3	3.746	125	129	135	rVB	85944	120609	2.33%	0.187%
4	4.175	198	202	207	rVB	31498	46226	0.89%	0.072%
5	6.593	609	613	615	rBV4	3737	5575	0.11%	0.009%
6	6.622	615	618	624	rVV5	7461	13027	0.25%	0.020%
7	6.722	629	635	648	rVV	1327415	2175820	42.11%	3.369%
8	6.834	648	654	670	rVV	989112	1692719	32.76%	2.621%
9	7.028	681	687	700	rVB	1355929	2141330	41.44%	3.316%
10	7.469	755	762	771	rVB	1157682	1797390	34.78%	2.783%
11	8.234	886	892	904	rBV	1497292	2491455	48.21%	3.858%
12	8.634	952	960	975	rVV	1381793	2230420	43.16%	3.454%
13	9.252	1060	1065	1068	rBV6	6309	10582	0.20%	0.016%
14	9.346	1073	1081	1094	rBV	1096213	1768028	34.21%	2.738%
15	9.457	1098	1100	1105	rVB5	4782	5248	0.10%	0.008%
16	9.893	1165	1174	1188	rBV	1474557	2484474	48.08%	3.847%
17	10.234	1224	1232	1245	rBV	1488806	2493041	48.24%	3.861%
18	10.416	1256	1263	1281	rBV	1210915	2609919	50.51%	4.041%
19	11.187	1391	1394	1397	rBV5	3293	5185	0.10%	0.008%
20	11.728	1482	1486	1489	rBV6	4237	6182	0.12%	0.010%
21	11.775	1493	1494	1500	rVV5	4980	7122	0.14%	0.011%
22	11.845	1500	1506	1514	rVB	27871	50801	0.98%	0.079%
23	13.563	1790	1798	1811	rBV	2521389	3667007	70.96%	5.678%
24	13.804	1832	1839	1850	rBV	2904243	4122020	79.77%	6.383%
25	14.004	1866	1873	1876	rVB9	2254	5203	0.10%	0.008%
26	14.110	1885	1891	1900	rBV	2210669	3196429	61.86%	4.950%
27	14.404	1934	1941	1959	rBV	1051691	1647110	31.87%	2.551%
28	14.816	2008	2011	2014	rBV5	3431	5506	0.11%	0.009%
29	15.110	2054	2061	2074	rBV	3550919	4941889	95.63%	7.653%
30	15.245	2078	2084	2092	rBV	588001	826400	15.99%	1.280%
31	15.351	2098	2102	2107	rVB2	16755	20918	0.40%	0.032%
32	16.539	2301	2304	2310	rBV8	6434	8191	0.16%	0.013%
33	16.645	2320	2322	2327	rVB4	7672	10758	0.21%	0.017%
34	16.857	2352	2358	2368	rBV	2687461	3533453	68.38%	5.472%
35	16.957	2368	2375	2388	rVV	3759190	5016601	97.08%	7.768%
36	17.269	2423	2428	2430	rBV5	5336	8456	0.16%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060324\
Data File : BM045808.D
Acq On : 03 Jun 2024 17:08
Operator : MA/JU
Sample : PB161265BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Title : SVOA CALIBRATION

37	17.439	2453	2457	2459	rBV5	4599	6658	0.13%	0.010%
38	17.616	2485	2487	2491	rVB5	5304	5764	0.11%	0.009%
39	17.845	2525	2526	2531	rVB5	4200	5362	0.10%	0.008%
40	18.822	2687	2692	2696	rBV3	42999	57014	1.10%	0.088%
41	18.892	2700	2704	2708	rVV	35325	48122	0.93%	0.075%
42	19.251	2760	2765	2778	rVB	3826657	5167461	100.00%	8.002%
43	21.068	3068	3074	3085	rBV	2116952	2823530	54.64%	4.372%
44	23.604	3498	3505	3520	rVB2	1495856	3209674	62.11%	4.970%
45	23.786	3529	3536	3548	rVB	1098779	2423788	46.90%	3.753%




Sum of corrected areas: 64577984

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060324\
Data File : BM045808.D
Acq On : 03 Jun 2024 17:08
Operator : MA/JU
Sample : PB161265BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK265

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

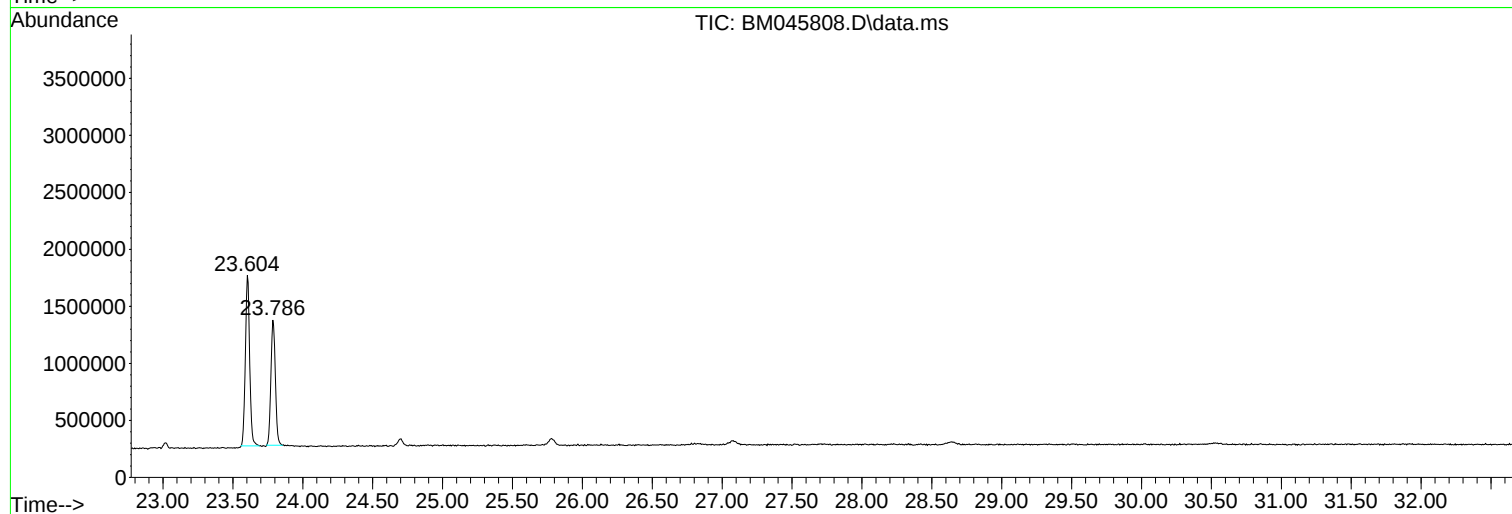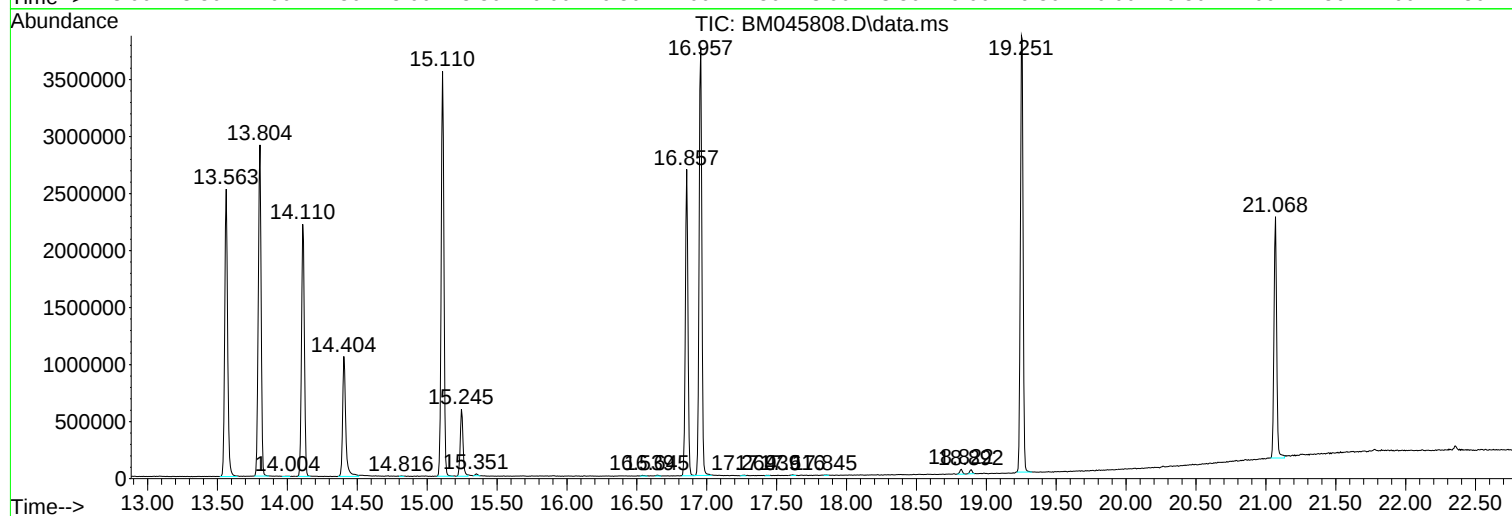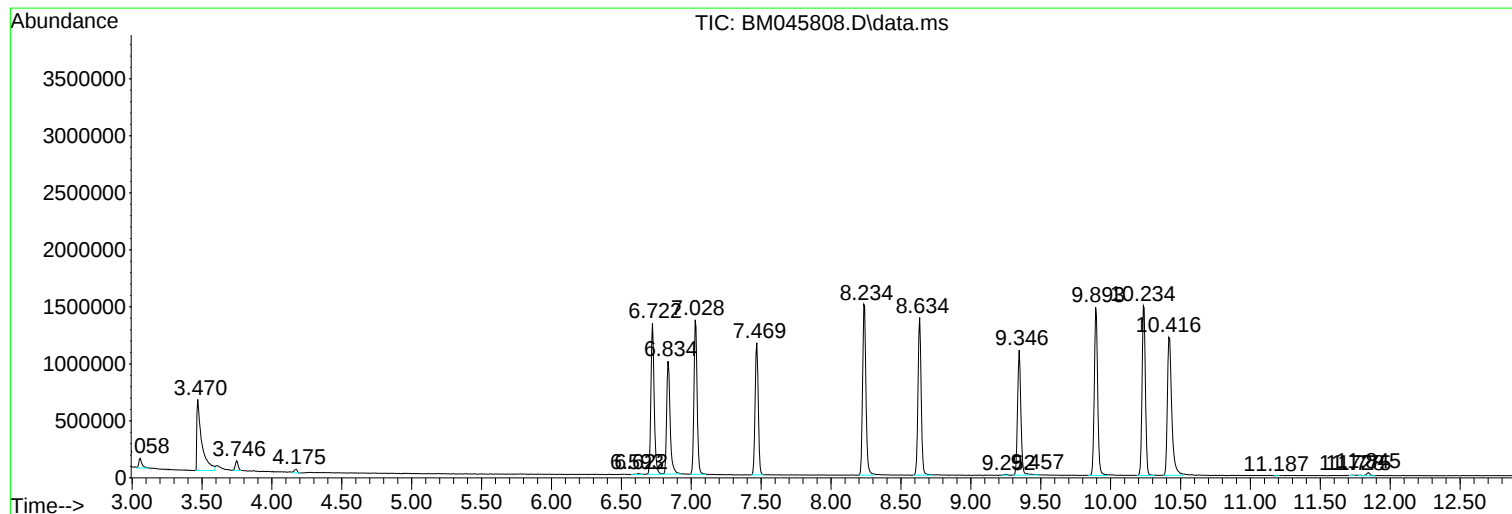

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060324\
Data File : BM045808.D
Acq On : 03 Jun 2024 17:08
Operator : MA/JU
Sample : PB161265BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK265

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060324\
Data File : BM045808.D
Acq On : 03 Jun 2024 17:08
Operator : MA/JU
Sample : PB161265BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK265

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM053124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc