

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060420\
 Data File : BM026252.D
 Acq On : 04 Jun 2020 11:13
 Operator : JU/CG
 Sample : L2844-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF3

Quant Time: Jun 04 11:46:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 04 10:01:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	113060	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	432269	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	246704	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	522333	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	595350	20.00	ng/ul	0.00
86) Perylene-d12	23.17	264	661542	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	19985	5.33	ng/uL	0.00
5) Phenol-d5	6.66	99	72524	7.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	205677	28.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	191953	23.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.18	113	134517	17.40	ng/ul	0.00
19) Nitrobenzene-d5	8.61	128	112411	31.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	119902	34.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	219853	31.41	ng/ul	0.00
29) 4-Chloroaniline-d4	10.38	131	15424	2.17	ng/ul	0.01
44) Dimethylphthalate-d6	13.53	166	724700	36.63	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	845398	36.07	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	19851	5.67	ng/ul	0.00
58) Fluorene-d10	15.11	176	614506	35.71	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.24	200	97053	31.87	ng/ul	0.00
71) Anthracene-d10	16.96	188	983882	38.22	ng/ul	0.00
79) Pyrene-d10	19.26	212	1153445	37.72	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	1059823	30.10	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.58	163	79698	3.837	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060420\
Data File : BM026252.D
Acq On : 04 Jun 2020 11:13
Operator : JU/CG
Sample : L2844-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF3

Quant Time: Jun 04 11:46:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 04 10:01:49 2020
Response via : Initial Calibration

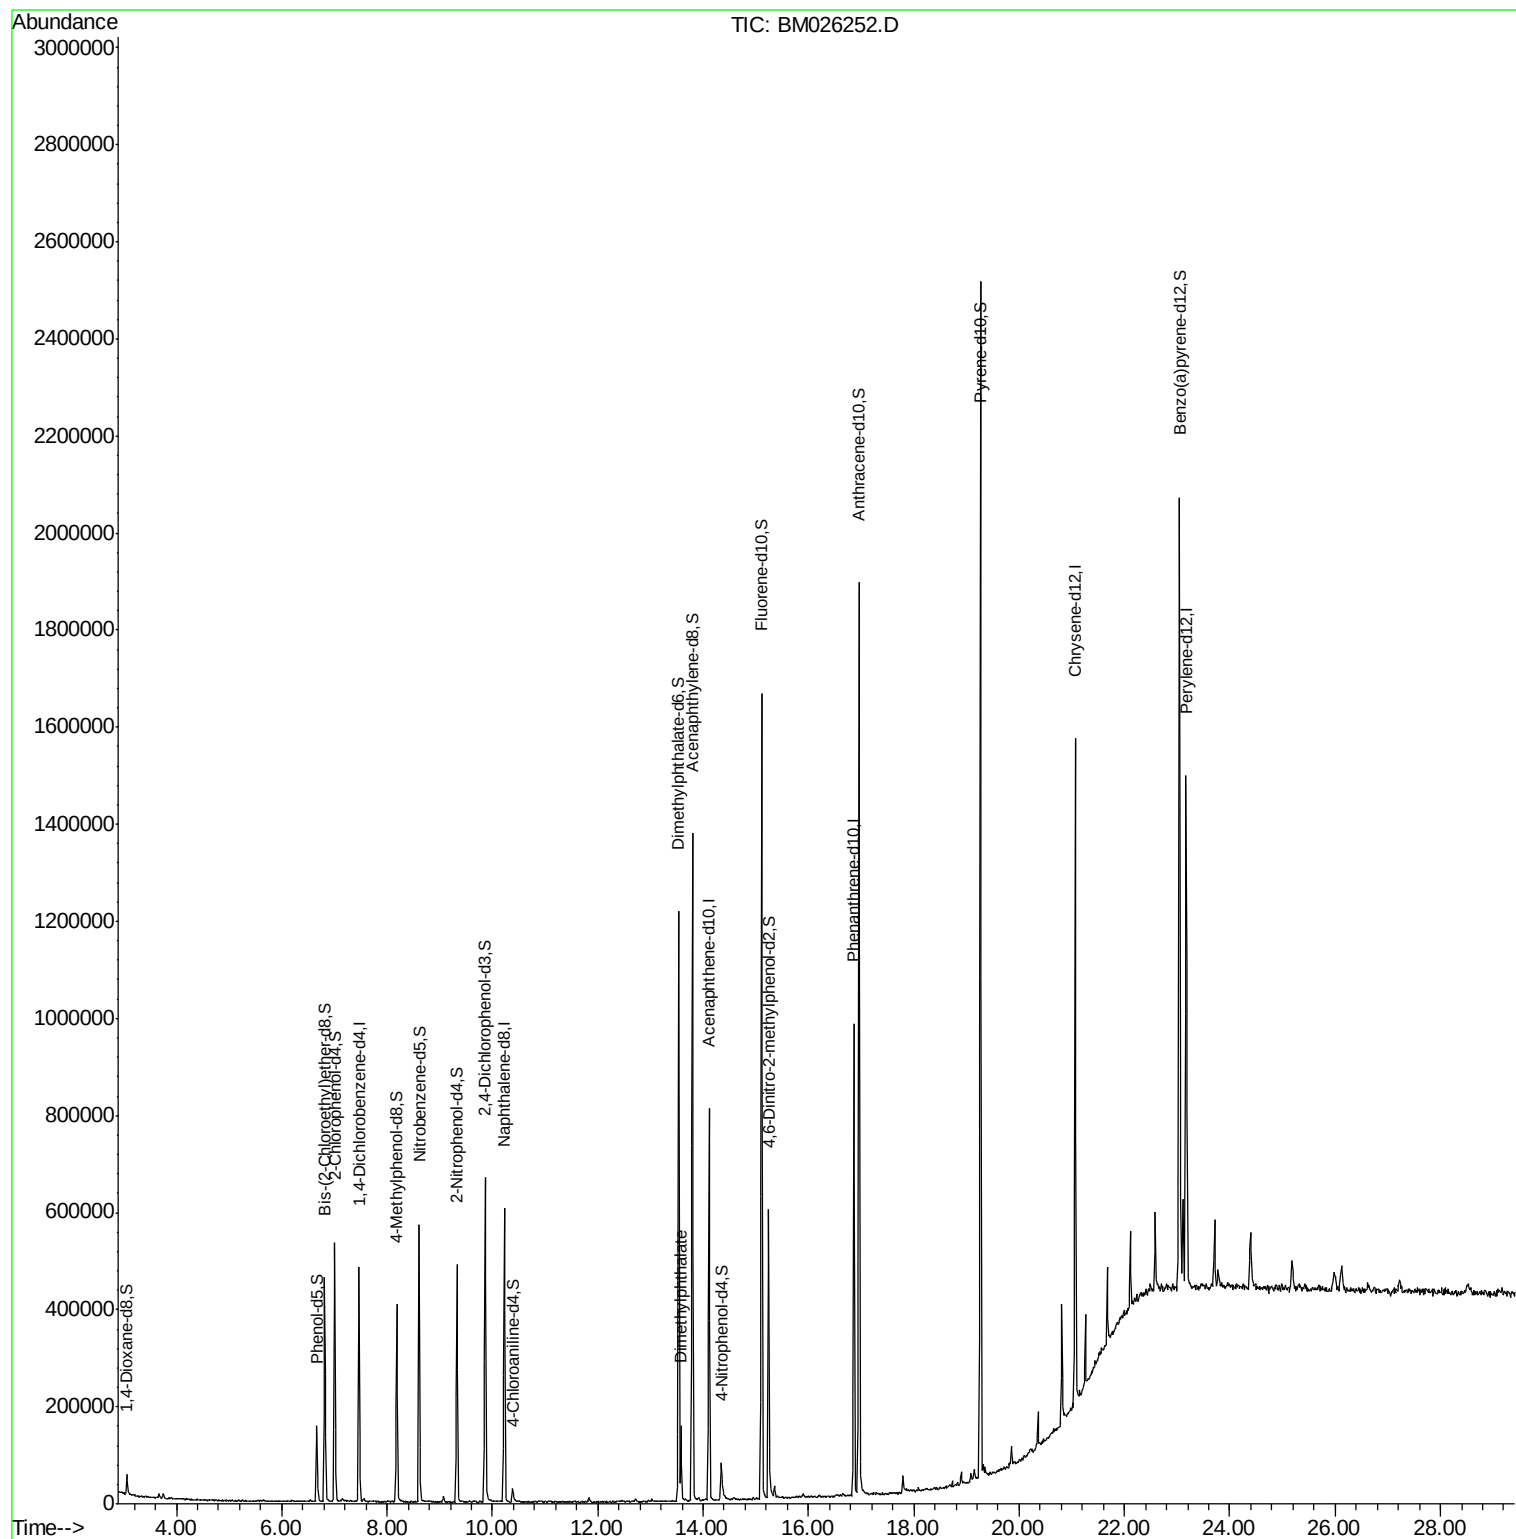

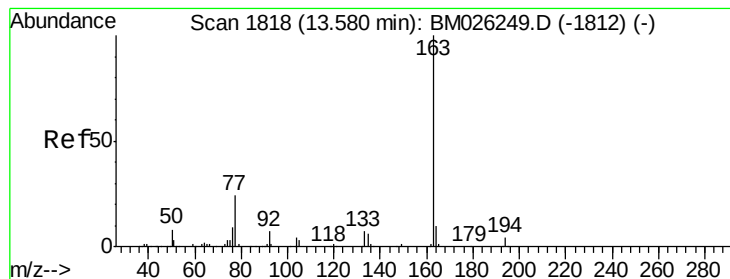

#45

Dimethylphthalate

Concen: 3.837 ng/ul

RT: 13.58 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BM026252.D

Acq: 04 Jun 2020 11:13

Instrument :

BNA_M

ClientSampleId :

C0AF3


Tot Ion:163 Resp: 79698

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 9.8 8.0 12.0

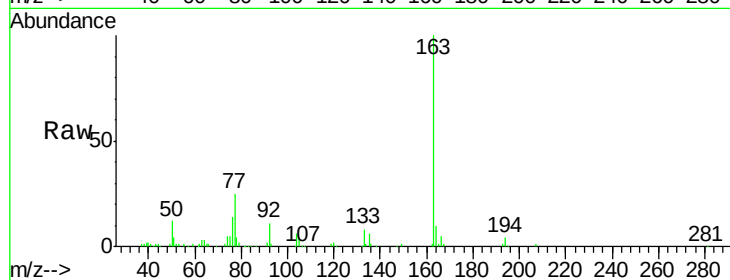

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

