

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060420\
 Data File : BM026253.D
 Acq On : 04 Jun 2020 11:49
 Operator : JU/CG
 Sample : L2844-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE6

Quant Time: Jun 04 12:32:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 04 10:01:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	115746	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	464409	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	268863	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	581118	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	625570	20.00	ng/ul	0.00
86) Perylene-d12	23.17	264	661643	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	20402	5.32	ng/uL	0.00
5) Phenol-d5	6.66	99	78794	7.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	237195	32.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	216843	26.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.18	113	138249	17.47	ng/ul	0.00
19) Nitrobenzene-d5	8.61	128	128840	34.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	135598	36.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	222007	29.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	15259	2.00	ng/ul	0.02
44) Dimethylphthalate-d6	13.53	166	748773	34.73	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	875525	34.28	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	20865	5.46	ng/ul	0.00
58) Fluorene-d10	15.11	176	661045	35.25	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.24	200	106288	31.37	ng/ul	0.00
71) Anthracene-d10	16.96	188	1055888	36.87	ng/ul	0.00
79) Pyrene-d10	19.26	212	1202519	37.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	1209721	34.35	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.58	163	96691	4.271	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060420\
Data File : BM026253.D
Acq On : 04 Jun 2020 11:49
Operator : JU/CG
Sample : L2844-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE6

Quant Time: Jun 04 12:32:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 04 10:01:49 2020
Response via : Initial Calibration

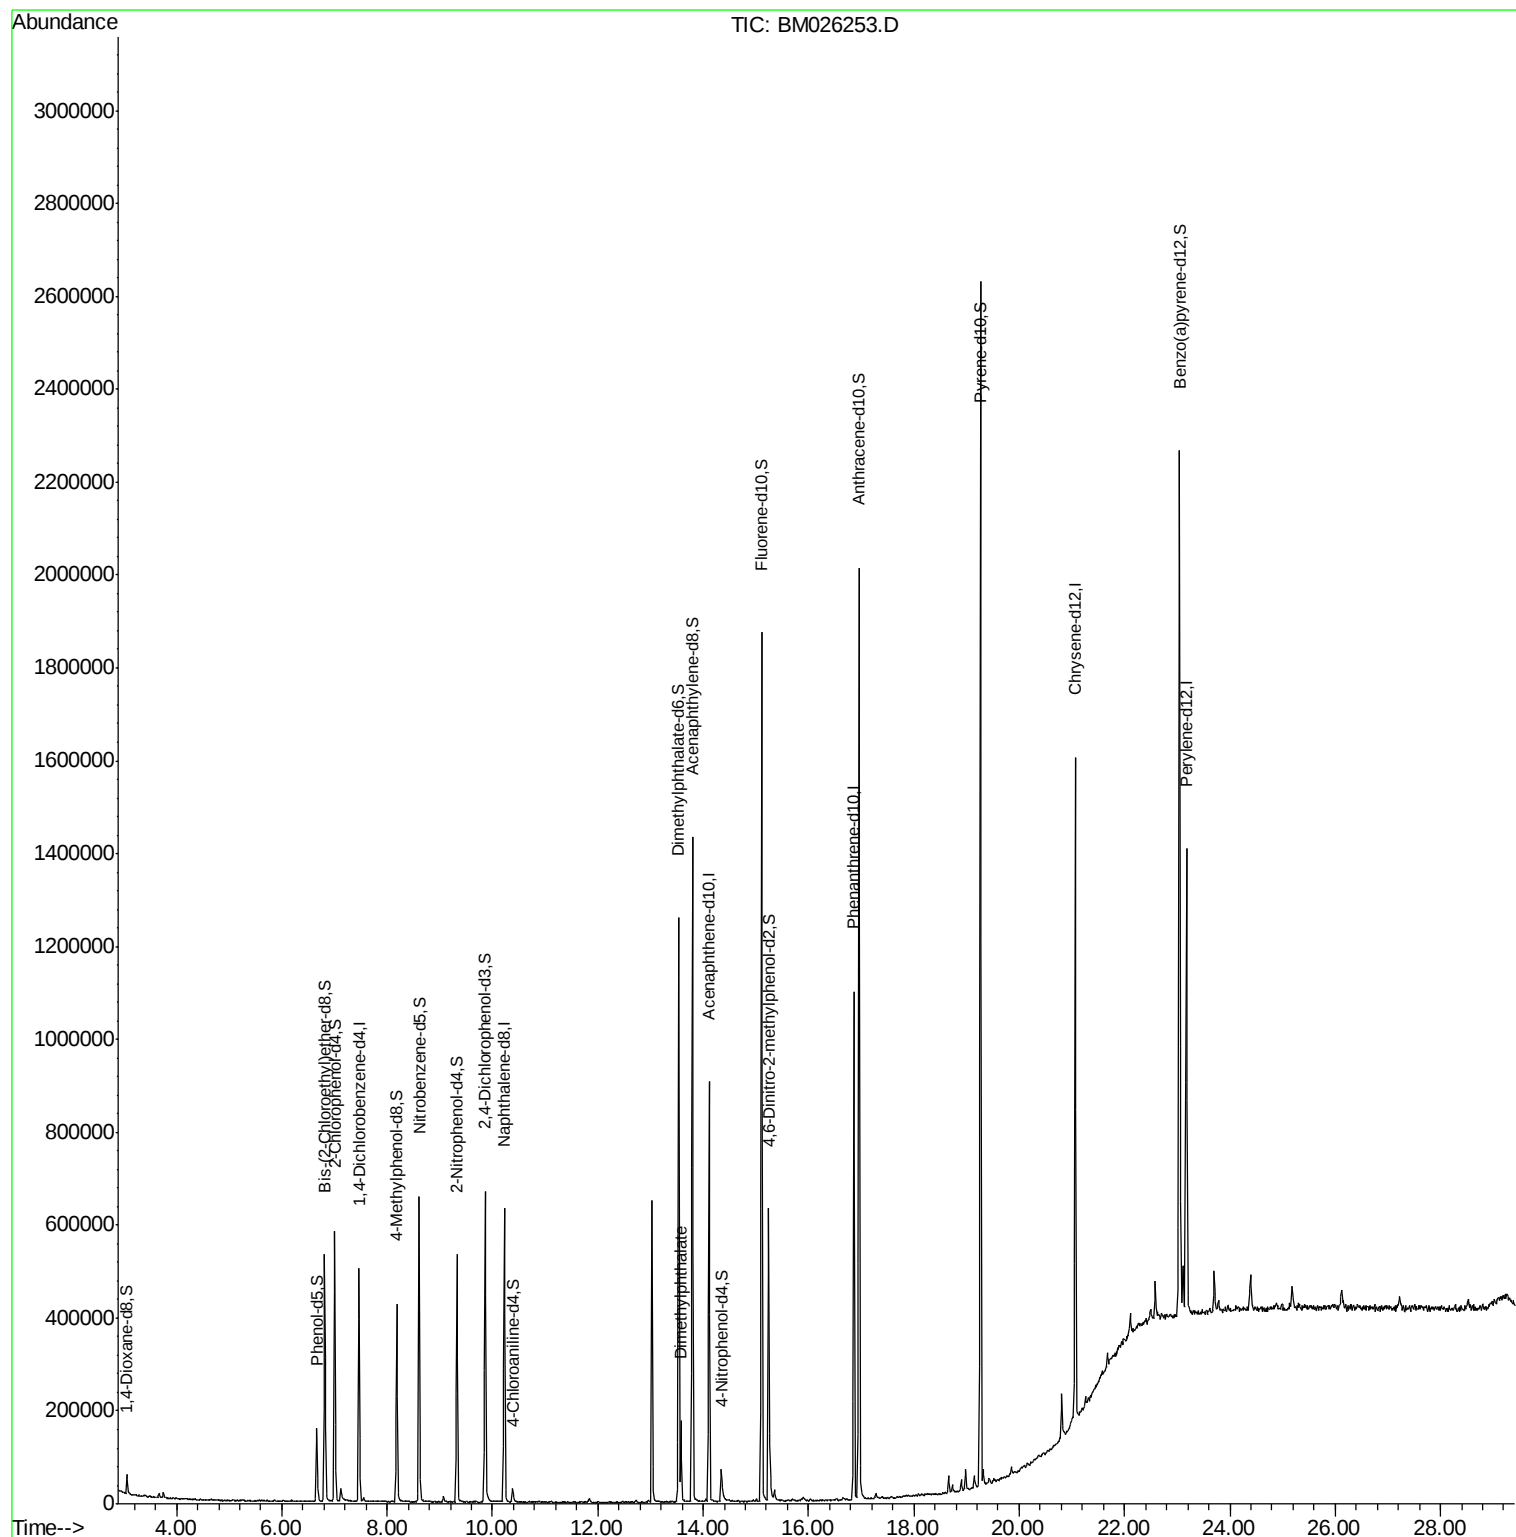

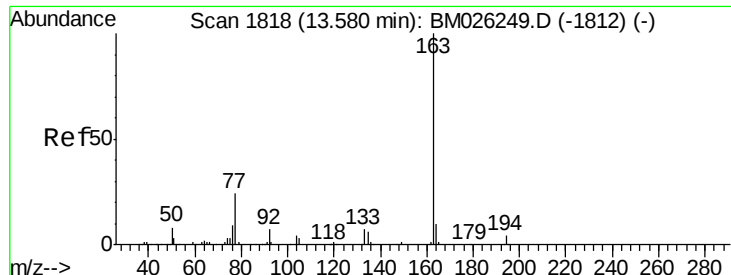

#45

Dimethylphthalate

Concen: 4.271 ng/ul

RT: 13.58 min Scan# 1818

Delta R.T. -0.00 min

Lab File: BM026253.D

Acq: 04 Jun 2020 11:49

Instrument :

BNA_M

ClientSampleId :

C0AE6


Tot Ion:163 Resp: 96691

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.0 8.0 12.0

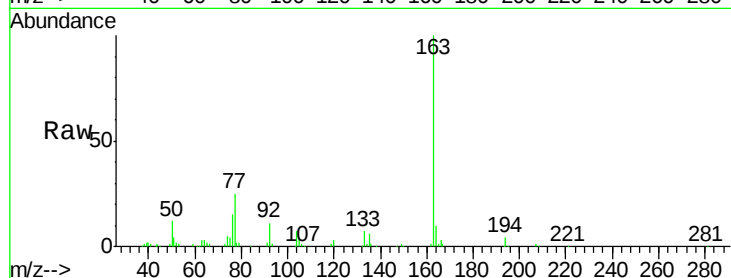

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

