

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060420\
 Data File : BM026263.D
 Acq On : 04 Jun 2020 18:35
 Operator : JU/CG
 Sample : L2844-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE8

Quant Time: Jun 04 19:06:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 04 10:01:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	104019	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	415180	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	243194	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	518471	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	571828	20.00	ng/ul	0.00
86) Perylene-d12	23.17	264	634025	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.05	96	20321	5.89	ng/uL	0.00
5) Phenol-d5	6.66	99	81920	8.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	214529	32.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	204414	27.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.18	113	137212	19.29	ng/ul	0.00
19) Nitrobenzene-d5	8.61	128	114634	33.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	120902	36.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	202370	30.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.38	131	21161	3.10	ng/ul	0.01
44) Dimethylphthalate-d6	13.53	166	696988	35.74	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	811883	35.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	20902	6.05	ng/ul	0.00
58) Fluorene-d10	15.11	176	623399	36.75	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.24	200	104600	34.60	ng/ul	0.00
71) Anthracene-d10	16.96	188	1040496	40.73	ng/ul	0.00
79) Pyrene-d10	19.26	212	1199742	40.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	1121333	33.23	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.58	163	120520	5.886	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM060420\
Data File : BM026263.D
Acq On : 04 Jun 2020 18:35
Operator : JU/CG
Sample : L2844-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE8

Quant Time: Jun 04 19:06:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 04 10:01:49 2020
Response via : Initial Calibration

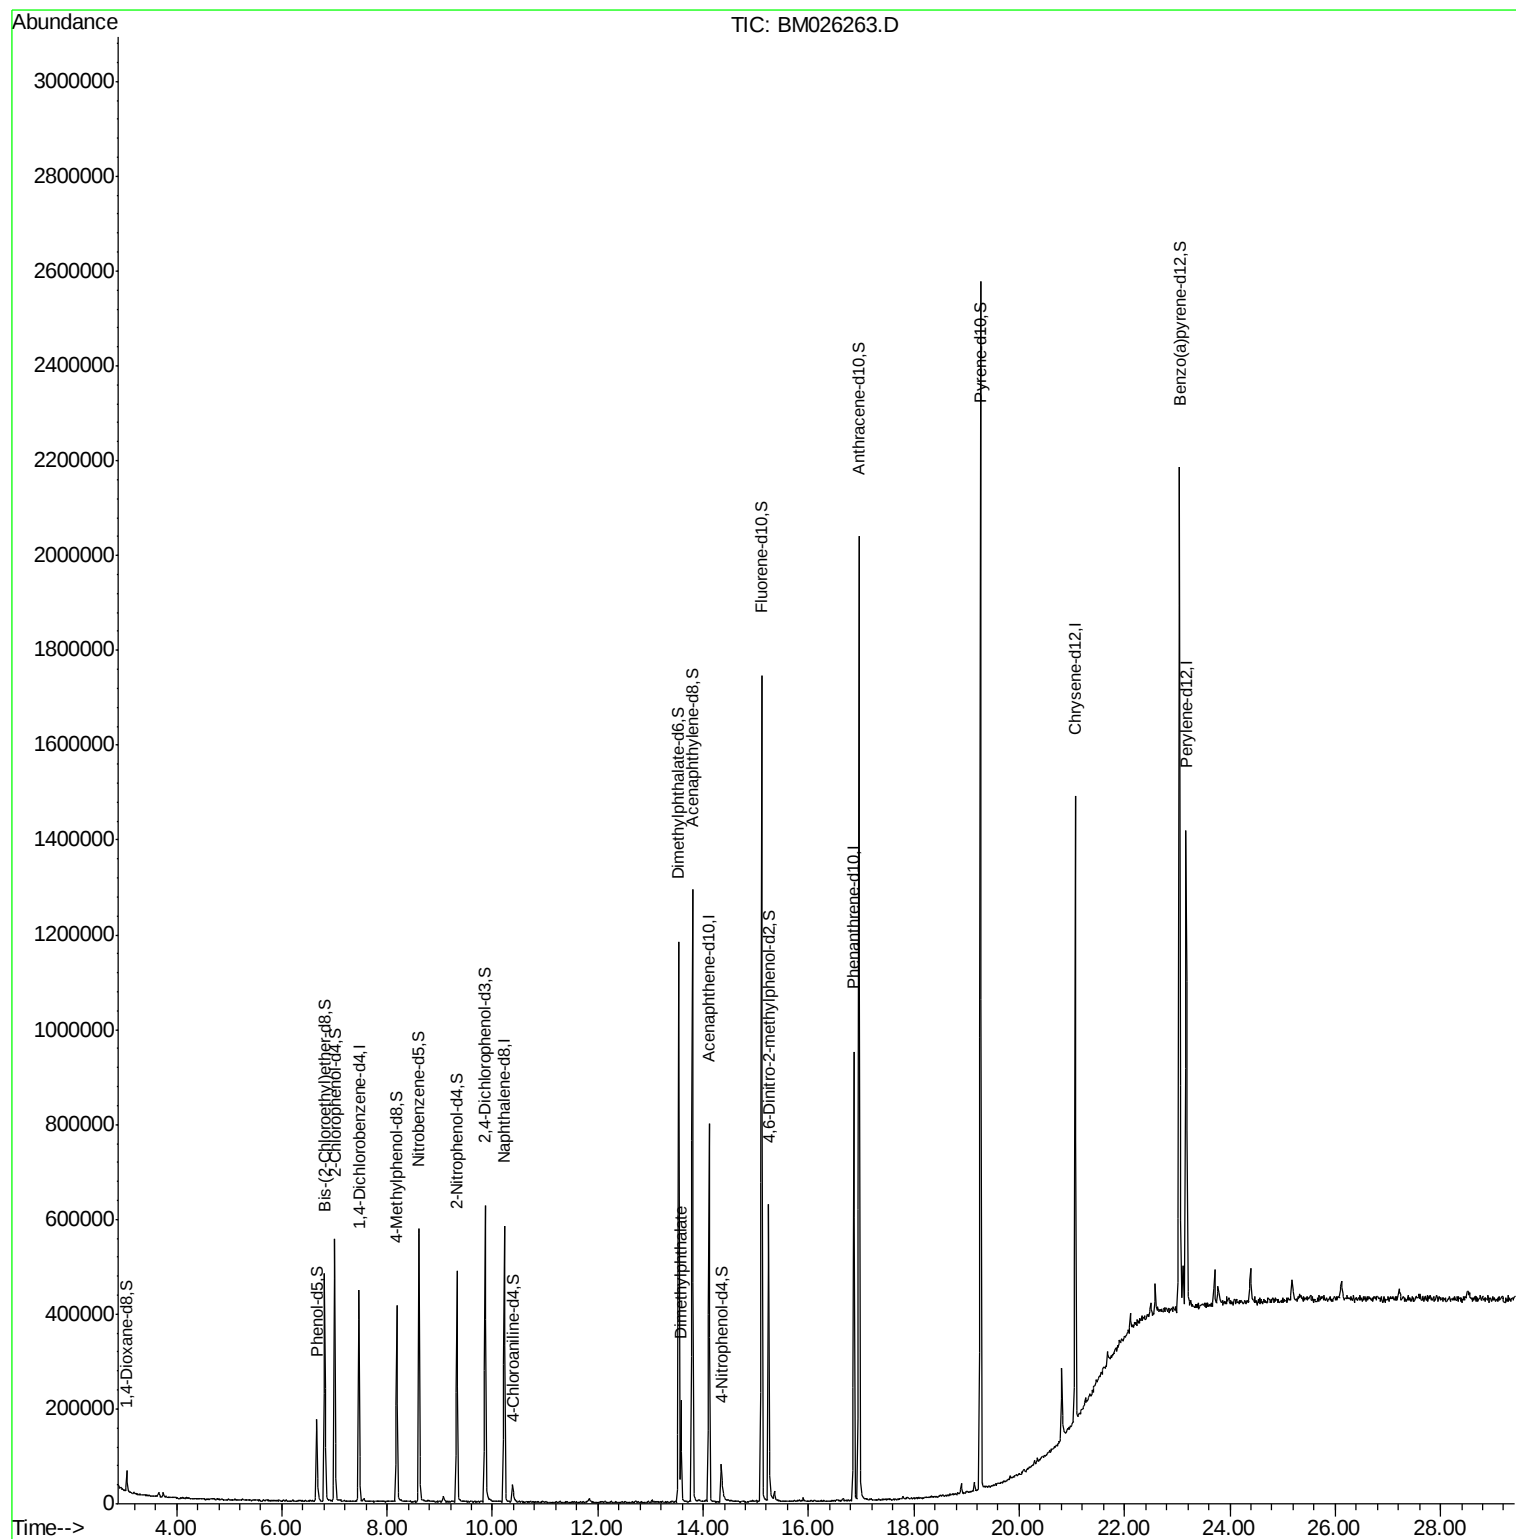

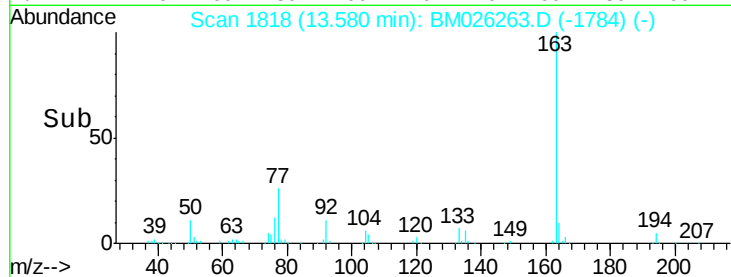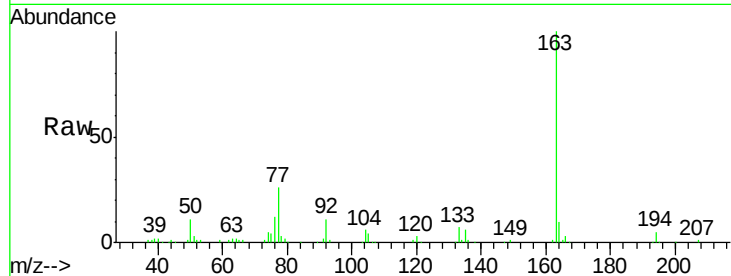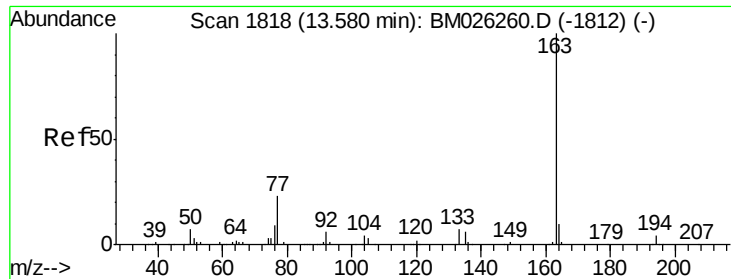

#45

Dimethylphthalate

Concen: 5.886 ng/ul

RT: 13.58 min Scan# 1818

Delta R.T. 0.00 min

Lab File: BM026263.D

Acq: 04 Jun 2020 18:35

Instrument :

BNA_M

ClientSampleId :

C0AE8

Tot Ion:163 Resp: 120520

Ion Ratio Lower Upper

163 100

194 4.6 3.2 4.8

164 9.6 8.0 12.0

